

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG091319\
Data File : FG005938.D
Signal(s) : FID1A.ch
Acq On : 14 Sep 2019 00:01
Operator : DD\AJ
Sample : K4663-04 5X
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
OK-01-091119

Integration File: autoint1.e
Quant Time: Sep 14 04:12:36 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG090719.M
Quant Title :
QLast Update : Mon Sep 09 05:03:58 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.726	273307	2.433 ug/ml

Target Compounds

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG091319\
Data File : FG005938.D
Signal(s) : FID1A.ch
Acq On : 14 Sep 2019 00:01
Operator : DD\AJ
Sample : K4663-04 5X
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
OK-01-091119

Integration File: autoint1.e
Quant Time: Sep 14 04:12:36 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG090719.M
Quant Title :
QLast Update : Mon Sep 09 05:03:58 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

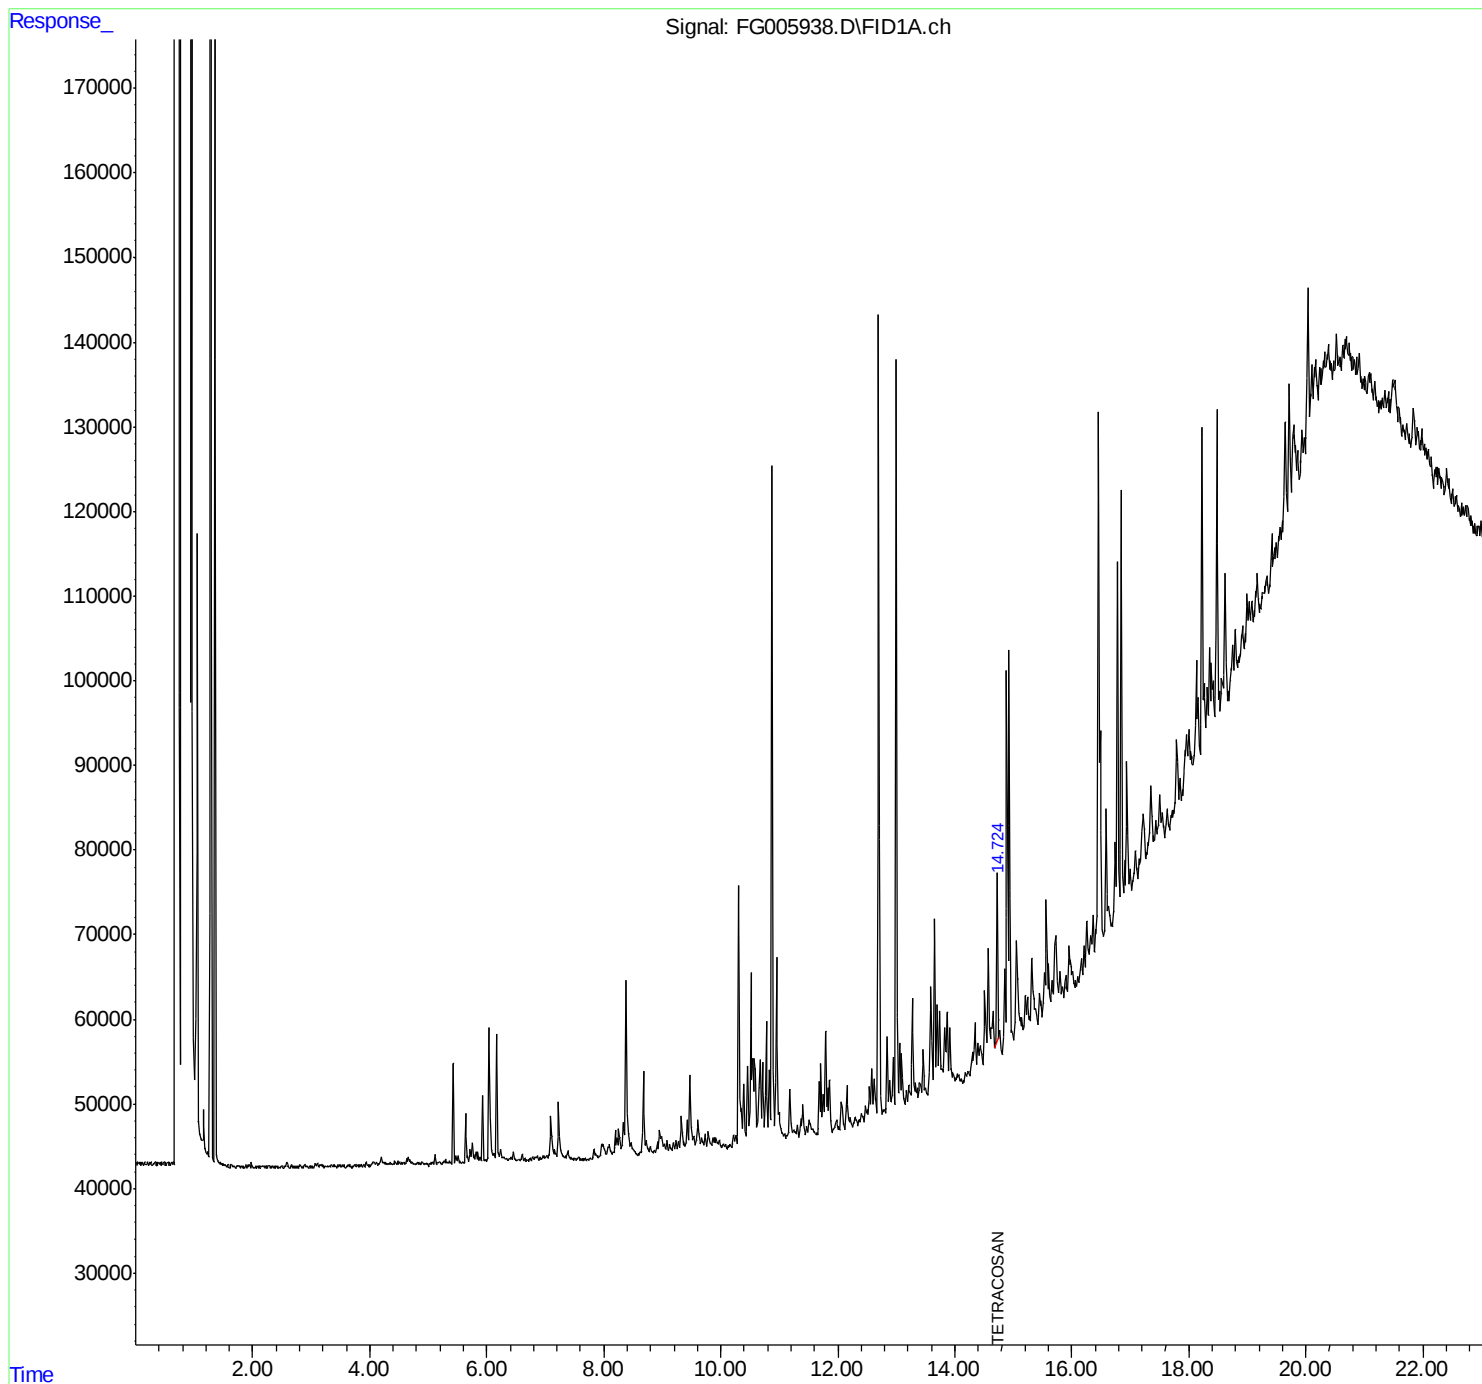

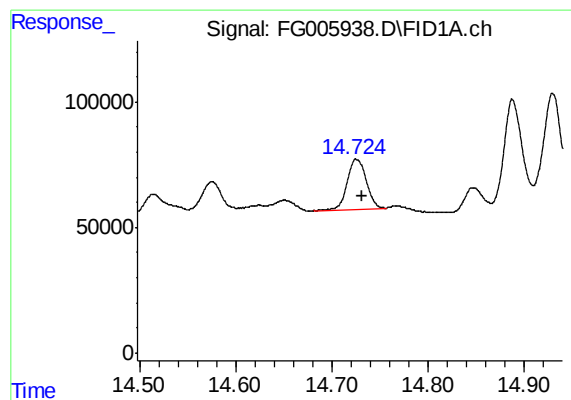

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.726 min
Delta R.T.: -0.005 min
Response: 273307
Conc: 2.43 ug/ml

Instrument :
FID_G
ClientSampleId :
OK-01-091119