

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_G\Data\FG091422\  
Data File : FG010555.D  
Signal(s) : FID1A.ch  
Acq On : 14 Sep 2022 11:47  
Operator : YP\AJ  
Sample : MECL2  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
FID\_G  
ClientSampleId :

Integration File: autoint1.e  
Quant Time: Sep 15 05:31:36 2022  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_G\Method\FG082622.M  
Quant Title :  
QLast Update : Fri Aug 26 23:48:05 2022  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

| Compound                    | R.T.   | Response | Conc Units  |
|-----------------------------|--------|----------|-------------|
| -----                       |        |          |             |
| System Monitoring Compounds |        |          |             |
| Target Compounds            |        |          |             |
| 13) N-TRIACONTANE           | 17.849 | 30579    | 0.236 ug/ml |
| 14) N-DOTRIACONTANE         | 18.682 | 23474    | 0.184 ug/ml |
| 15) N-TETRATRIACONTANE      | 19.466 | 107147   | 0.866 ug/ml |
| 16) N-HEXATRIACONTANE       | 20.205 | 27099    | 0.233 ug/ml |
| 18) N-TETRACONTANE          | 21.744 | 49934    | 0.424 ug/ml |
| -----                       |        |          |             |

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_G\Data\FG091422\  
Data File : FG010555.D  
Signal(s) : FID1A.ch  
Acq On : 14 Sep 2022 11:47  
Operator : YP\AJ  
Sample : MECL2  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
FID\_G  
ClientSampleId :

Integration File: autoint1.e  
Quant Time: Sep 15 05:31:36 2022  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_G\Method\FG082622.M  
Quant Title :  
QLast Update : Fri Aug 26 23:48:05 2022  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

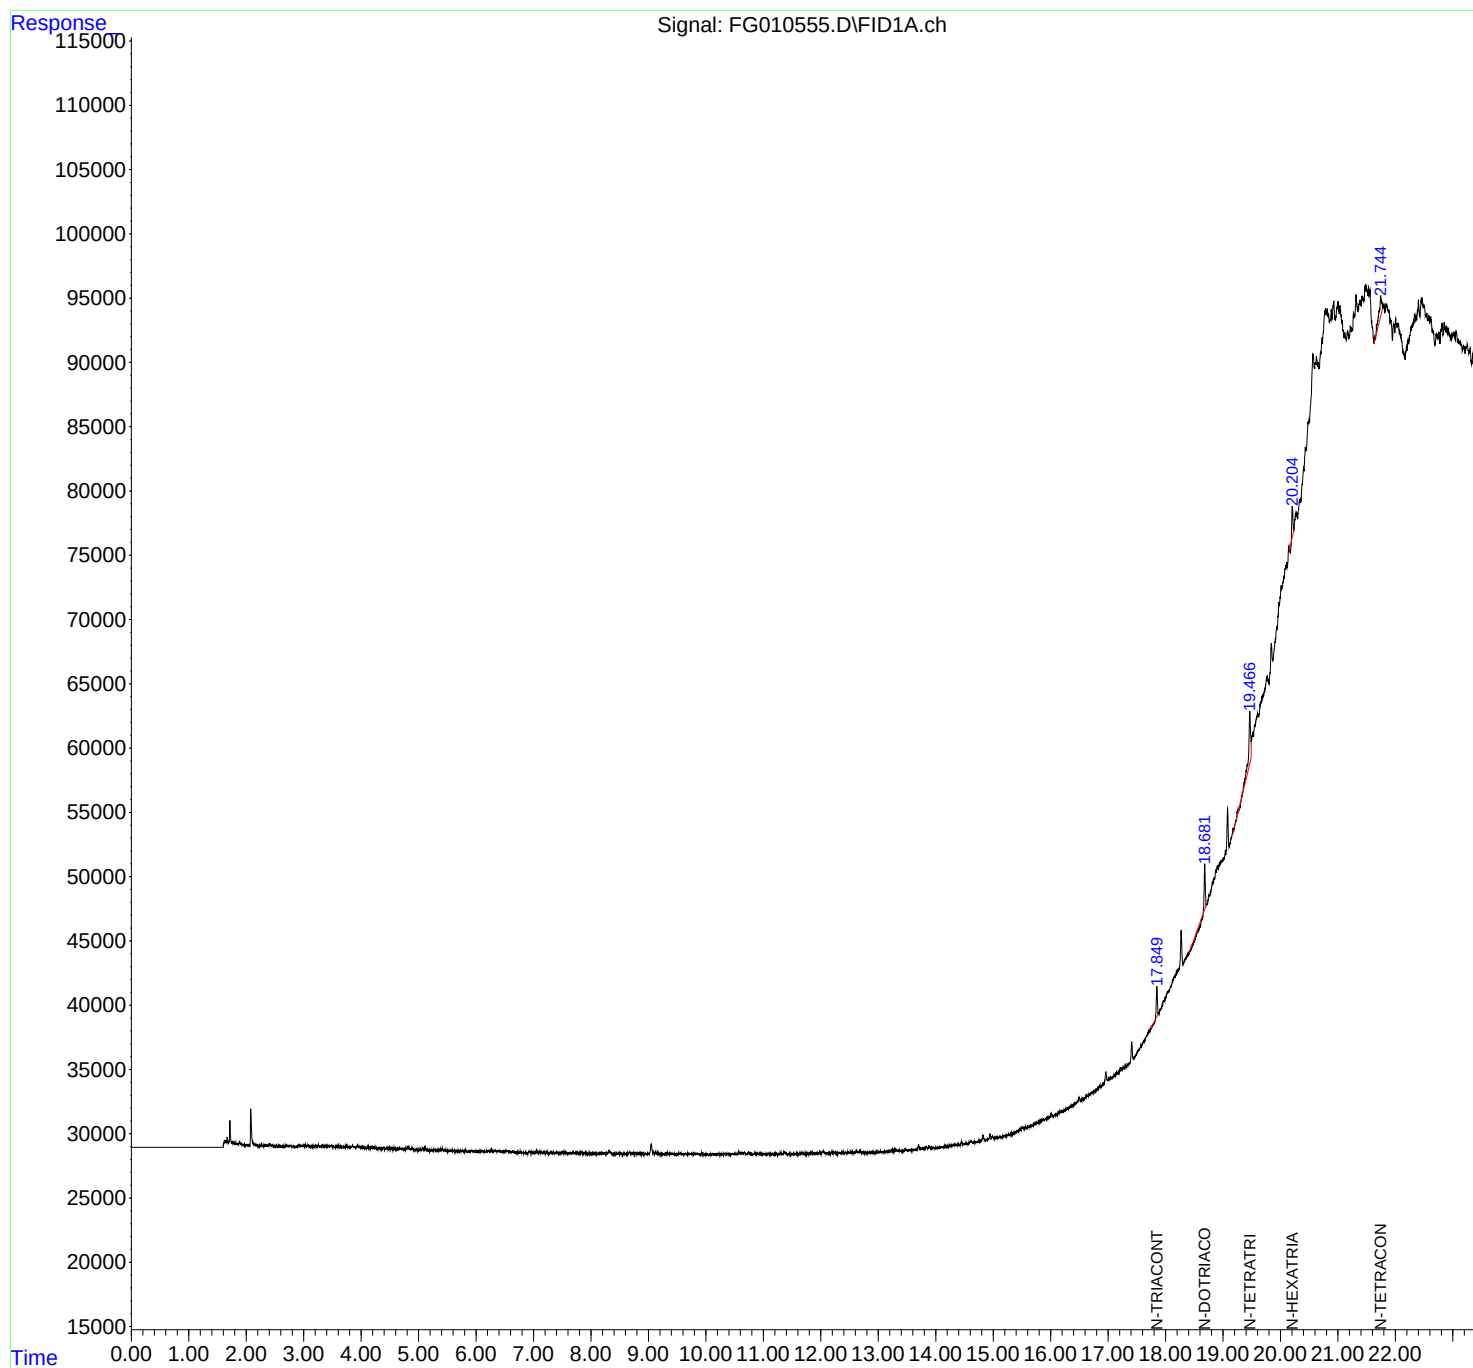


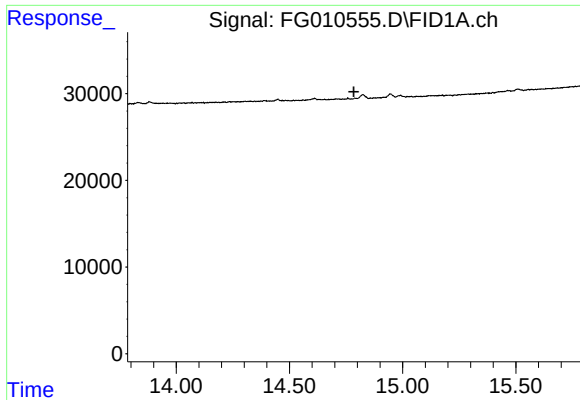

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 0.000 min  
Exp R.T.: 14.785 min  
Response: 0  
Conc: N.D.

Instrument :  
FID\_G  
ClientSampleId :

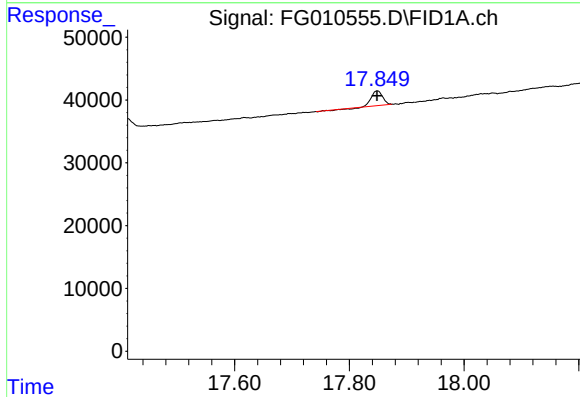


#13 N-TRIACONTANE

R.T.: 17.849 min  
Delta R.T.: 0.000 min  
Response: 30579  
Conc: 0.24 ug/ml

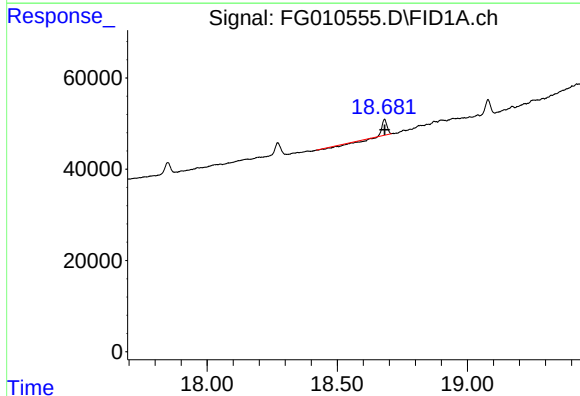


#14 N-DOTRIACONTANE

R.T.: 18.682 min  
Delta R.T.: 0.000 min  
Response: 23474  
Conc: 0.18 ug/ml

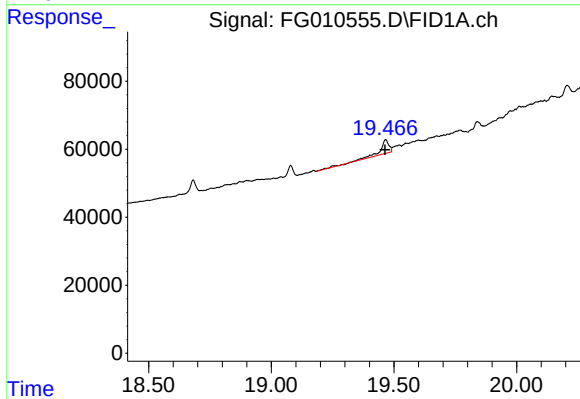

#15 N-TETRATRIACONTANE


R.T.: 19.466 min  
Delta R.T.: 0.003 min  
Response: 107147  
Conc: 0.87 ug/ml

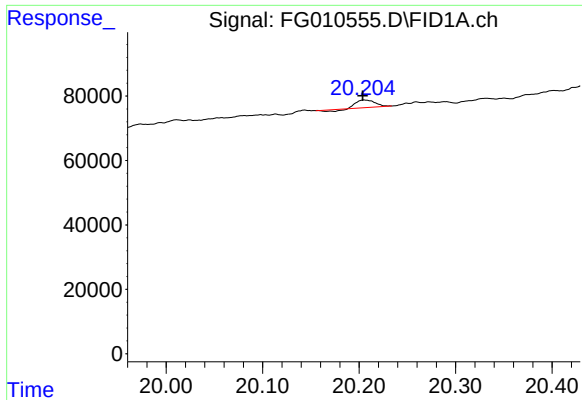

#16 N-HEXATRIACONTANE

R.T.: 20.205 min  
Delta R.T.: 0.002 min  
Response: 27099  
Conc: 0.23 ug/ml

Instrument :  
FID\_G  
ClientSampleId :

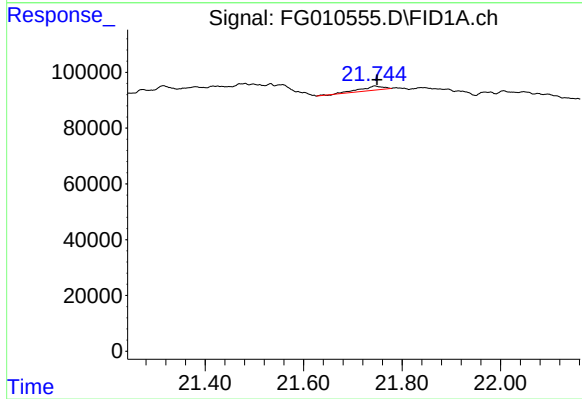

#18 N-TETRACONTANE

R.T.: 21.744 min  
Delta R.T.: -0.005 min  
Response: 49934  
Conc: 0.42 ug/ml