

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG091422\
Data File : FG010559.D
Signal(s) : FID1A.ch
Acq On : 14 Sep 2022 15:22
Operator : YP\AJ
Sample : PB147636BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Sep 15 05:32:26 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG082622.M
Quant Title :
QLast Update : Fri Aug 26 23:48:05 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.786	1857060	15.174 ug/ml
Target Compounds			
15) N-TETRATRIACONTANE	19.469	45867	0.371 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG091422\
Data File : FG010559.D
Signal(s) : FID1A.ch
Acq On : 14 Sep 2022 15:22
Operator : YP\AJ
Sample : PB147636BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Sep 15 05:32:26 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG082622.M
Quant Title :
QLast Update : Fri Aug 26 23:48:05 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

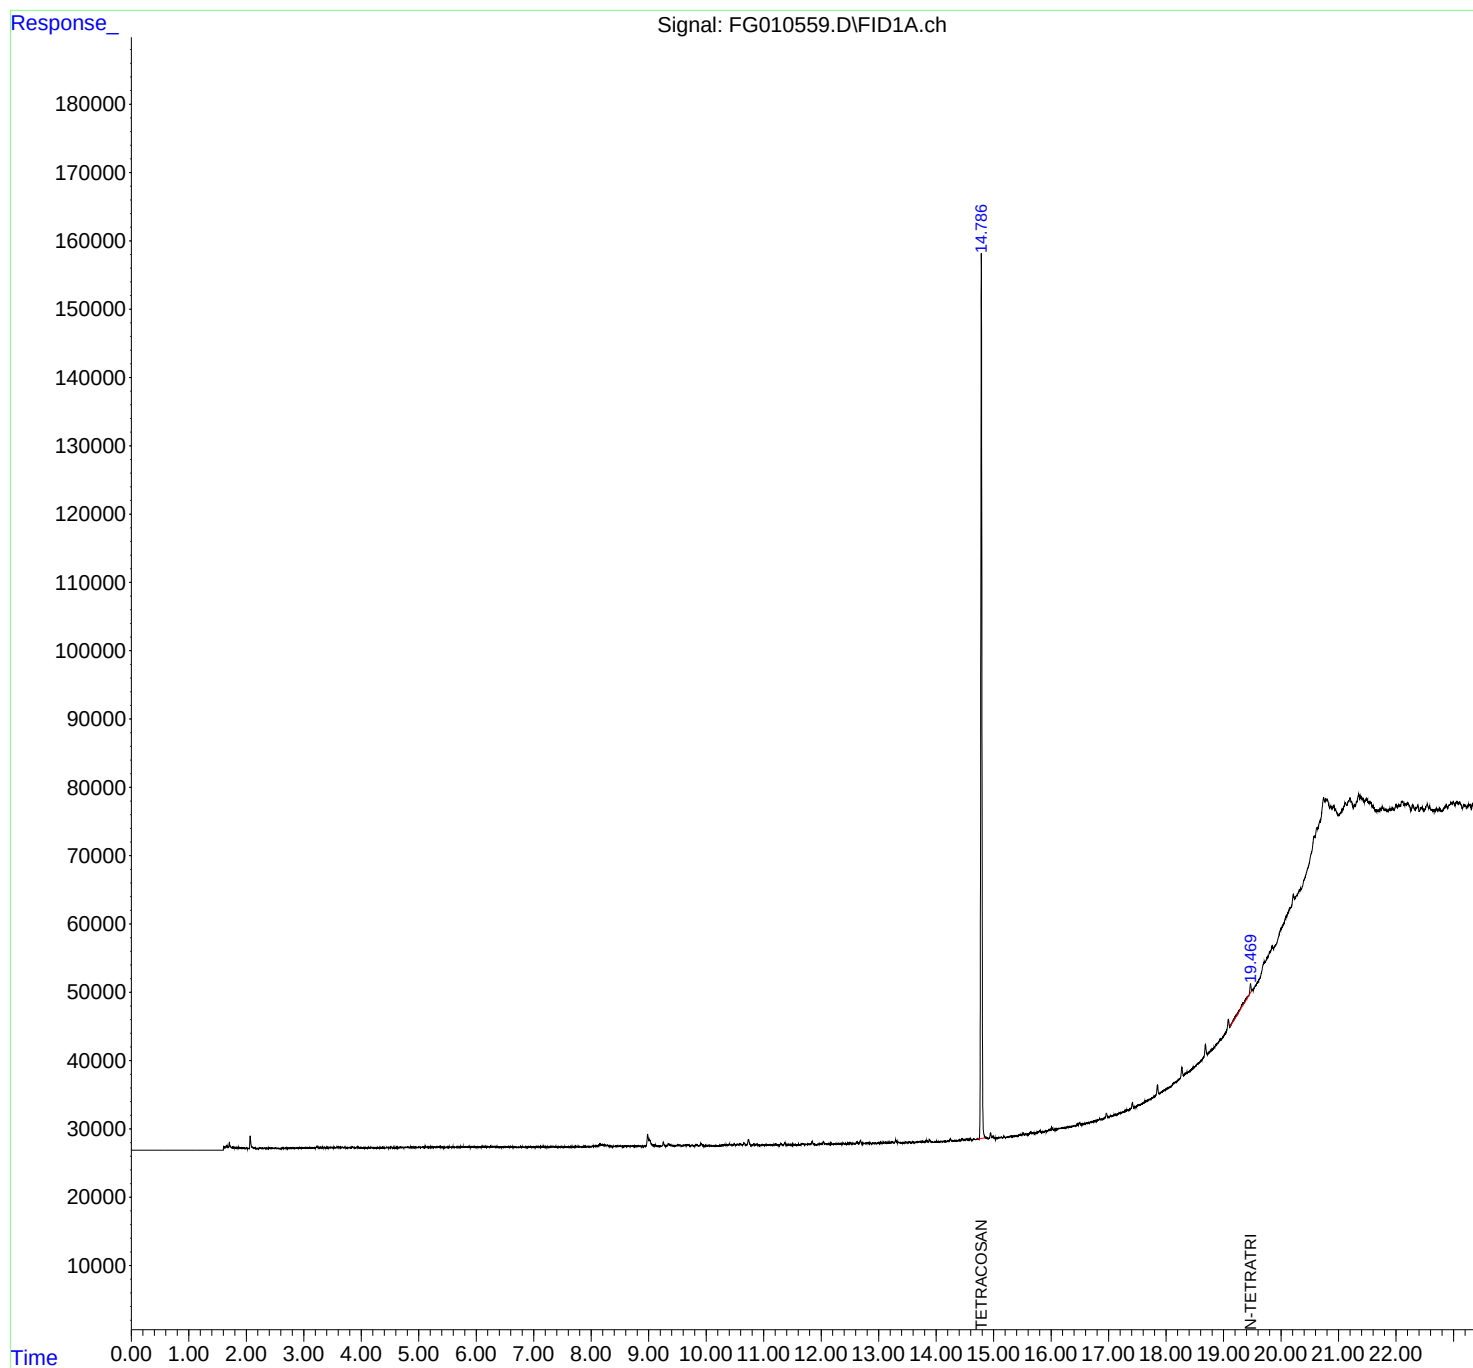


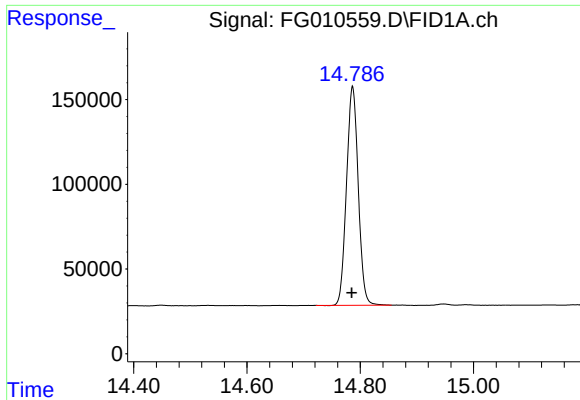

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.786 min
Delta R.T.: 0.002 min
Response: 1857060
Conc: 15.17 ug/ml

Instrument :
FID_G
ClientSampleId :

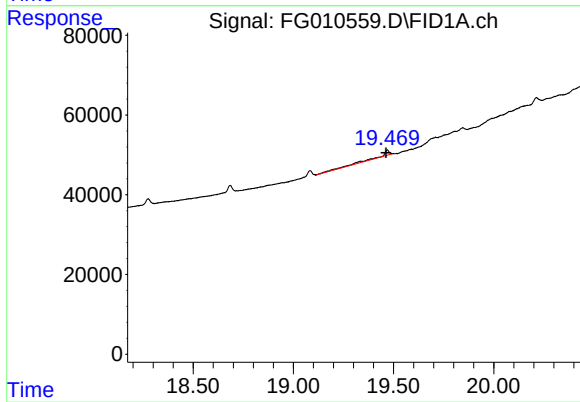

#15 N-TETRATRIACONTANE

R.T.: 19.469 min
Delta R.T.: 0.006 min
Response: 45867
Conc: 0.37 ug/ml