

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG091422\
 Data File : FG010566.D
 Signal(s) : FID1A.ch
 Acq On : 14 Sep 2022 19:49
 Operator : YP\AJ
 Sample : 50 PPM TRPH STD
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :
 50 PPM TRPH STD

Integration File: autoint1.e
 Quant Time: Sep 15 05:33:53 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG082622.M
 Quant Title :
 QLast Update : Fri Aug 26 23:48:05 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.794	5606956	45.814 ug/ml
Target Compounds			
2) N-DECANE	4.316	6830970	53.293 ug/ml
3) N-DODECANE	6.498	6933036	52.679 ug/ml
4) N-TETRADECANE	8.329	6935068	51.238 ug/ml
5) N-HEXADECANE	9.937	6989144	49.878 ug/ml
6) N-OCTADECANE	11.382	6933748	48.564 ug/ml
7) N-EICOSANE	12.693	6772163	47.430 ug/ml
8) N-DOCOSANE	13.893	6459289	46.352 ug/ml
10) N-TETRACOSANE	14.998	6289739	45.393 ug/ml
11) N-HEXACOSANE	16.020	6080193	44.819 ug/ml
12) N-OCTACOSANE	16.972	5995837	45.339 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG091422\
Data File : FG010566.D
Signal(s) : FID1A.ch
Acq On : 14 Sep 2022 19:49
Operator : YP\AJ
Sample : 50 PPM TRPH STD
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
50 PPM TRPH STD

Integration File: autoint1.e
Quant Time: Sep 15 05:33:53 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG082622.M
Quant Title :
QLast Update : Fri Aug 26 23:48:05 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

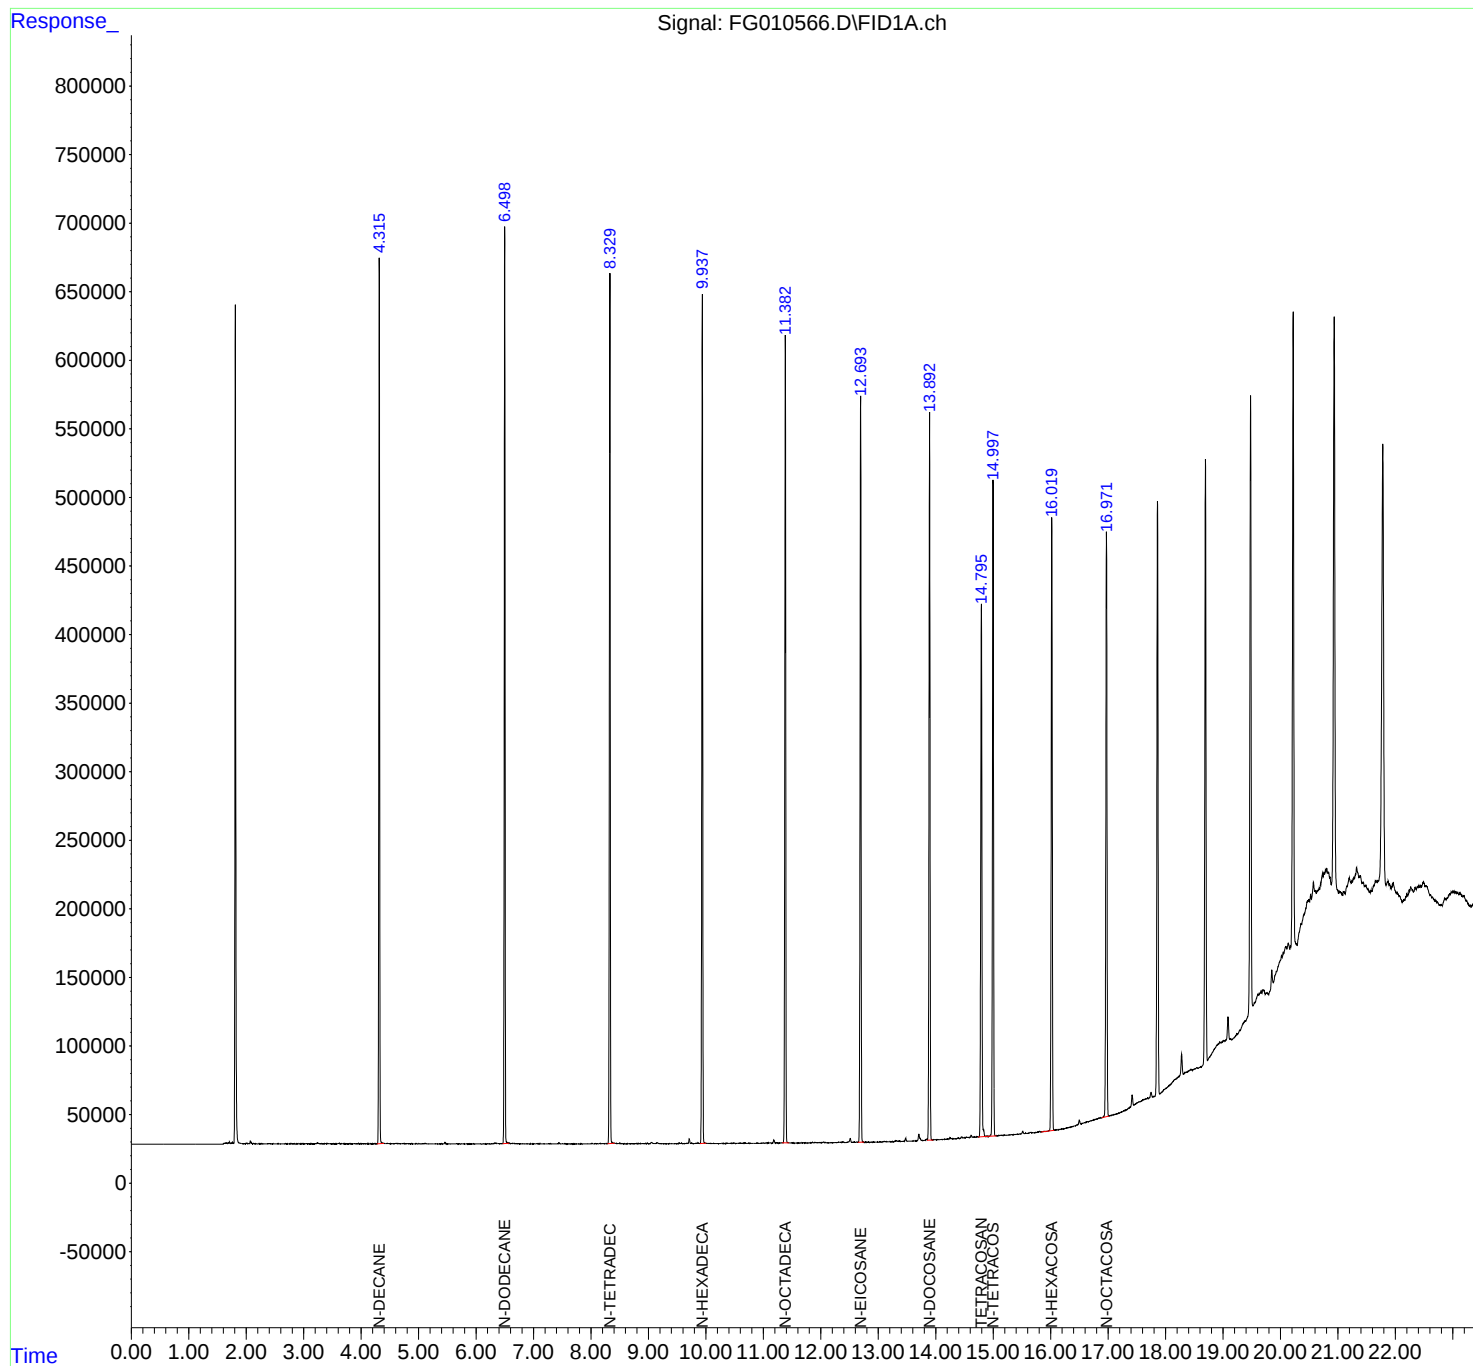


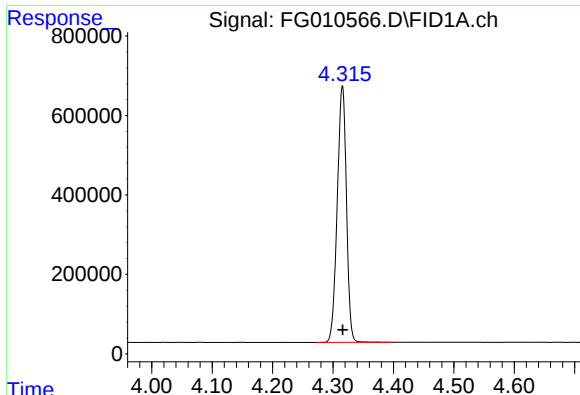

#2 N-DECANE


R.T.: 4.316 min
Delta R.T.: 0.000 min
Response: 6830970
Conc: 53.29 ug/ml

Instrument :
FID_G
ClientSampleId :
50 PPM TRPH STD

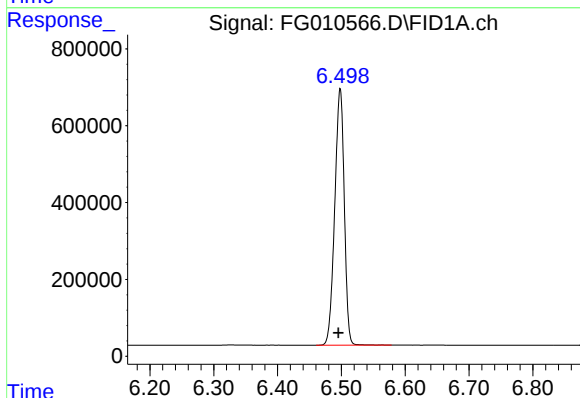


#3 N-DODECANE

R.T.: 6.498 min
Delta R.T.: 0.003 min
Response: 6933036
Conc: 52.68 ug/ml

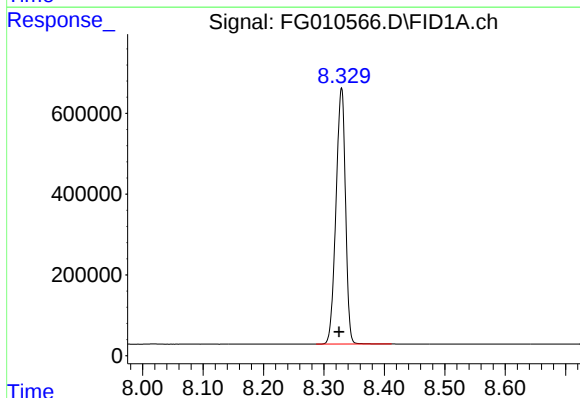


#4 N-TETRADECANE

R.T.: 8.329 min
Delta R.T.: 0.004 min
Response: 6935068
Conc: 51.24 ug/ml

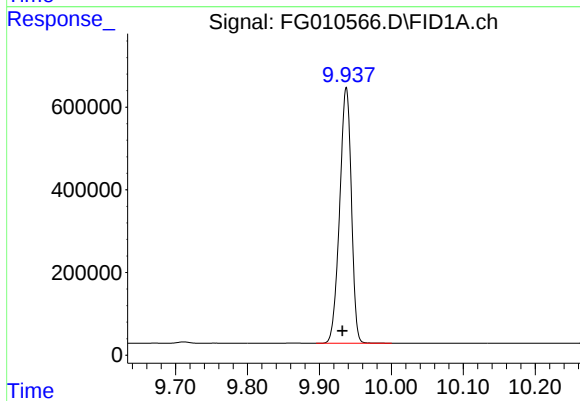

#5 N-HEXADECANE


R.T.: 9.937 min
Delta R.T.: 0.005 min
Response: 6989144
Conc: 49.88 ug/ml

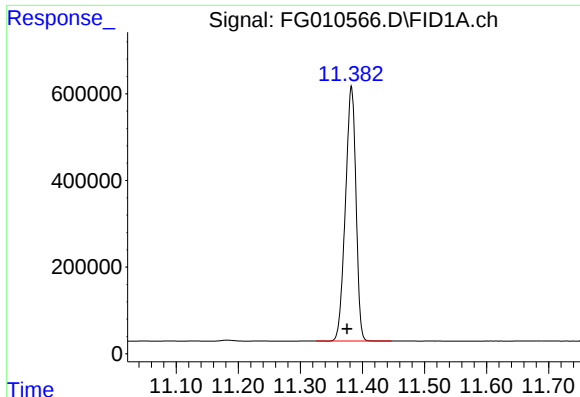

#6 N-OCTADECANE


R.T.: 11.382 min
Delta R.T.: 0.007 min
Response: 6933748
Conc: 48.56 ug/ml

Instrument :
FID_G
ClientSampleId :
50 PPM TRPH STD

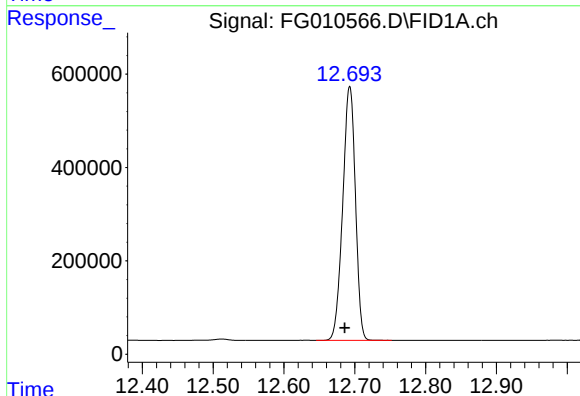


#7 N-EICOSANE

R.T.: 12.693 min
Delta R.T.: 0.007 min
Response: 6772163
Conc: 47.43 ug/ml

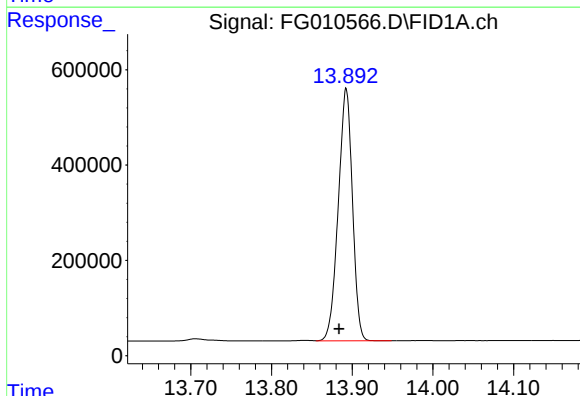


#8 N-DOCOSANE

R.T.: 13.893 min
Delta R.T.: 0.009 min
Response: 6459289
Conc: 46.35 ug/ml

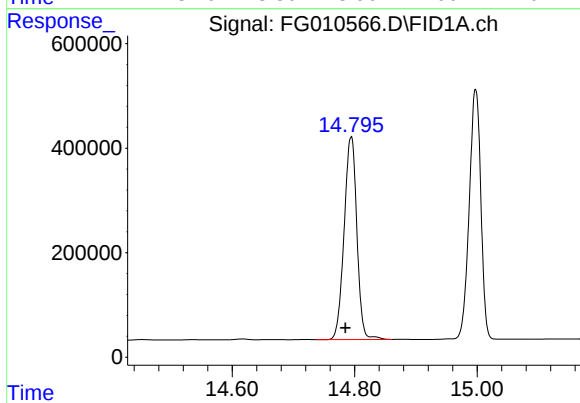

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.794 min
Delta R.T.: 0.010 min
Response: 5606956
Conc: 45.81 ug/ml

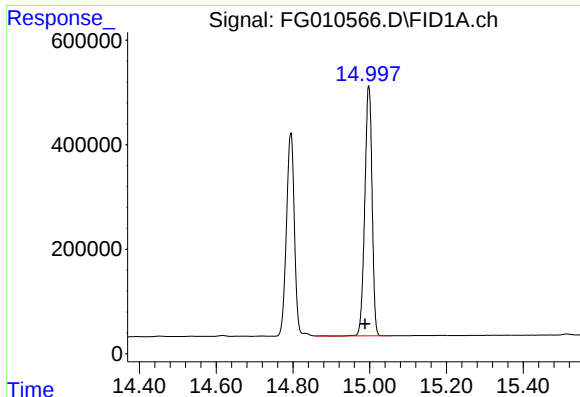

#10 N-TETRACOSANE


R.T.: 14.998 min
Delta R.T.: 0.009 min
Response: 6289739
Conc: 45.39 ug/ml

Instrument :
FID_G
ClientSampleId :
50 PPM TRPH STD

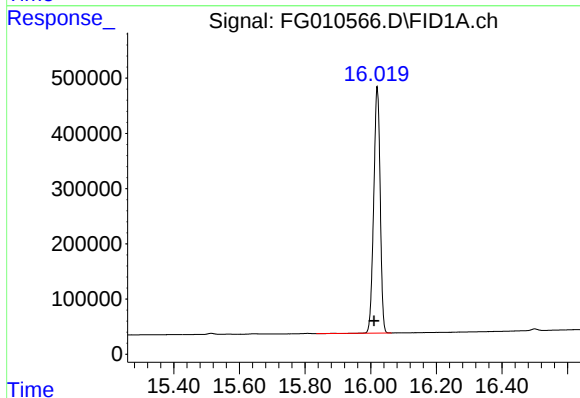

#11 N-HEXACOSANE

R.T.: 16.020 min
Delta R.T.: 0.009 min
Response: 6080193
Conc: 44.82 ug/ml

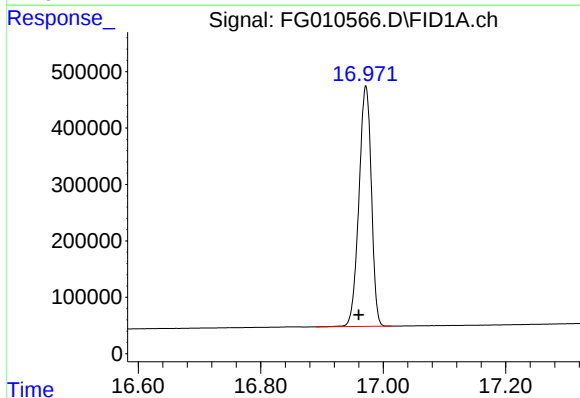

#12 N-OCTACOSANE

R.T.: 16.972 min
Delta R.T.: 0.011 min
Response: 5995837
Conc: 45.34 ug/ml