

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG091522\
 Data File : FG010575.D
 Signal(s) : FID1A.ch
 Acq On : 15 Sep 2022 14:19
 Operator : YP\AJ
 Sample : PB147654BL
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Sep 16 04:16:18 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG082622.M
 Quant Title :
 QLast Update : Fri Aug 26 23:48:05 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.793	1476376	12.063 ug/ml
Target Compounds			
13) N-TRIACONTANE	17.860	97013	0.749 ug/ml
16) N-HEXATRIACONTANE	20.221	29644	0.255 ug/ml
18) N-TETRACONTANE	21.717	202367	1.716 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG091522\
Data File : FG010575.D
Signal(s) : FID1A.ch
Acq On : 15 Sep 2022 14:19
Operator : YP\AJ
Sample : PB147654BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Sep 16 04:16:18 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG082622.M
Quant Title :
QLast Update : Fri Aug 26 23:48:05 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

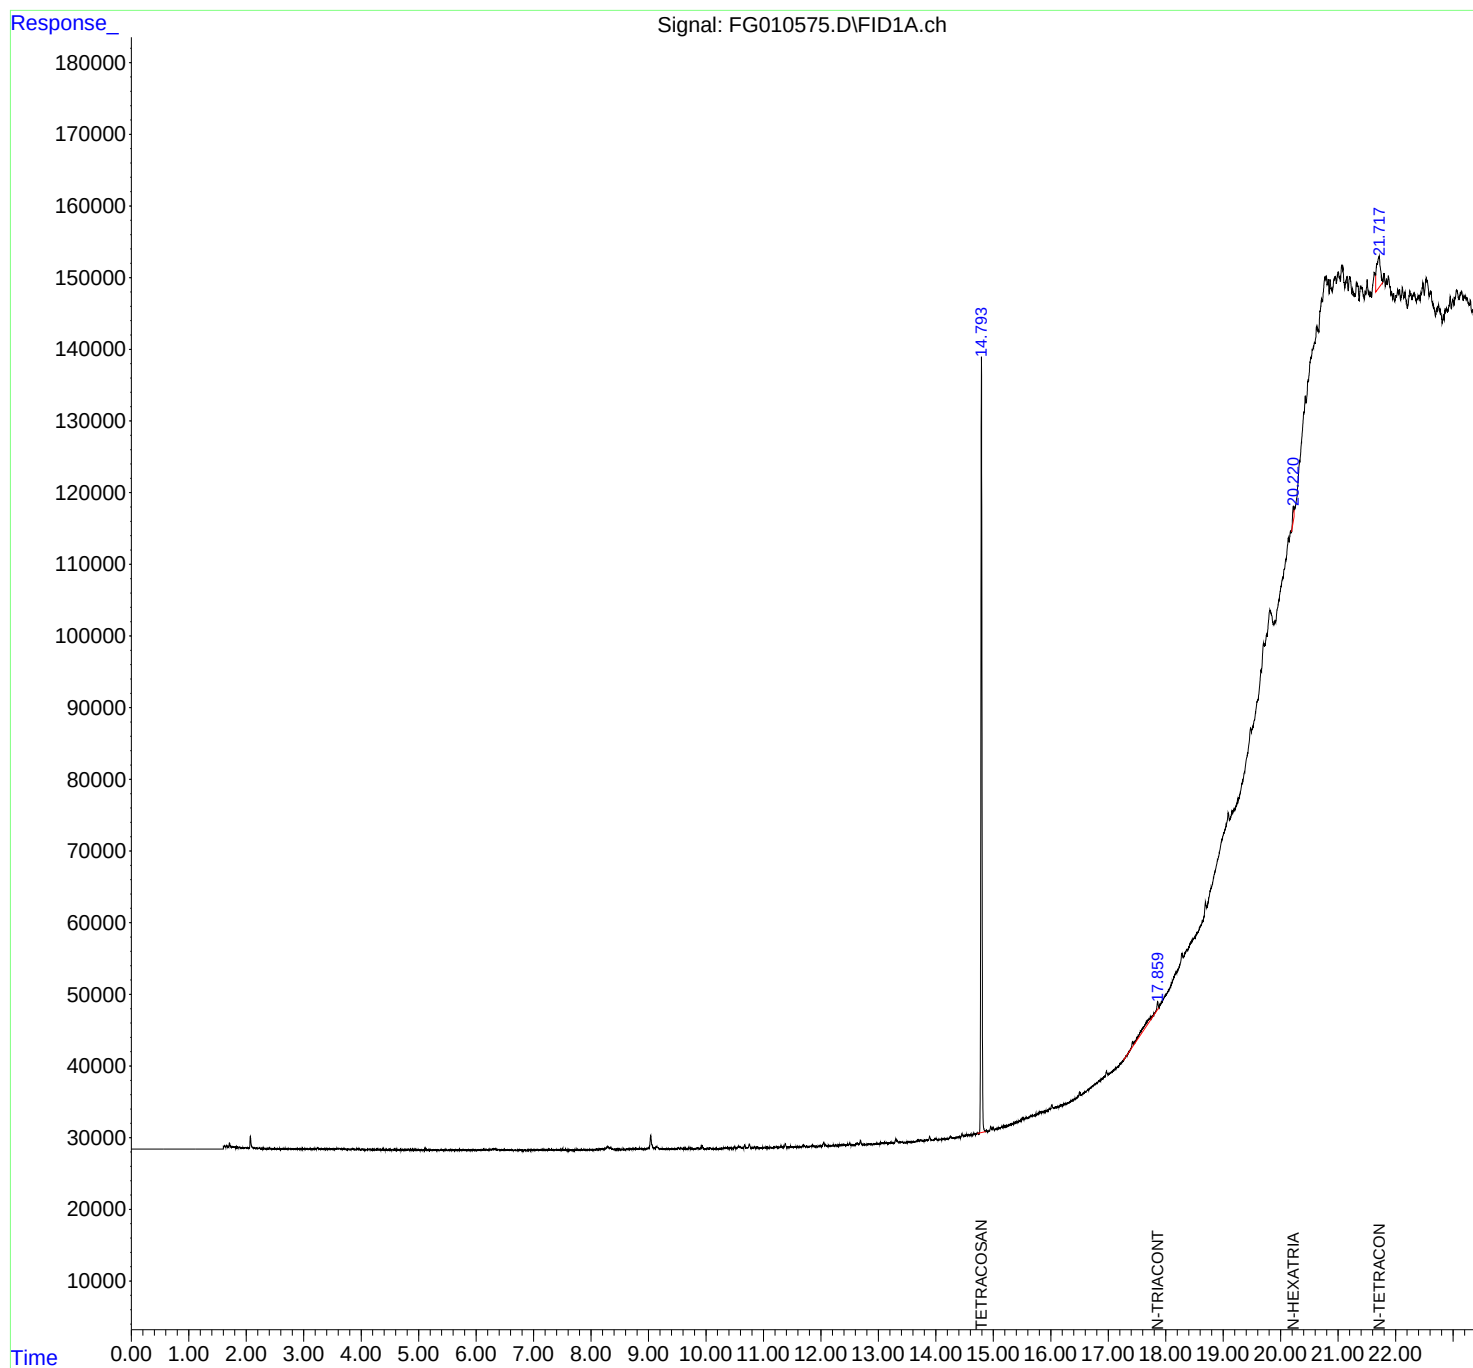


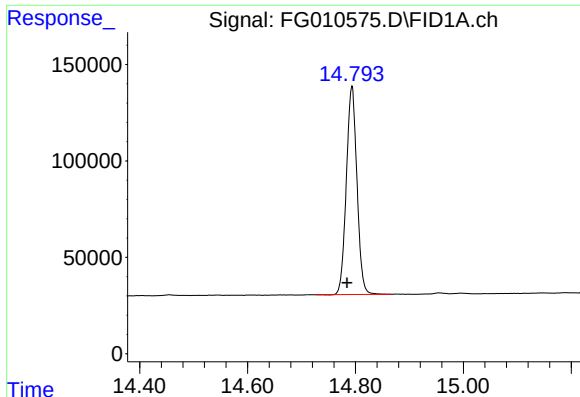

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.793 min
Delta R.T.: 0.009 min
Response: 1476376
Conc: 12.06 ug/ml

Instrument :
FID_G
ClientSampleId :

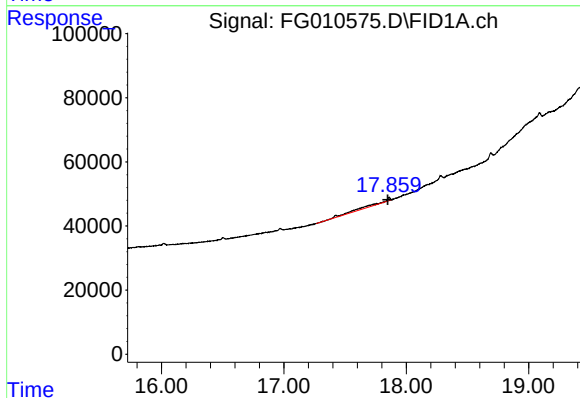


#13 N-TRIACONTANE

R.T.: 17.860 min
Delta R.T.: 0.012 min
Response: 97013
Conc: 0.75 ug/ml

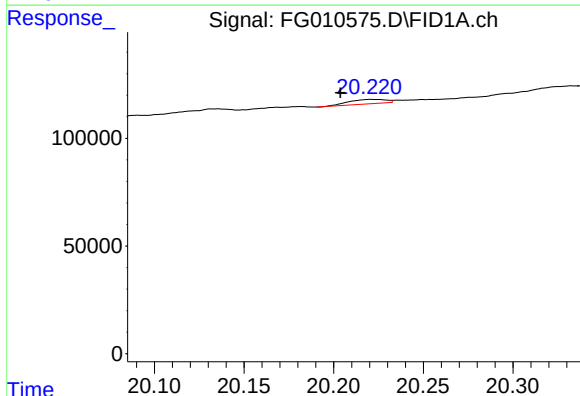

#16 N-HEXATRIACONTANE

R.T.: 20.221 min
Delta R.T.: 0.017 min
Response: 29644
Conc: 0.26 ug/ml

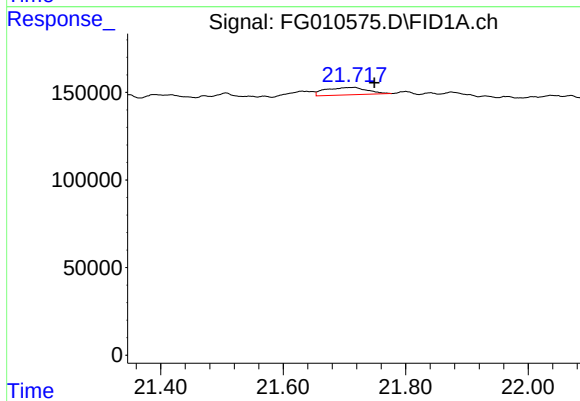

#18 N-TETRACONTANE

R.T.: 21.717 min
Delta R.T.: -0.032 min
Response: 202367
Conc: 1.72 ug/ml