

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG091522\
 Data File : FG010574.D
 Signal(s) : FID1A.ch
 Acq On : 15 Sep 2022 13:43
 Operator : YP\AJ
 Sample : 50 PPM TRPH STD
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :
 50 PPM TRPH STD

Integration File: autoint1.e
 Quant Time: Sep 16 04:16:10 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG082622.M
 Quant Title :
 QLast Update : Fri Aug 26 23:48:05 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.796	5604750	45.796 ug/ml
Target Compounds			
2) N-DECANE	4.316	6777348	52.874 ug/ml
3) N-DODECANE	6.499	6899774	52.426 ug/ml
4) N-TETRADECANE	8.330	6953052	51.371 ug/ml
5) N-HEXADECANE	9.938	7040694	50.246 ug/ml
6) N-OCTADECANE	11.384	7011363	49.107 ug/ml
7) N-EICOSANE	12.695	6856863	48.024 ug/ml
8) N-DOCOSANE	13.895	6534447	46.891 ug/ml
10) N-TETRACOSANE	15.000	6341215	45.765 ug/ml
11) N-HEXACOSANE	16.021	6095728	44.934 ug/ml
12) N-OCTACOSANE	16.974	6002009	45.386 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG091522\
Data File : FG010574.D
Signal(s) : FID1A.ch
Acq On : 15 Sep 2022 13:43
Operator : YP\AJ
Sample : 50 PPM TRPH STD
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
50 PPM TRPH STD

Integration File: autoint1.e
Quant Time: Sep 16 04:16:10 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG082622.M
Quant Title :
QLast Update : Fri Aug 26 23:48:05 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

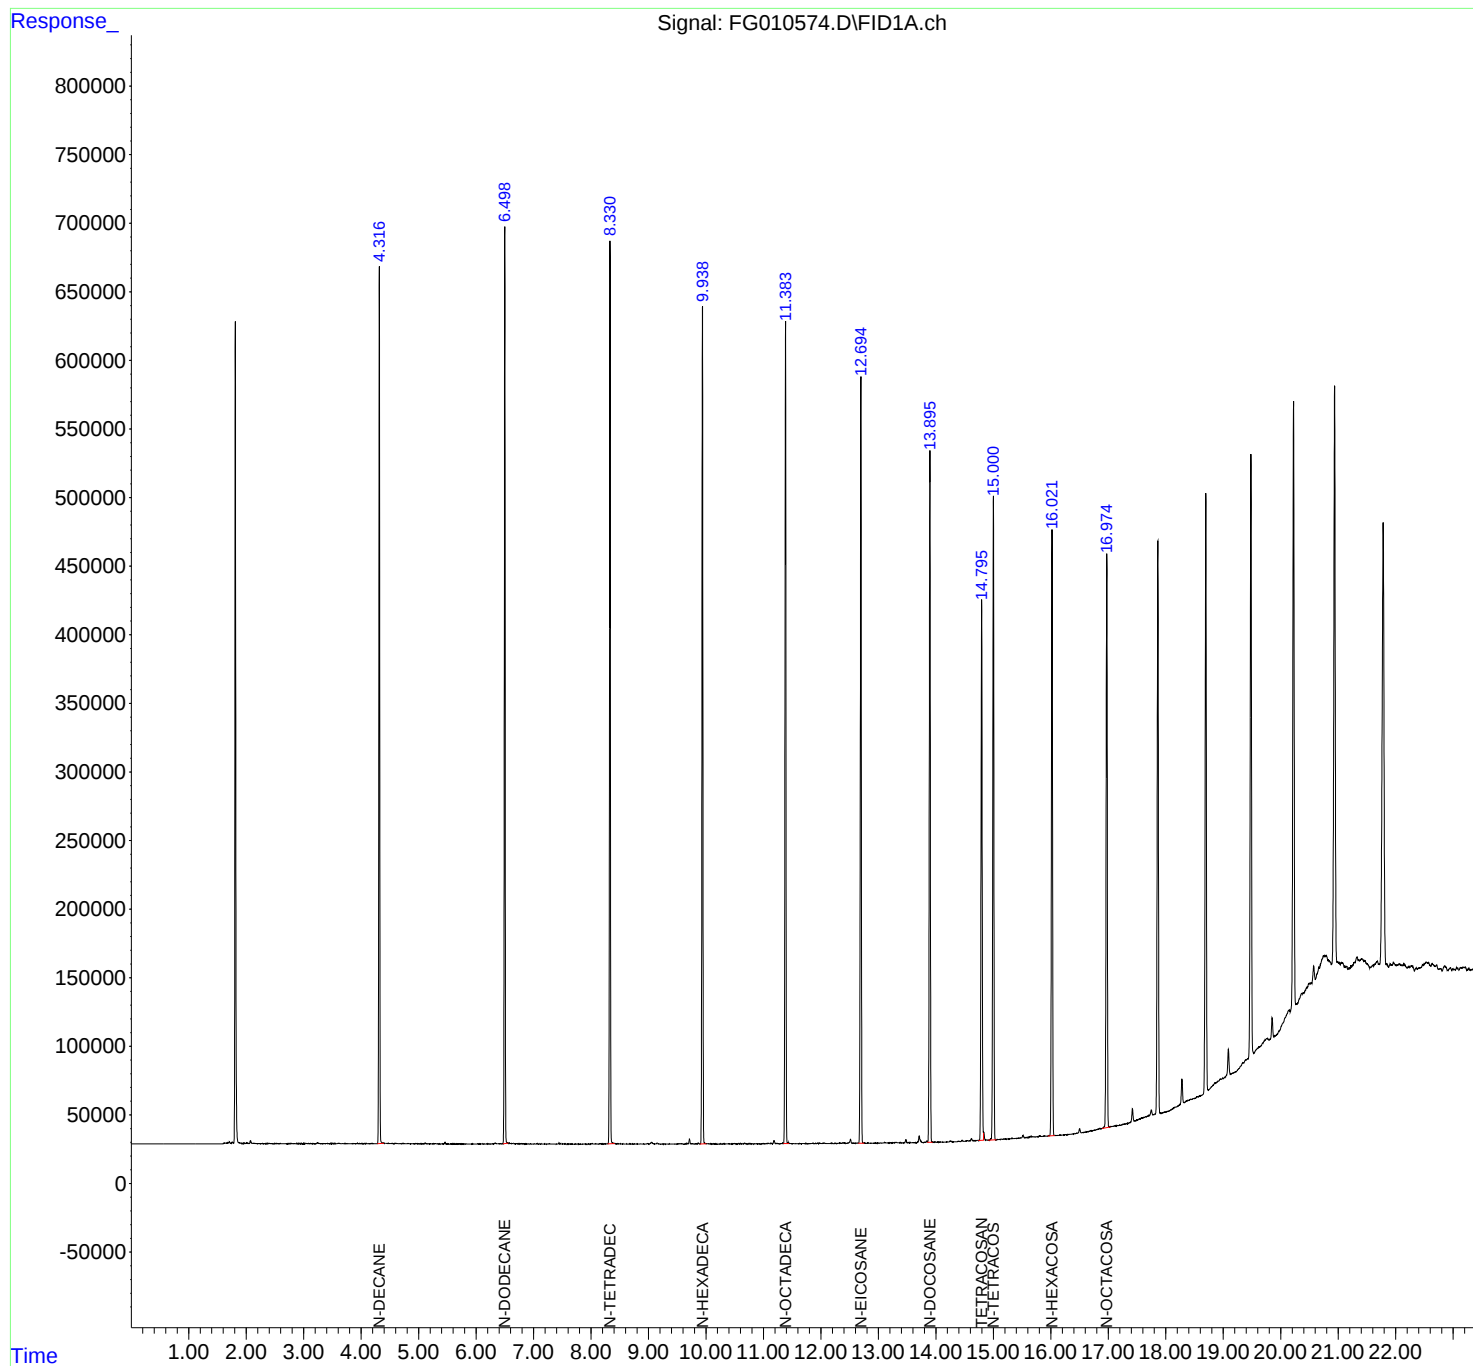


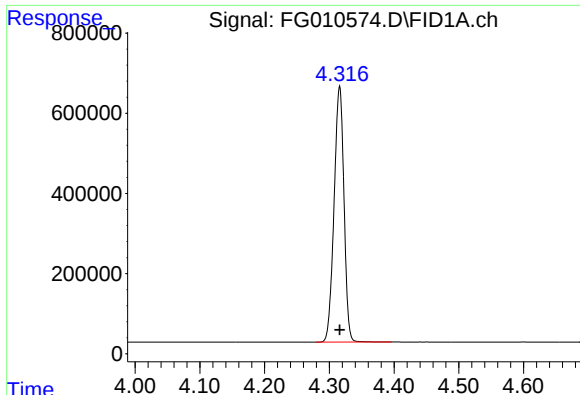

#2 N-DECANE


R.T.: 4.316 min
Delta R.T.: 0.000 min
Response: 6777348
Conc: 52.87 ug/ml

Instrument :
FID_G
ClientSampleId :
50 PPM TRPH STD

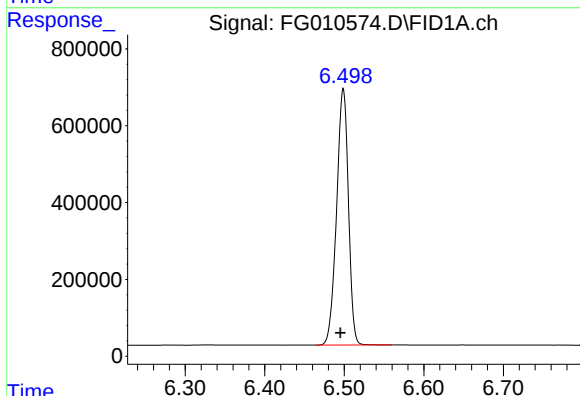


#3 N-DODECANE

R.T.: 6.499 min
Delta R.T.: 0.003 min
Response: 6899774
Conc: 52.43 ug/ml

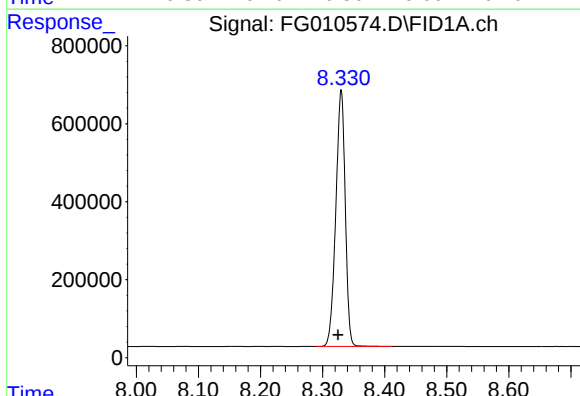


#4 N-TETRADECANE

R.T.: 8.330 min
Delta R.T.: 0.005 min
Response: 6953052
Conc: 51.37 ug/ml

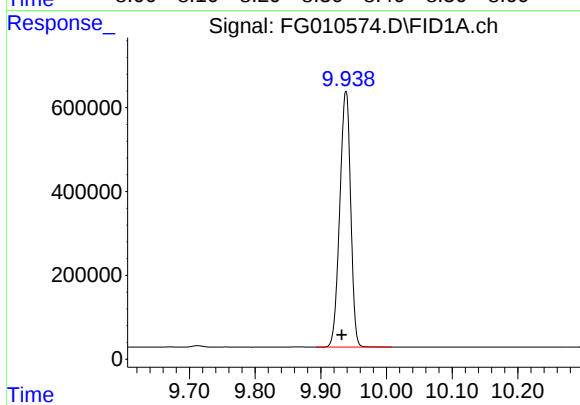

#5 N-HEXADECANE


R.T.: 9.938 min
Delta R.T.: 0.007 min
Response: 7040694
Conc: 50.25 ug/ml

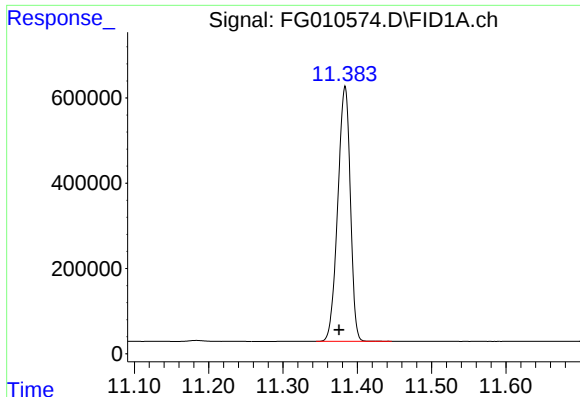

#6 N-OCTADECANE


R.T.: 11.384 min
Delta R.T.: 0.008 min
Response: 7011363
Conc: 49.11 ug/ml

Instrument :
FID_G
ClientSampleId :
50 PPM TRPH STD

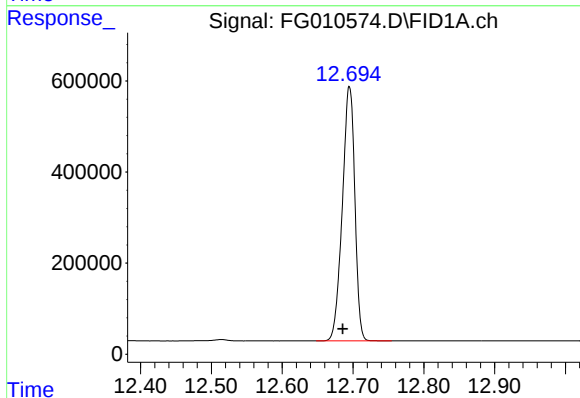


#7 N-EICOSANE

R.T.: 12.695 min
Delta R.T.: 0.009 min
Response: 6856863
Conc: 48.02 ug/ml

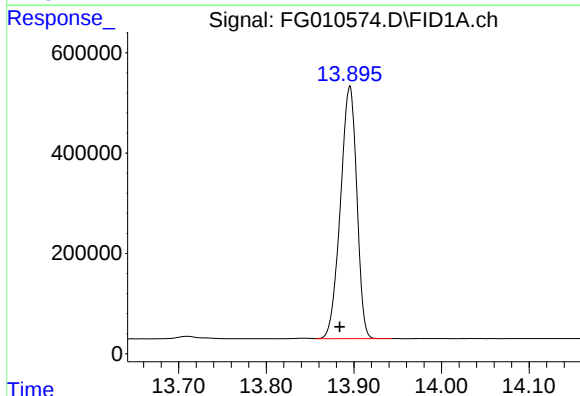


#8 N-DOCOSANE

R.T.: 13.895 min
Delta R.T.: 0.012 min
Response: 6534447
Conc: 46.89 ug/ml

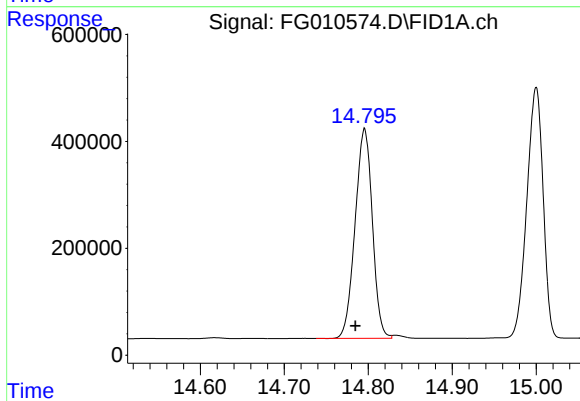

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.796 min
Delta R.T.: 0.011 min
Response: 5604750
Conc: 45.80 ug/ml

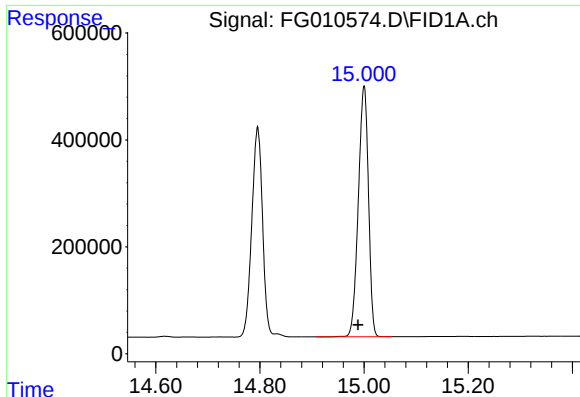

#10 N-TETRACOSANE


R.T.: 15.000 min
Delta R.T.: 0.012 min
Response: 6341215
Conc: 45.76 ug/ml

Instrument :
FID_G
ClientSampleId :
50 PPM TRPH STD

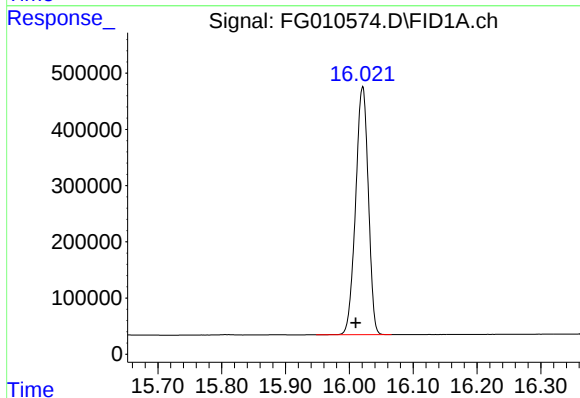

#11 N-HEXACOSANE

R.T.: 16.021 min
Delta R.T.: 0.011 min
Response: 6095728
Conc: 44.93 ug/ml

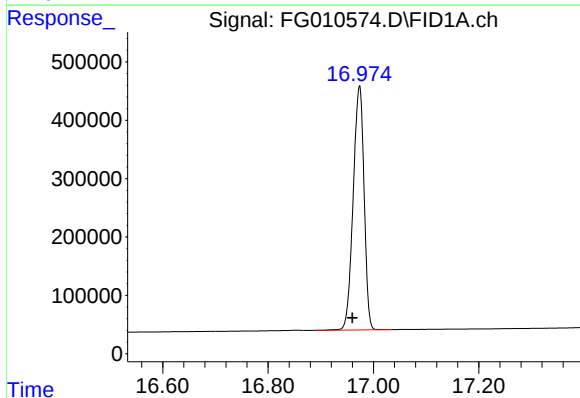

#12 N-OCTACOSANE

R.T.: 16.974 min
Delta R.T.: 0.013 min
Response: 6002009
Conc: 45.39 ug/ml