

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG091523\
Data File : FG012913.D
Signal(s) : FID1A.ch
Acq On : 15 Sep 2023 15:12
Operator : YP\AJ
Sample : RT MARKER
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Sep 15 15:43:12 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG090123.M
Quant Title :
QLast Update : Thu Aug 31 16:39:19 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

3)	N-DODECANE	6.768	2250827	16.630 ug/ml
12)	N-OCTACOSANE	17.256	1958676	16.719 ug/ml
13)	N-TRIACONTANE	18.144	177415	1.568 ug/ml
14)	N-DOTRIACONTANE	18.978	249803	2.398 ug/ml
15)	N-TETRATRIACONTANE	19.760	214459	2.320 ug/ml
16)	N-HEXATRIACONTANE	20.501	161101	1.988 ug/ml
17)	N-OCTATRIACONTANE	21.256	147829	1.936 ug/ml
18)	N-TETRACONTANE	22.204	148543	1.910 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG091523\
Data File : FG012913.D
Signal(s) : FID1A.ch
Acq On : 15 Sep 2023 15:12
Operator : YP\AJ
Sample : RT MARKER
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Sep 15 15:43:12 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG090123.M
Quant Title :
QLast Update : Thu Aug 31 16:39:19 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

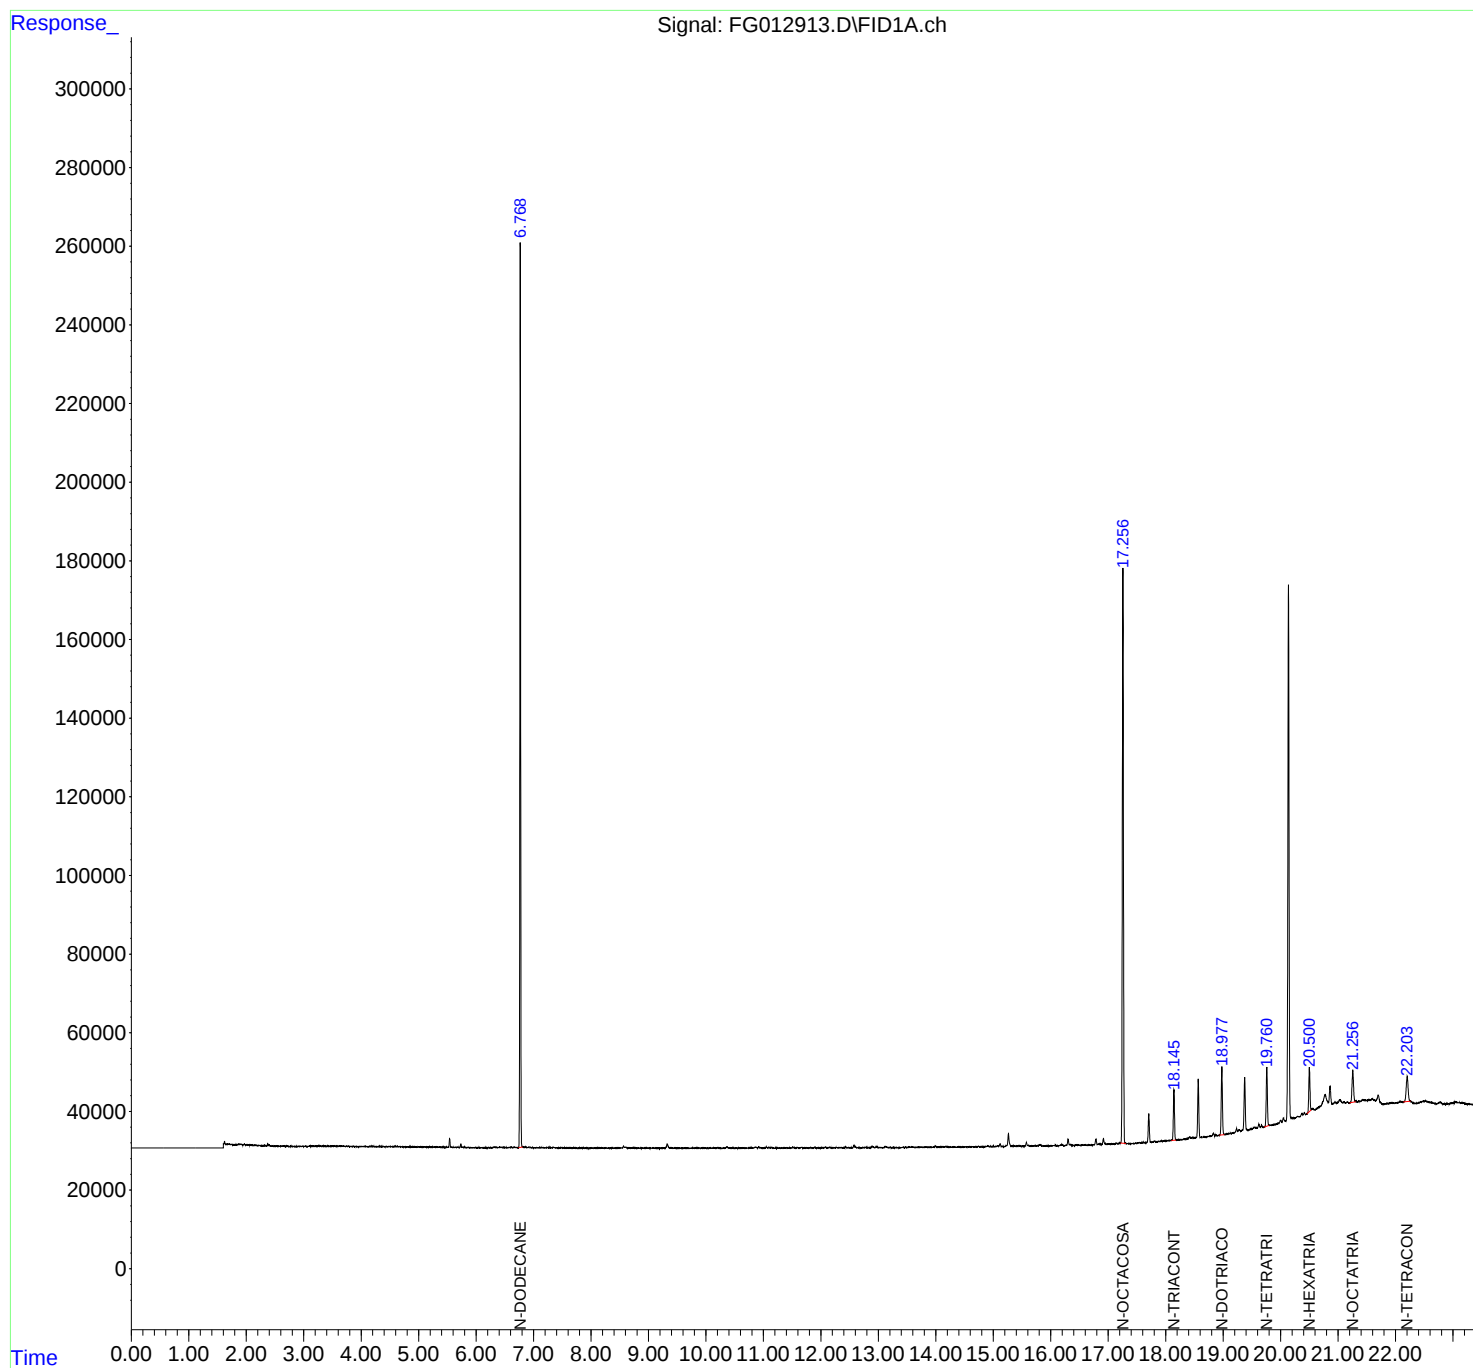


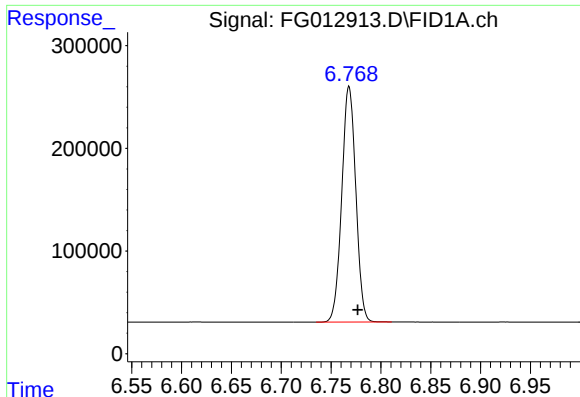

#3 N-DODECANE


R.T.: 6.768 min
Delta R.T.: -0.009 min
Response: 2250827
Conc: 16.63 ug/ml

Instrument :
FID_G
ClientSampleId :

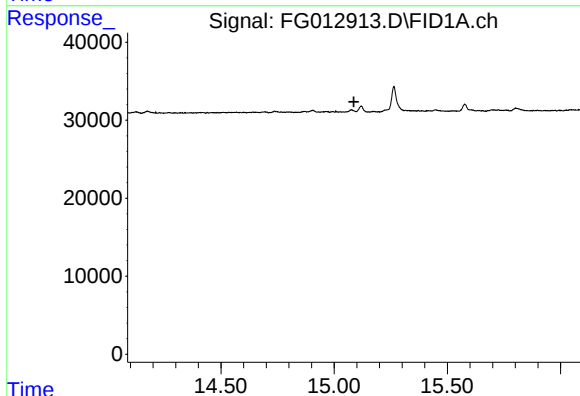


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 15.087 min
Response: 0
Conc: N.D.

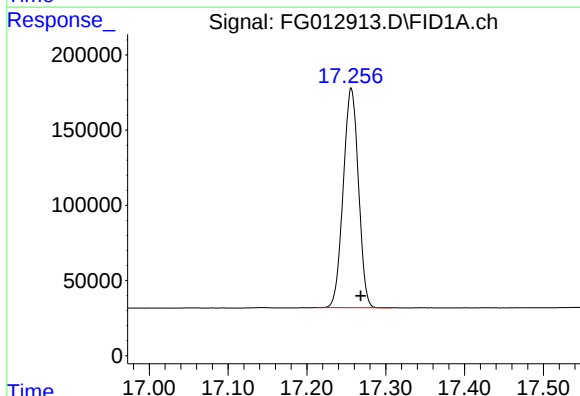


#12 N-OCTACOSANE

R.T.: 17.256 min
Delta R.T.: -0.012 min
Response: 1958676
Conc: 16.72 ug/ml

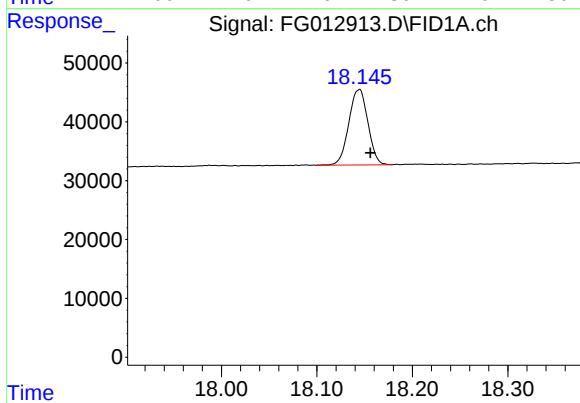

#13 N-TRIACONTANE


R.T.: 18.144 min
Delta R.T.: -0.012 min
Response: 177415
Conc: 1.57 ug/ml

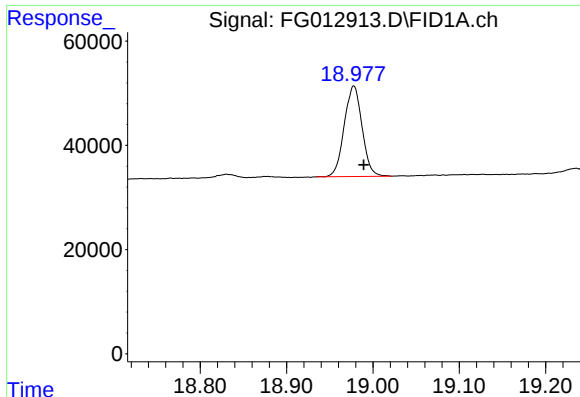

#14 N-DOTRIACONTANE


R.T.: 18.978 min
Delta R.T.: -0.012 min
Response: 249803
Conc: 2.40 ug/ml

Instrument :
FID_G
ClientSampleId :

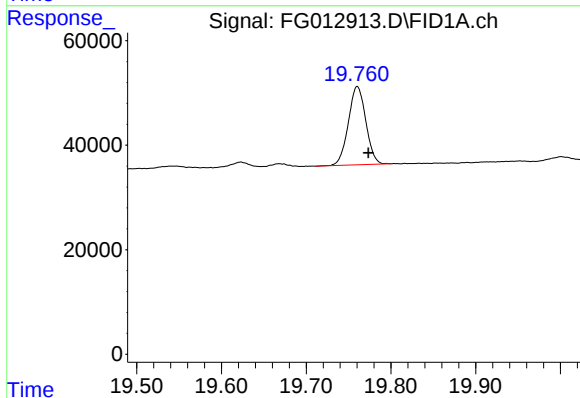


#15 N-TETRATRIACONTANE

R.T.: 19.760 min
Delta R.T.: -0.013 min
Response: 214459
Conc: 2.32 ug/ml

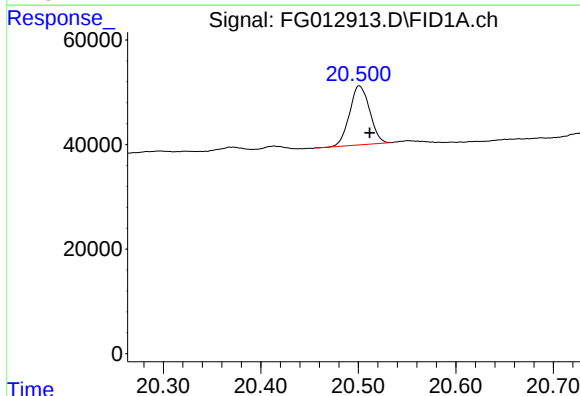


#16 N-HEXATRIACONTANE

R.T.: 20.501 min
Delta R.T.: -0.011 min
Response: 161101
Conc: 1.99 ug/ml

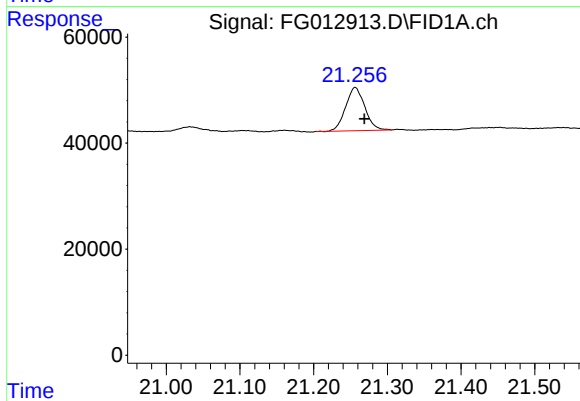

#17 N-OCTATRIACONTANE

R.T.: 21.256 min
Delta R.T.: -0.012 min
Response: 147829
Conc: 1.94 ug/ml

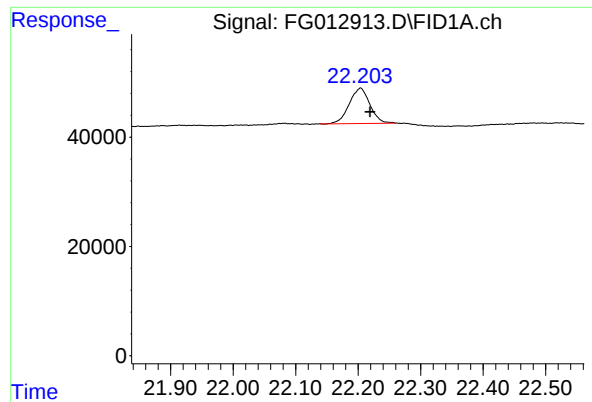

#18 N-TETRACONTANE

R.T.: 22.204 min
Delta R.T.: -0.015 min
Response: 148543
Conc: 1.91 ug/ml

Instrument :

FID_G

ClientSampleId :