

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG091523\
Data File : FG012919.D
Signal(s) : FID1A.ch
Acq On : 15 Sep 2023 18:12
Operator : YP\AJ
Sample : 04407-02
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
306-TP-3-5-CS-2

Integration File: autoint1.e
Quant Time: Sep 16 02:01:53 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG090123.M
Quant Title :
QLast Update : Thu Aug 31 16:39:19 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.080	1538715	13.766 ug/ml
Target Compounds			

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG091523\
Data File : FG012919.D
Signal(s) : FID1A.ch
Acq On : 15 Sep 2023 18:12
Operator : YP\AJ
Sample : 04407-02
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
306-TP-3-5-CS-2

Integration File: autoint1.e
Quant Time: Sep 16 02:01:53 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG090123.M
Quant Title :
QLast Update : Thu Aug 31 16:39:19 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

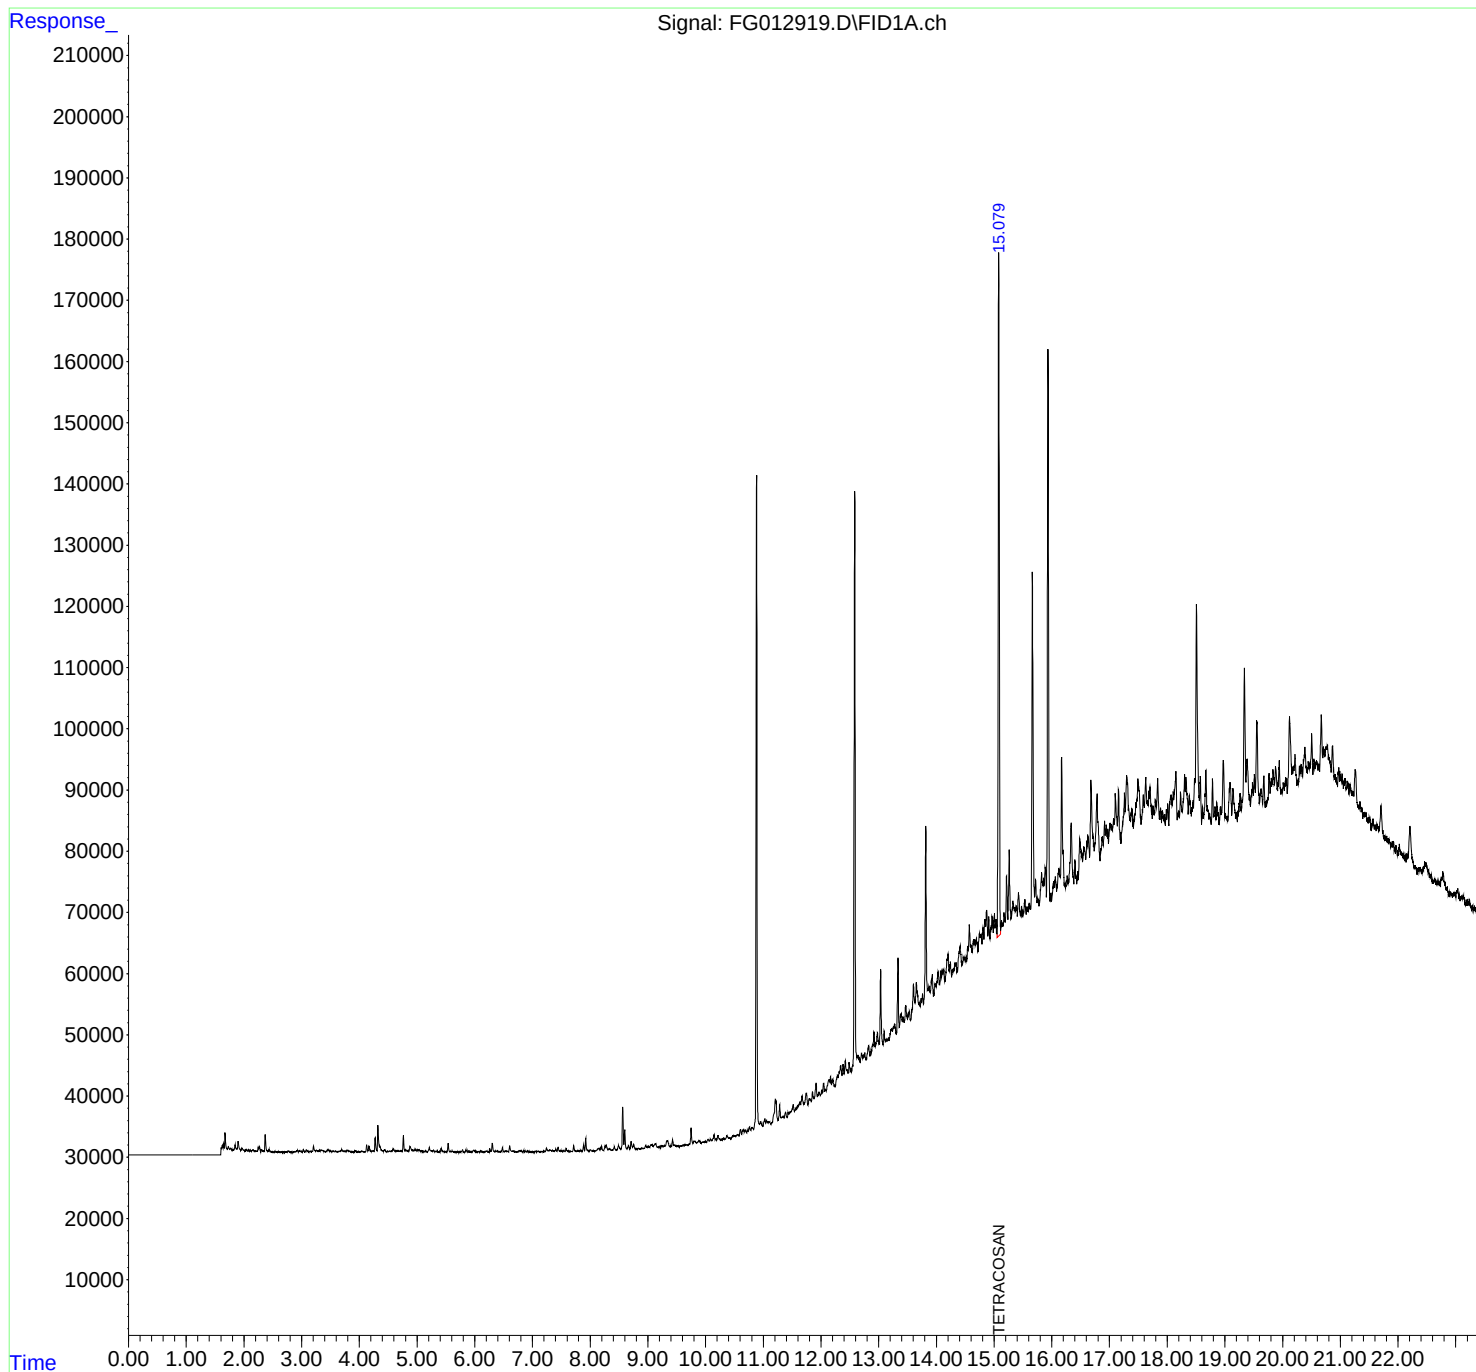

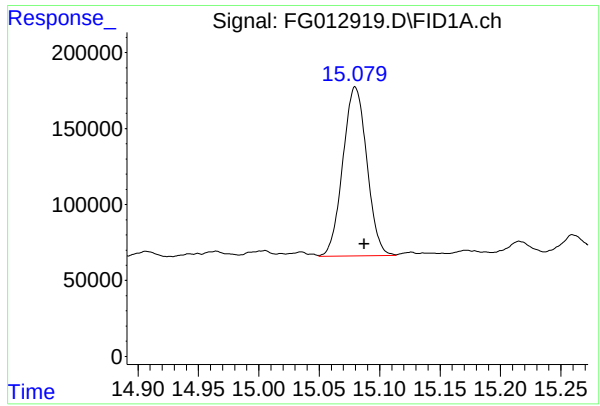

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 15.080 min
Delta R.T.: -0.008 min
Response: 1538715
Conc: 13.77 ug/ml

Instrument :
FID_G
ClientSampleId :
306-TP-3-5-CS-2