

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG091619\
 Data File : FG005964.D
 Signal(s) : FID1A.ch
 Acq On : 16 Sep 2019 19:34
 Operator : DD\AJ
 Sample : K4878-16 10X
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :
 TPA-9

Integration File: autoint1.e
 Quant Time: Sep 17 01:53:45 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG090719.M
 Quant Title :
 QLast Update : Mon Sep 09 05:03:58 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.732	220131	1.959 ug/ml
Target Compounds			
7) N-EICOSANE	12.587	275037	2.026 ug/ml
8) N-DOCOSANE	13.876	337633	2.567 ug/ml
10) N-TETRACOSANE	14.937	1639530	12.856 ug/ml
12) N-OCTACOSANE	16.952	721582	6.119 ug/ml
13) N-TRIACONTANE	17.809	192645	1.700 ug/ml
14) N-DOTRIACONTANE	18.629	749728	7.005 ug/ml
16) N-HEXATRIACONTANE	20.120	257567	2.585 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG091619\
Data File : FG005964.D
Signal(s) : FID1A.ch
Acq On : 16 Sep 2019 19:34
Operator : DD\AJ
Sample : K4878-16 10X
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
TPA-9

Integration File: autoint1.e
Quant Time: Sep 17 01:53:45 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG090719.M
Quant Title :
QLast Update : Mon Sep 09 05:03:58 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

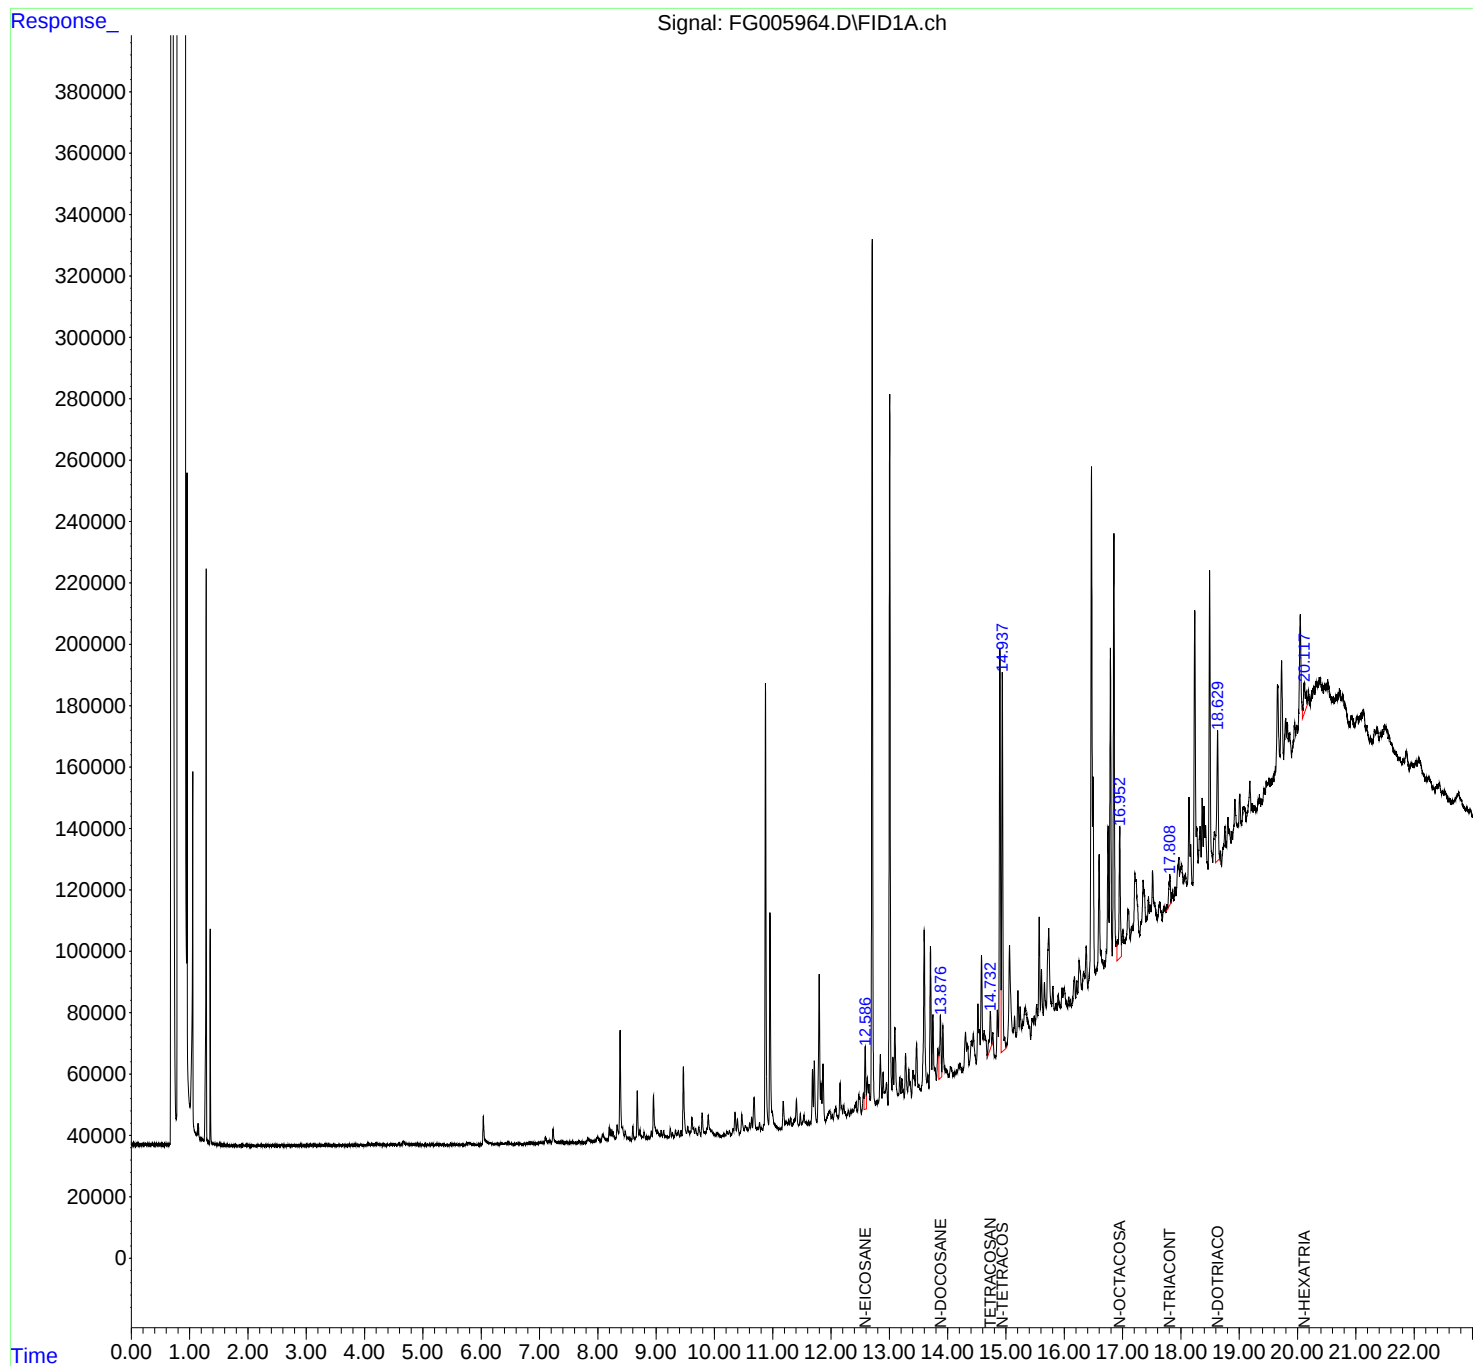


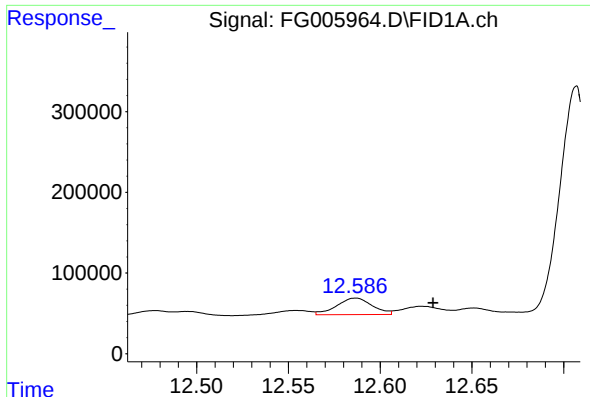

#7 N-EICOSANE


R.T.: 12.587 min
Delta R.T.: -0.042 min
Response: 275037
Conc: 2.03 ug/ml

Instrument :
FID_G
ClientSampleId :
TPA-9

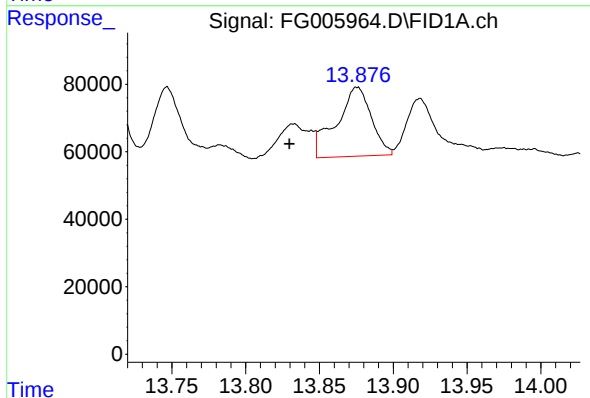


#8 N-DOCOSANE

R.T.: 13.876 min
Delta R.T.: 0.046 min
Response: 337633
Conc: 2.57 ug/ml

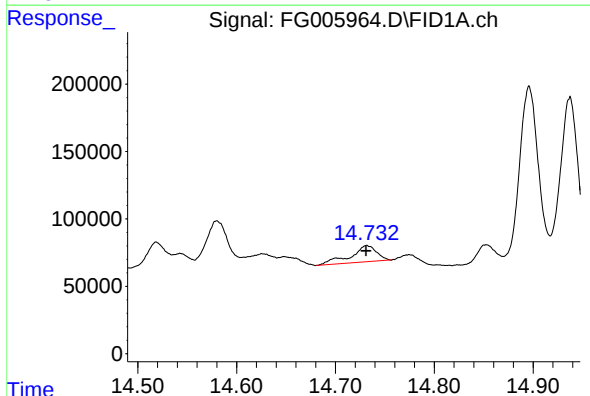


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.732 min
Delta R.T.: 0.001 min
Response: 220131
Conc: 1.96 ug/ml

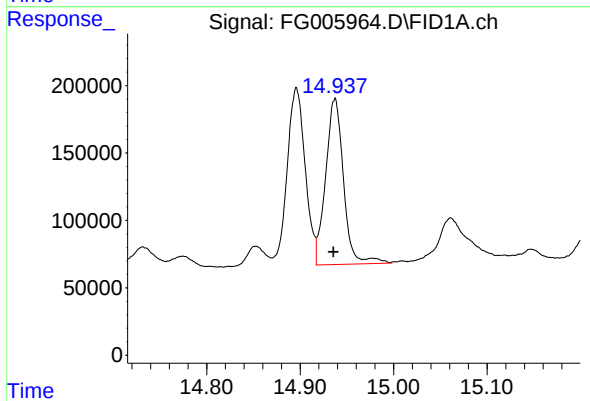

#10 N-TETRACOSANE


R.T.: 14.937 min
Delta R.T.: 0.002 min
Response: 1639530
Conc: 12.86 ug/ml

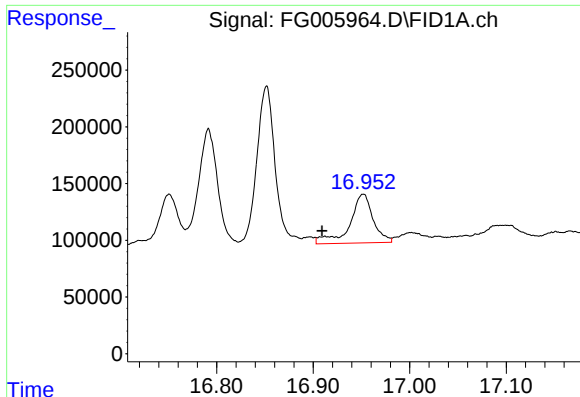

#12 N-OCTACOSANE


R.T.: 16.952 min
Delta R.T.: 0.042 min
Response: 721582
Conc: 6.12 ug/ml

Instrument :
FID_G
ClientSampleId :
TPA-9

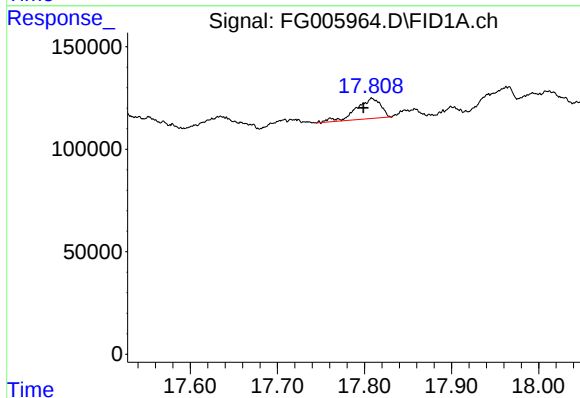


#13 N-TRIACONTANE

R.T.: 17.809 min
Delta R.T.: 0.010 min
Response: 192645
Conc: 1.70 ug/ml

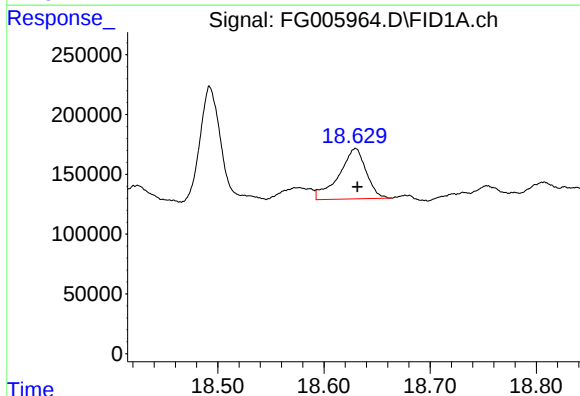

#14 N-DOTRIACONTANE

R.T.: 18.629 min
Delta R.T.: -0.002 min
Response: 749728
Conc: 7.01 ug/ml

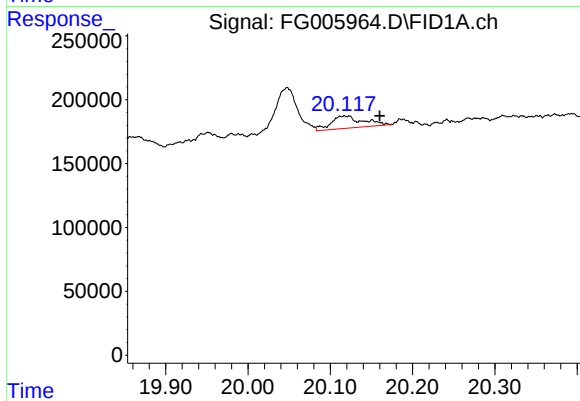

#16 N-HEXATRIACONTANE

R.T.: 20.120 min
Delta R.T.: -0.040 min
Response: 257567
Conc: 2.59 ug/ml