

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG091619\
Data File : FG005959.D
Signal(s) : FID1A.ch
Acq On : 16 Sep 2019 16:01
Operator : DD\AJ
Sample : K4878-26 5X
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
CSA-2-1

Integration File: autoint1.e
Quant Time: Sep 17 01:52:25 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG090719.M
Quant Title :
QLast Update : Mon Sep 09 05:03:58 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.733	428301	3.812 ug/ml

Target Compounds

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG091619\
Data File : FG005959.D
Signal(s) : FID1A.ch
Acq On : 16 Sep 2019 16:01
Operator : DD\AJ
Sample : K4878-26 5X
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
CSA-2-1

Integration File: autoint1.e
Quant Time: Sep 17 01:52:25 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG090719.M
Quant Title :
QLast Update : Mon Sep 09 05:03:58 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

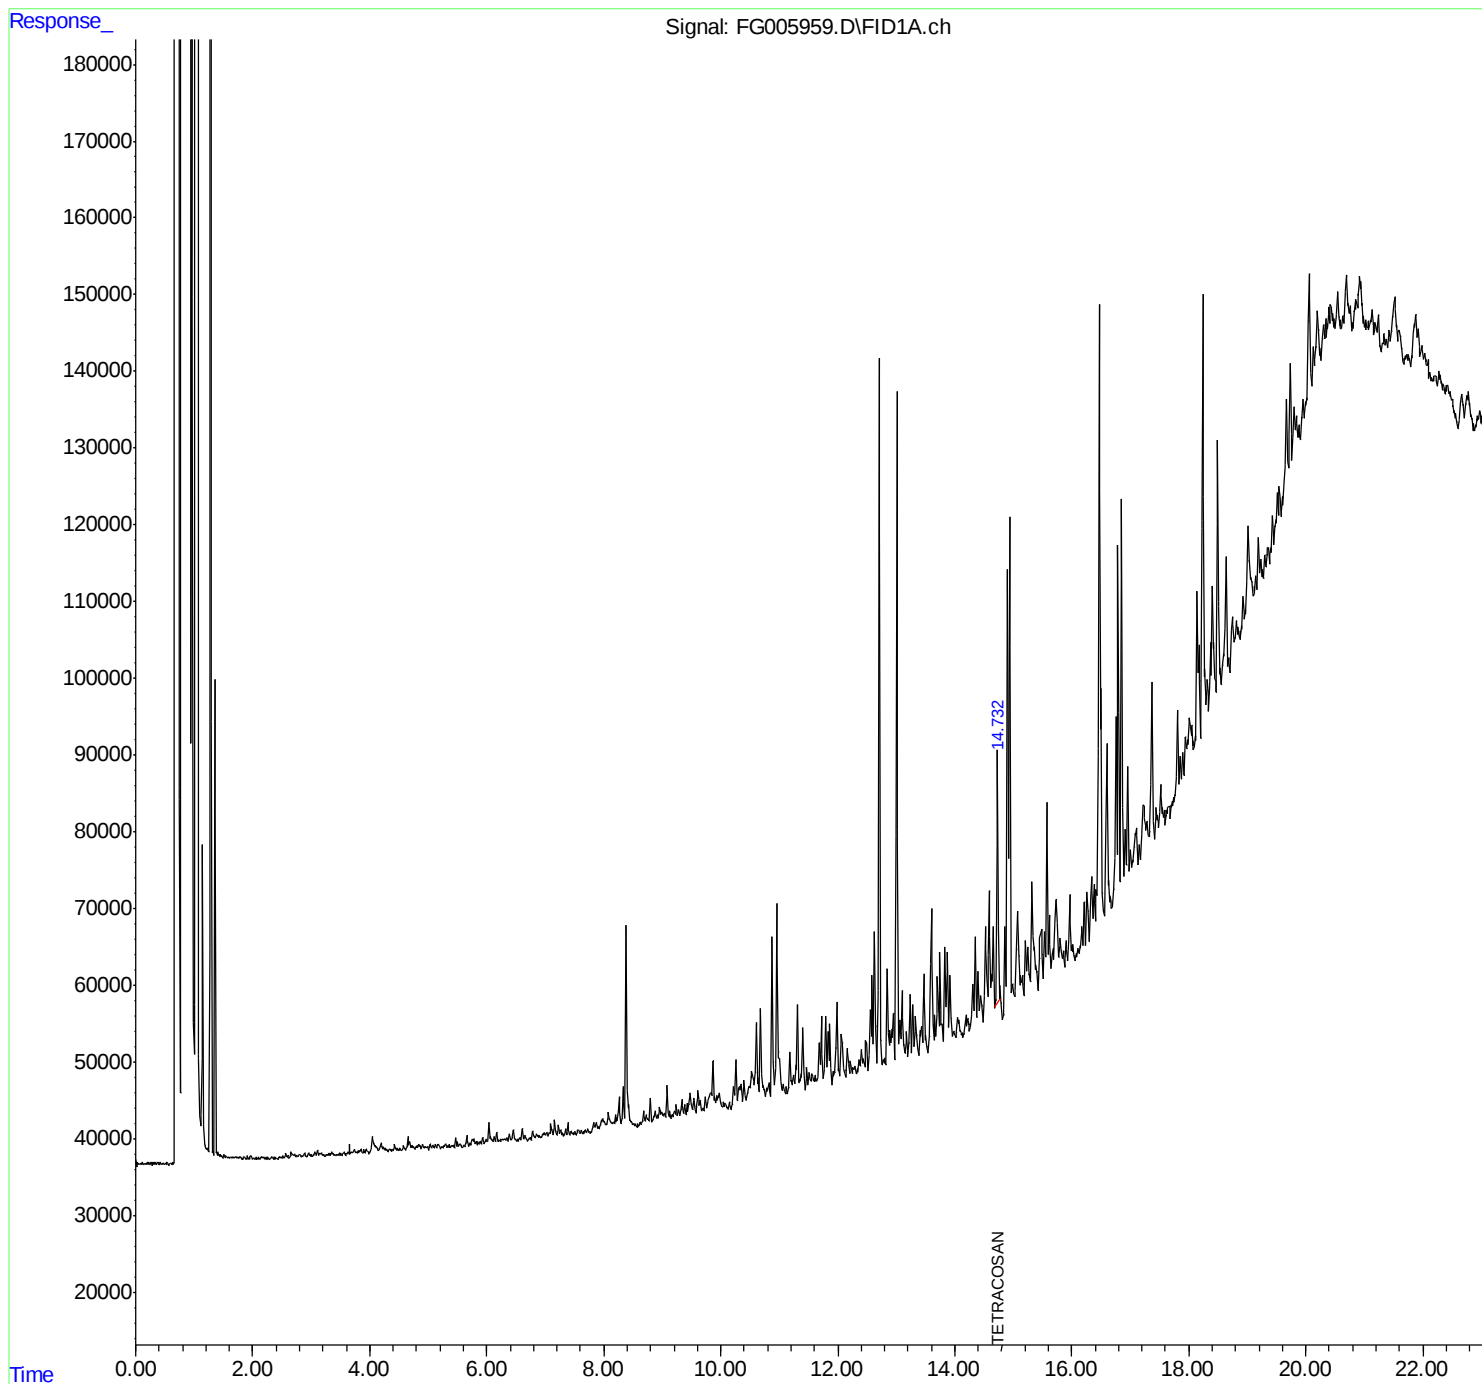

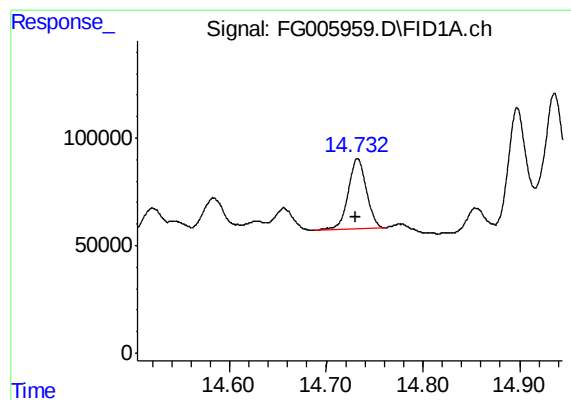

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.733 min
Delta R.T.: 0.002 min
Response: 428301
Conc: 3.81 ug/ml

Instrument :
FID_G
ClientSampleId :
CSA-2-1