

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG091622\
Data File : FG010591.D
Signal(s) : FID1A.ch
Acq On : 16 Sep 2022 13:27
Operator : YP\AJ
Sample : RT MARKER
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Sep 17 14:04:18 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG082622.M
Quant Title :
QLast Update : Fri Aug 26 23:48:05 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
3)	N-DODECANE	6.488	3240344	24.621 ug/ml
12)	N-OCTACOSANE	16.960	2908631	21.994 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG091622\
Data File : FG010591.D
Signal(s) : FID1A.ch
Acq On : 16 Sep 2022 13:27
Operator : YP\AJ
Sample : RT MARKER
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Sep 17 14:04:18 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG082622.M
Quant Title :
QLast Update : Fri Aug 26 23:48:05 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

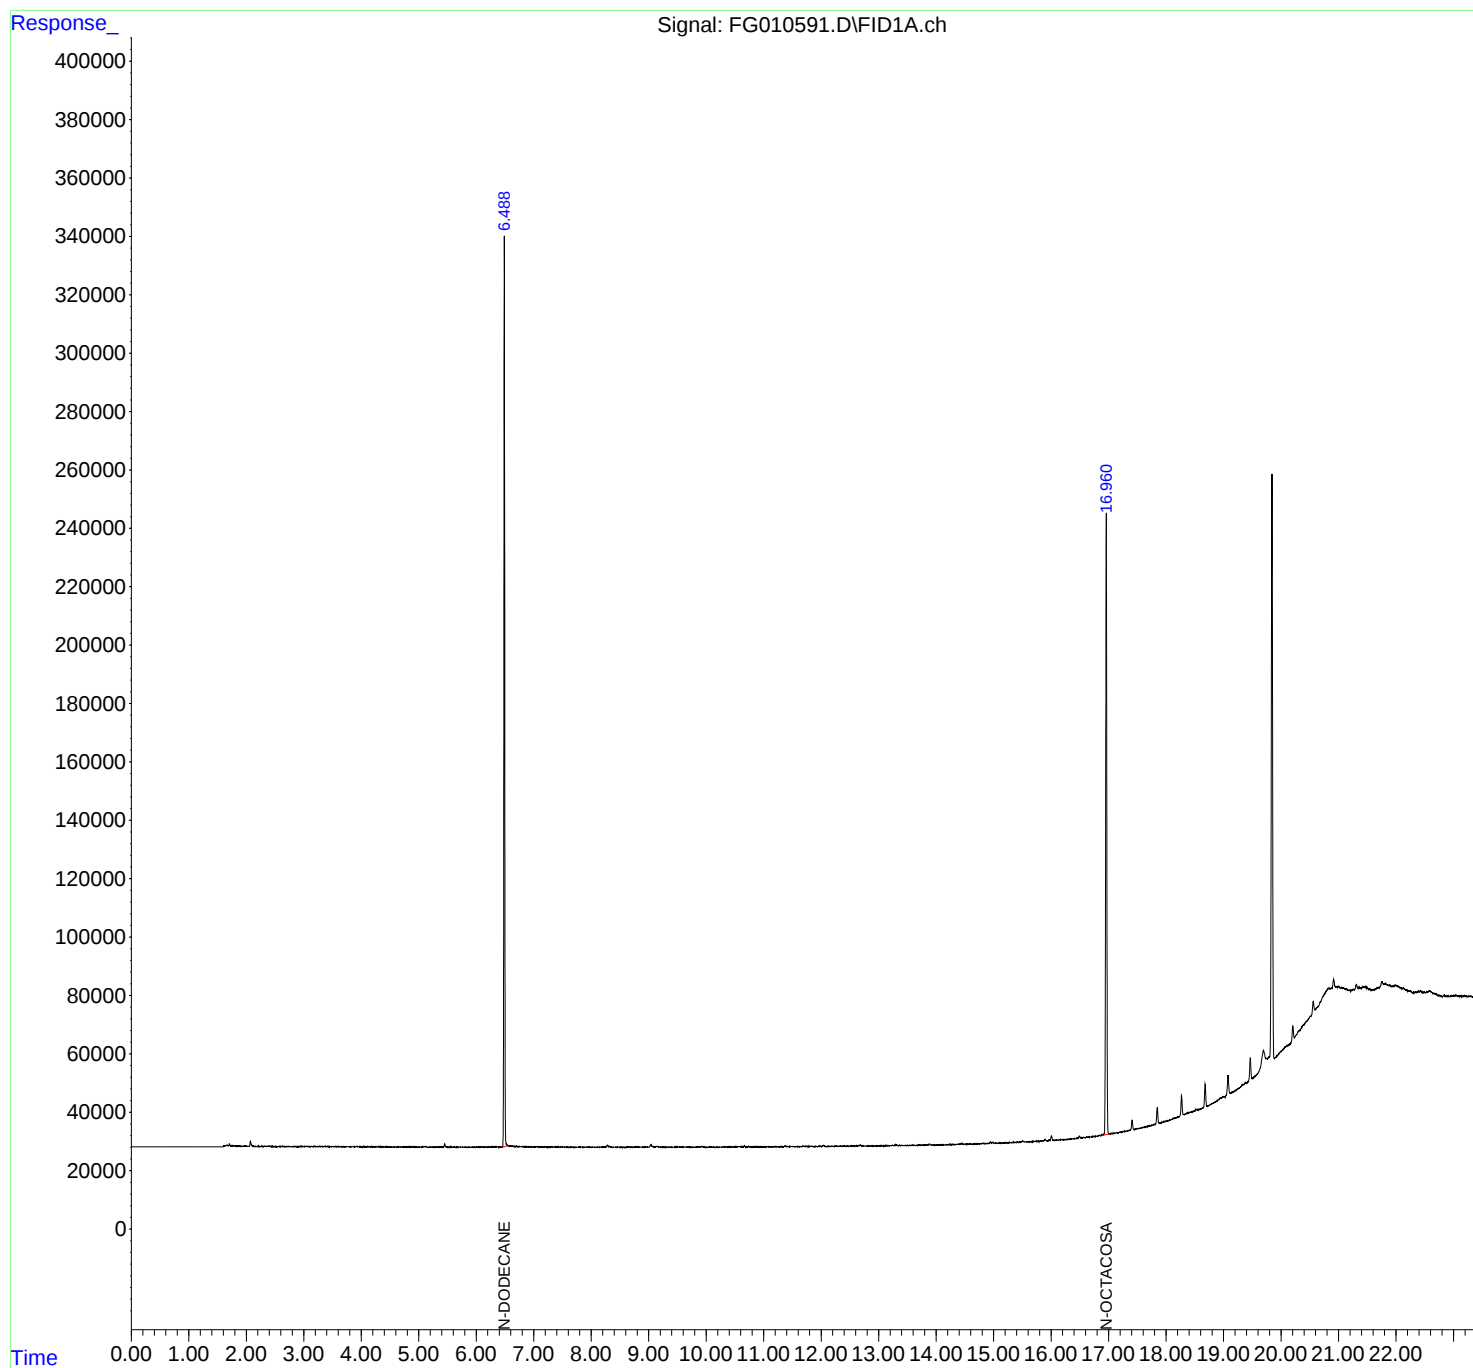


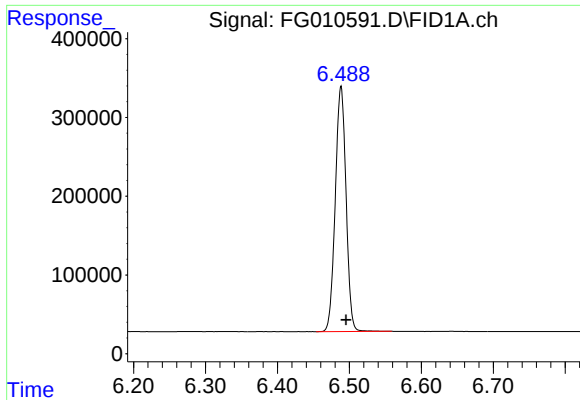

#3 N-DODECANE


R.T.: 6.488 min
Delta R.T.: -0.007 min
Response: 3240344
Conc: 24.62 ug/ml

Instrument :
FID_G
ClientSampleId :

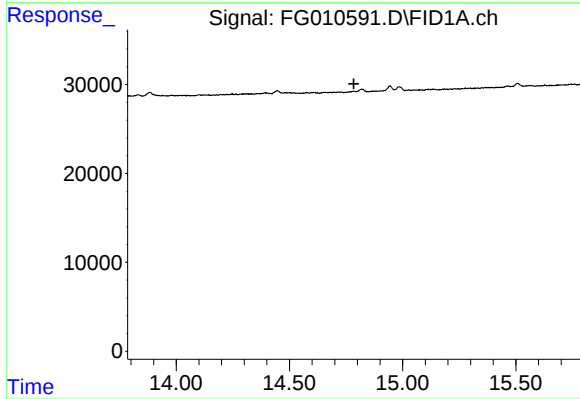

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.785 min
Response: 0
Conc: N.D.

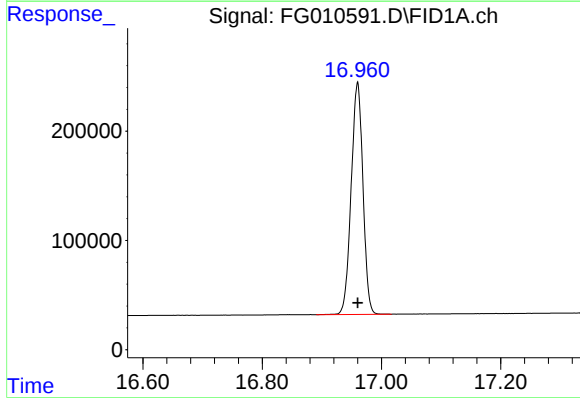

#12 N-OCTACOSANE

R.T.: 16.960 min
Delta R.T.: 0.000 min
Response: 2908631
Conc: 21.99 ug/ml