

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_G\Data\FG091818\  
Data File : FG002333.D  
Signal(s) : FID1A.ch  
Acq On : 18 Sep 2018 12:31  
Operator : AJ\SJ  
Sample : I.BLK  
Misc :  
ALS Vial : 2 Sample Multiplier: 1

Integration File: autoint1.e  
Quant Time: Sep 19 01:05:25 2018  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_G\Method\FG083018.M  
Quant Title :  
QLast Update : Thu Aug 30 14:49:31 2018  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
-----			
System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.422	2552710	20.233 ug/ml
Target Compounds			
14) N-DOTRIACONTANE	18.316	111681	0.757 ug/ml
-----			


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_G\Data\FG091818\  
Data File : FG002333.D  
Signal(s) : FID1A.ch  
Acq On : 18 Sep 2018 12:31  
Operator : AJ\SJ  
Sample : I.BLK  
Misc :  
ALS Vial : 2 Sample Multiplier: 1

Integration File: autoint1.e  
Quant Time: Sep 19 01:05:25 2018  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_G\Method\FG083018.M  
Quant Title :  
QLast Update : Thu Aug 30 14:49:31 2018  
Response via : Initial Calibration  
Integrator: ChemStation


Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

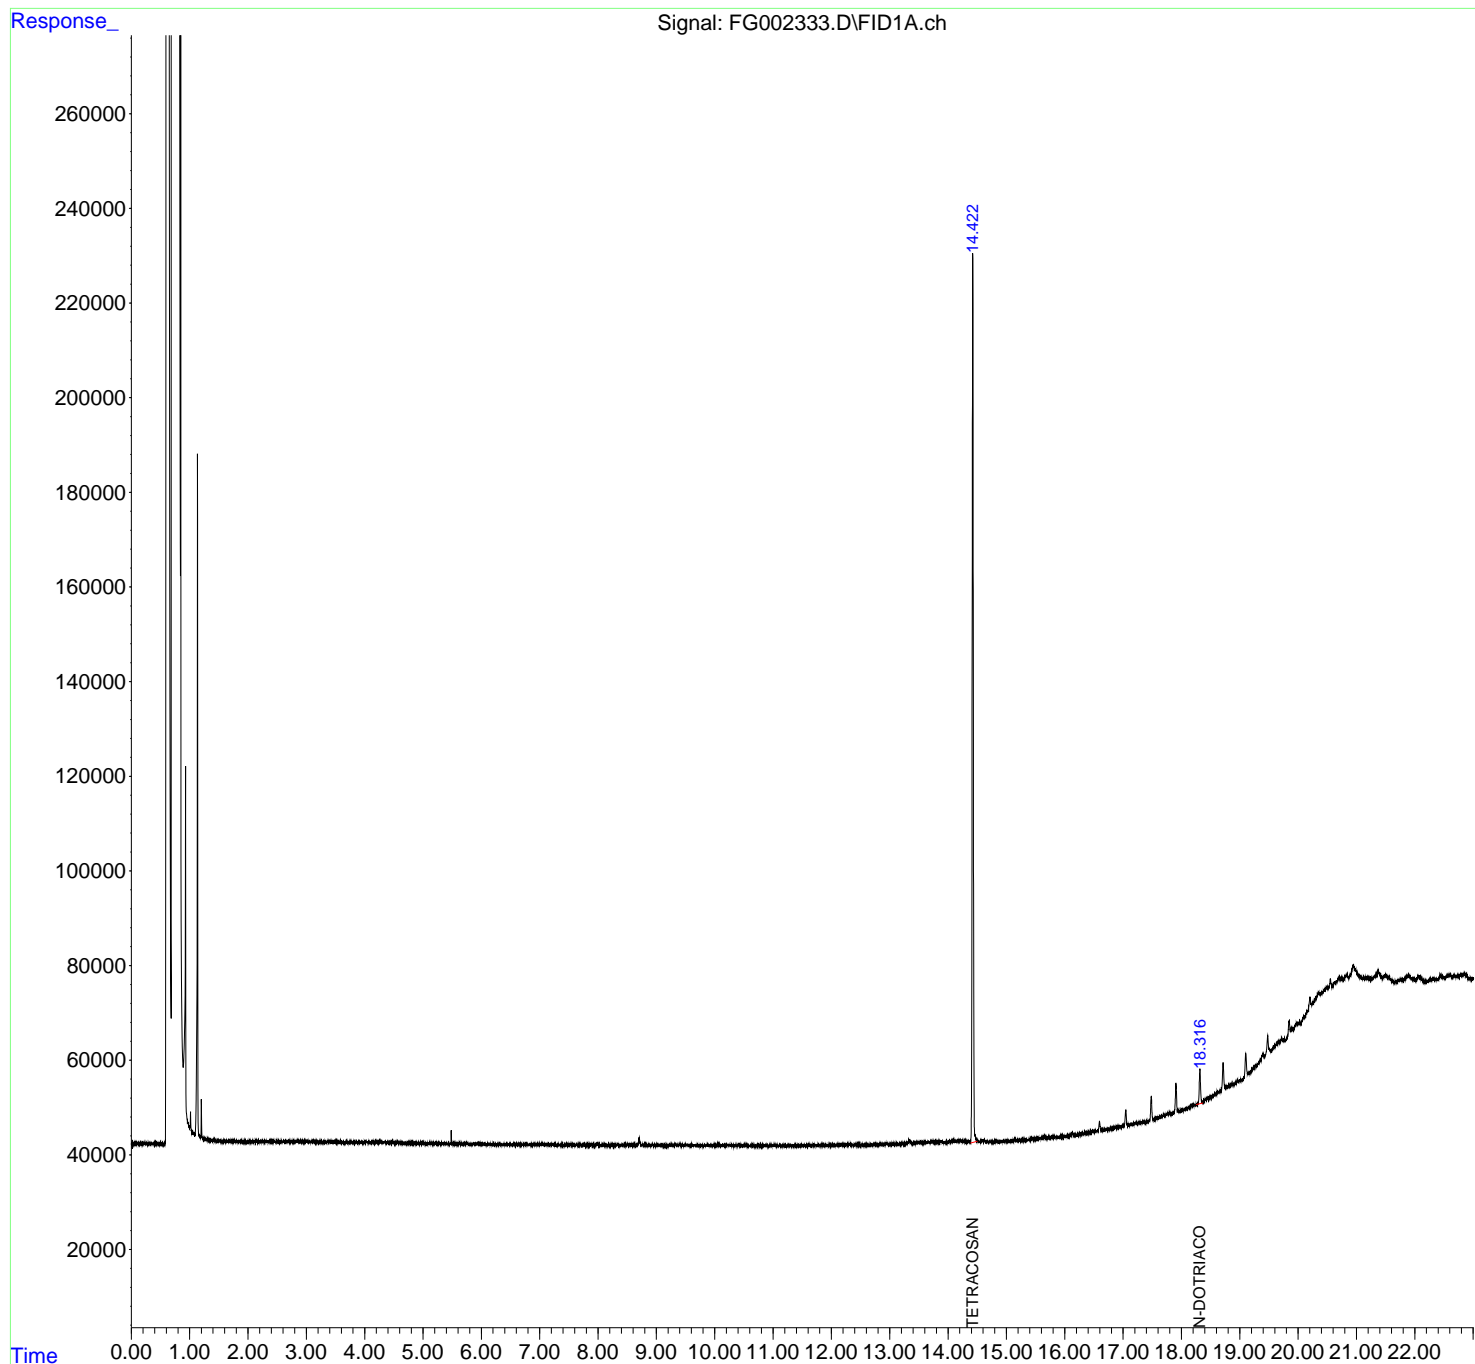

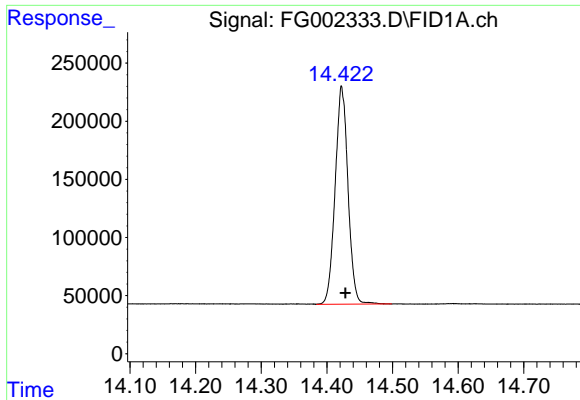

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.422 min  
Delta R.T.: -0.006 min  
Response: 2552710  
Conc: 20.23 ug/ml

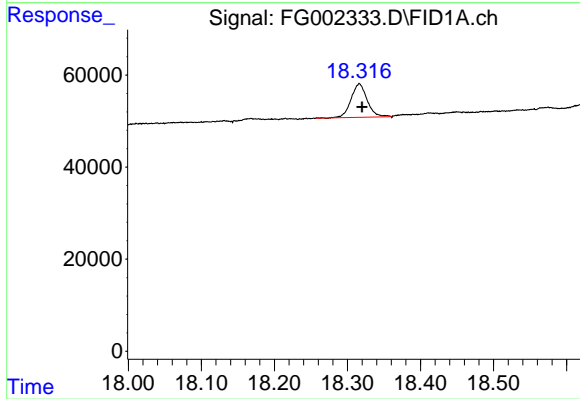

#14 N-DOTRIACONTANE

R.T.: 18.316 min  
Delta R.T.: -0.004 min  
Response: 111681  
Conc: 0.76 ug/ml