

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_G\Data\FG091919\  
Data File : FG006008.D  
Signal(s) : FID1A.ch  
Acq On : 19 Sep 2019 11:59  
Operator : DD\AJ  
Sample : RT MARKER  
Misc :  
ALS Vial : 4 Sample Multiplier: 1

Instrument :  
FID\_G  
ClientSampleId :

Integration File: autoint1.e  
Quant Time: Sep 20 01:44:05 2019  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_G\Method\FG090719.M  
Quant Title :  
QLast Update : Mon Sep 09 05:03:58 2019  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

| Compound                    | R.T.   | Response | Conc Units   |
|-----------------------------|--------|----------|--------------|
| -----                       |        |          |              |
| System Monitoring Compounds |        |          |              |
| Target Compounds            |        |          |              |
| 3) N-DODECANE               | 6.460  | 2378549  | 16.799 ug/ml |
| 12) N-OCTACOSANE            | 16.923 | 2270894  | 19.257 ug/ml |
| 15) N-TETRATRIACONTANE      | 19.442 | 173672   | 1.679 ug/ml  |
| 16) N-HEXATRIACONTANE       | 20.189 | 965750   | 9.693 ug/ml  |
| -----                       |        |          |              |

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_G\Data\FG091919\  
Data File : FG006008.D  
Signal(s) : FID1A.ch  
Acq On : 19 Sep 2019 11:59  
Operator : DD\AJ  
Sample : RT MARKER  
Misc :  
ALS Vial : 4 Sample Multiplier: 1

Instrument :  
FID\_G  
ClientSampleId :

Integration File: autoint1.e  
Quant Time: Sep 20 01:44:05 2019  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_G\Method\FG090719.M  
Quant Title :  
QLast Update : Mon Sep 09 05:03:58 2019  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

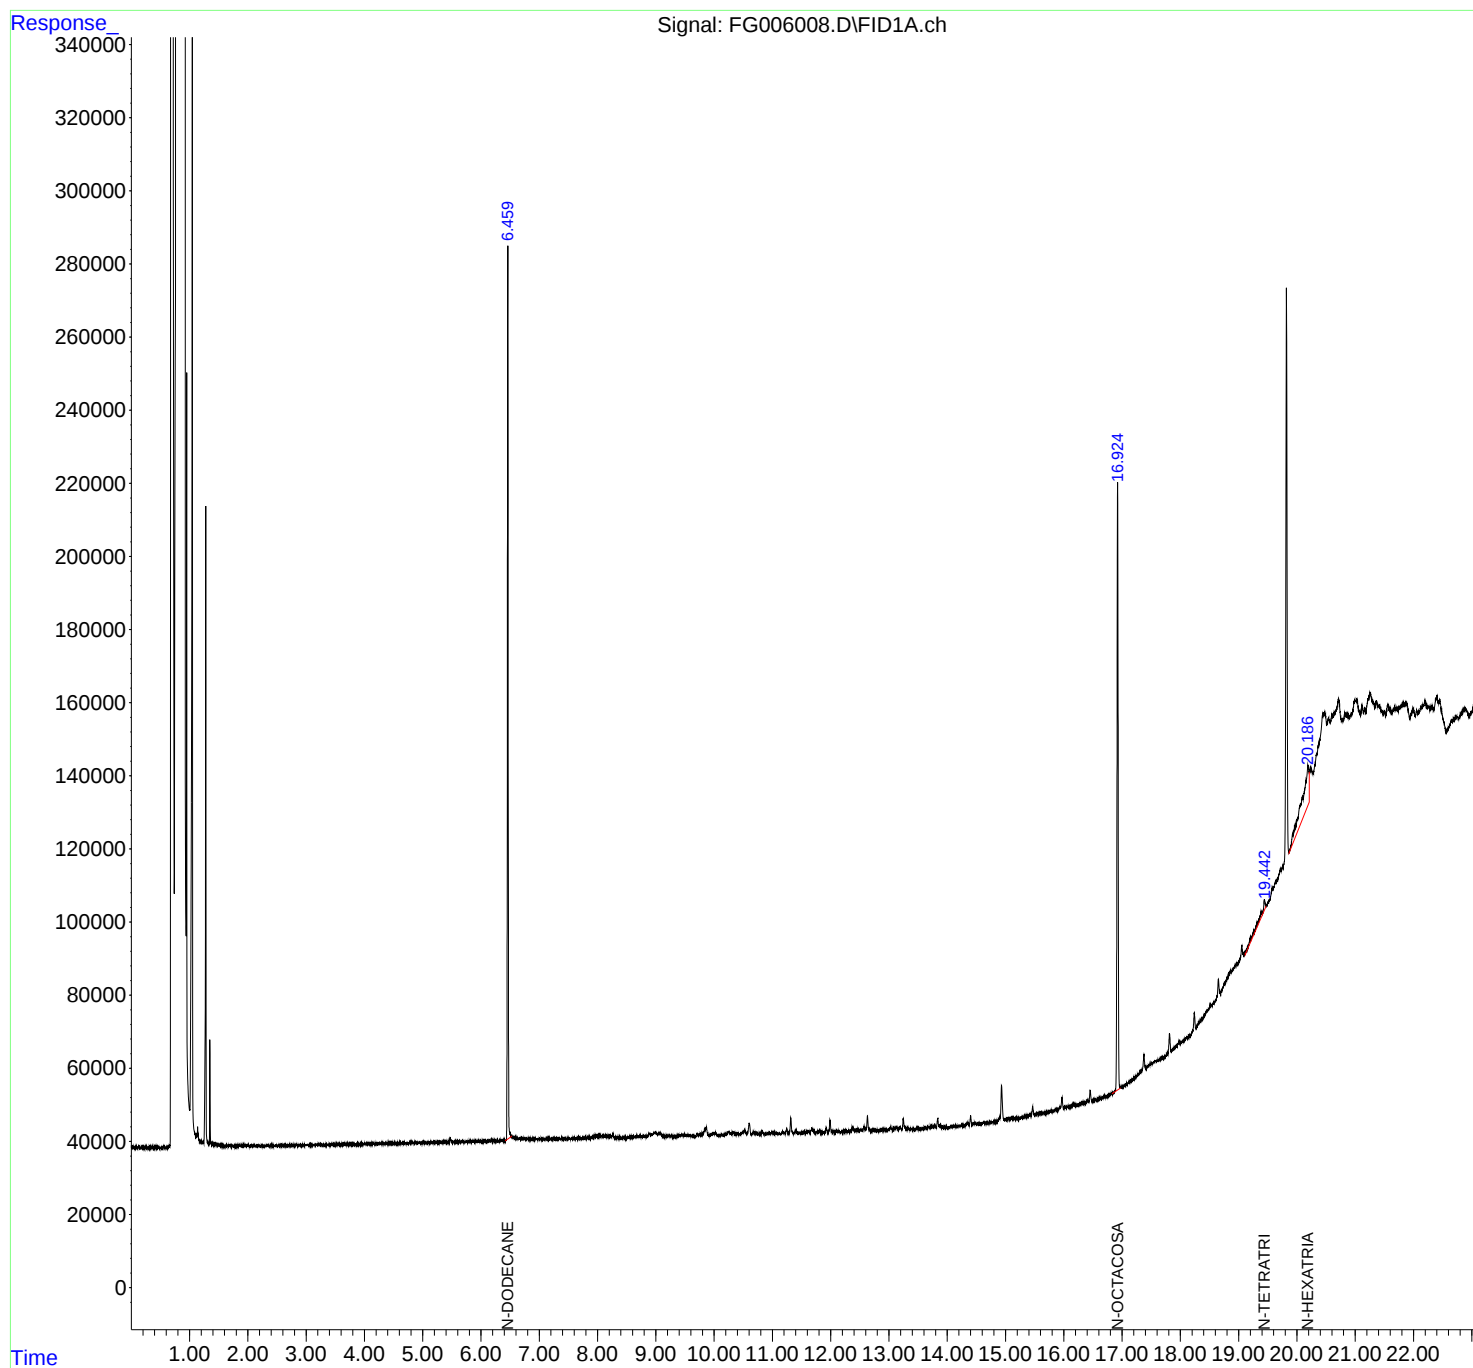


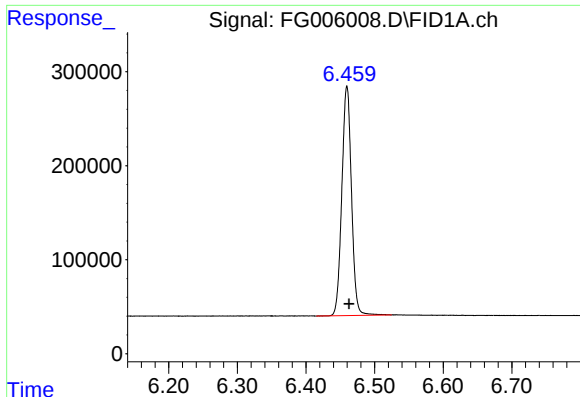

#3 N-DODECANE


R.T.: 6.460 min  
Delta R.T.: -0.003 min  
Response: 2378549  
Conc: 16.80 ug/ml

Instrument :  
FID\_G  
ClientSampleId :

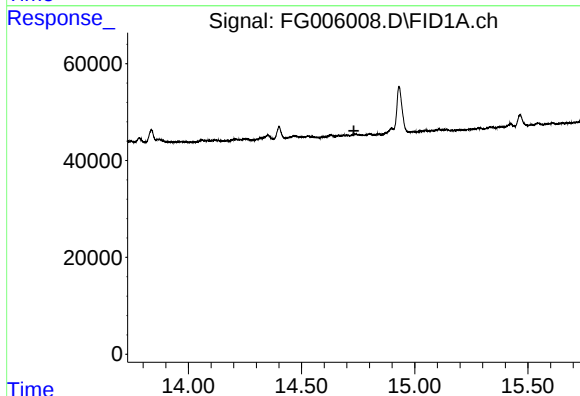


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min  
Exp R.T. : 14.731 min  
Response: 0  
Conc: N.D.

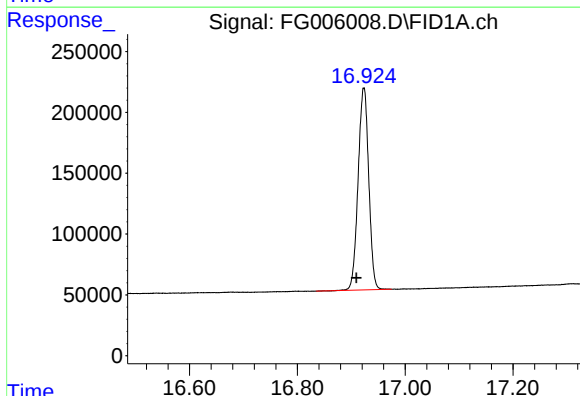


#12 N-OCTACOSANE

R.T.: 16.923 min  
Delta R.T.: 0.014 min  
Response: 2270894  
Conc: 19.26 ug/ml

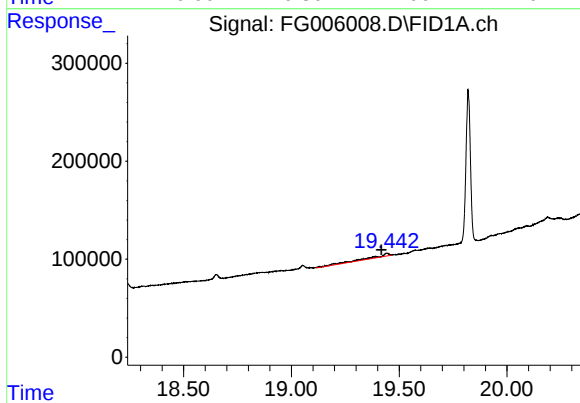

#15 N-TETRATRIACONTANE

R.T.: 19.442 min  
Delta R.T.: 0.024 min  
Response: 173672  
Conc: 1.68 ug/ml

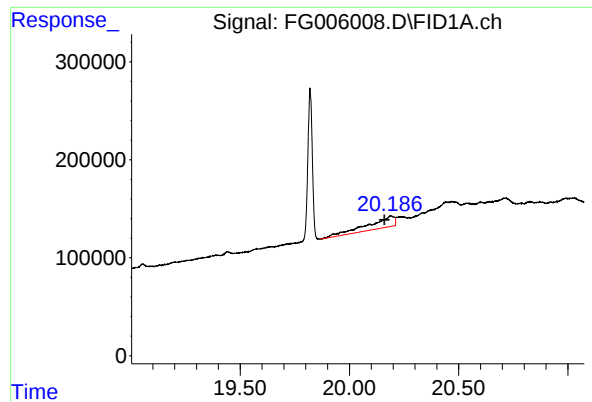

#16 N-HEXATRIACONTANE

R.T.: 20.189 min  
Delta R.T.: 0.029 min  
Response: 965750  
Conc: 9.69 ug/ml

Instrument :  
FID\_G  
ClientSampleId :