

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG091919\
 Data File : FG006013.D
 Signal(s) : FID1A.ch
 Acq On : 19 Sep 2019 14:25
 Operator : DD\AJ
 Sample : K4662-09 5X
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :
 CL-02-091819

Integration File: autoint1.e
 Quant Time: Sep 20 01:45:20 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG090719.M
 Quant Title :
 QLast Update : Mon Sep 09 05:03:58 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.733	384269	3.420 ug/ml
Target Compounds			
7) N-EICOSANE	12.591	196418	1.447 ug/ml
10) N-TETRACOSANE	14.944	726122	5.694 ug/ml
12) N-OCTACOSANE	16.859f	634475	5.380 ug/ml
13) N-TRIACONTANE	17.807	215562	1.902 ug/ml
14) N-DOTRIACONTANE	18.643	374948	3.503 ug/ml
15) N-TETRATRIACONTANE	19.431	291920	2.822 ug/ml
16) N-HEXATRIACONTANE	20.130	115684	1.161 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG091919\
Data File : FG006013.D
Signal(s) : FID1A.ch
Acq On : 19 Sep 2019 14:25
Operator : DD\AJ
Sample : K4662-09 5X
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
FID_G
ClientSampled :
CL-02-091819

Integration File: autoint1.e
Quant Time: Sep 20 01:45:20 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG090719.M
Quant Title :
QLast Update : Mon Sep 09 05:03:58 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

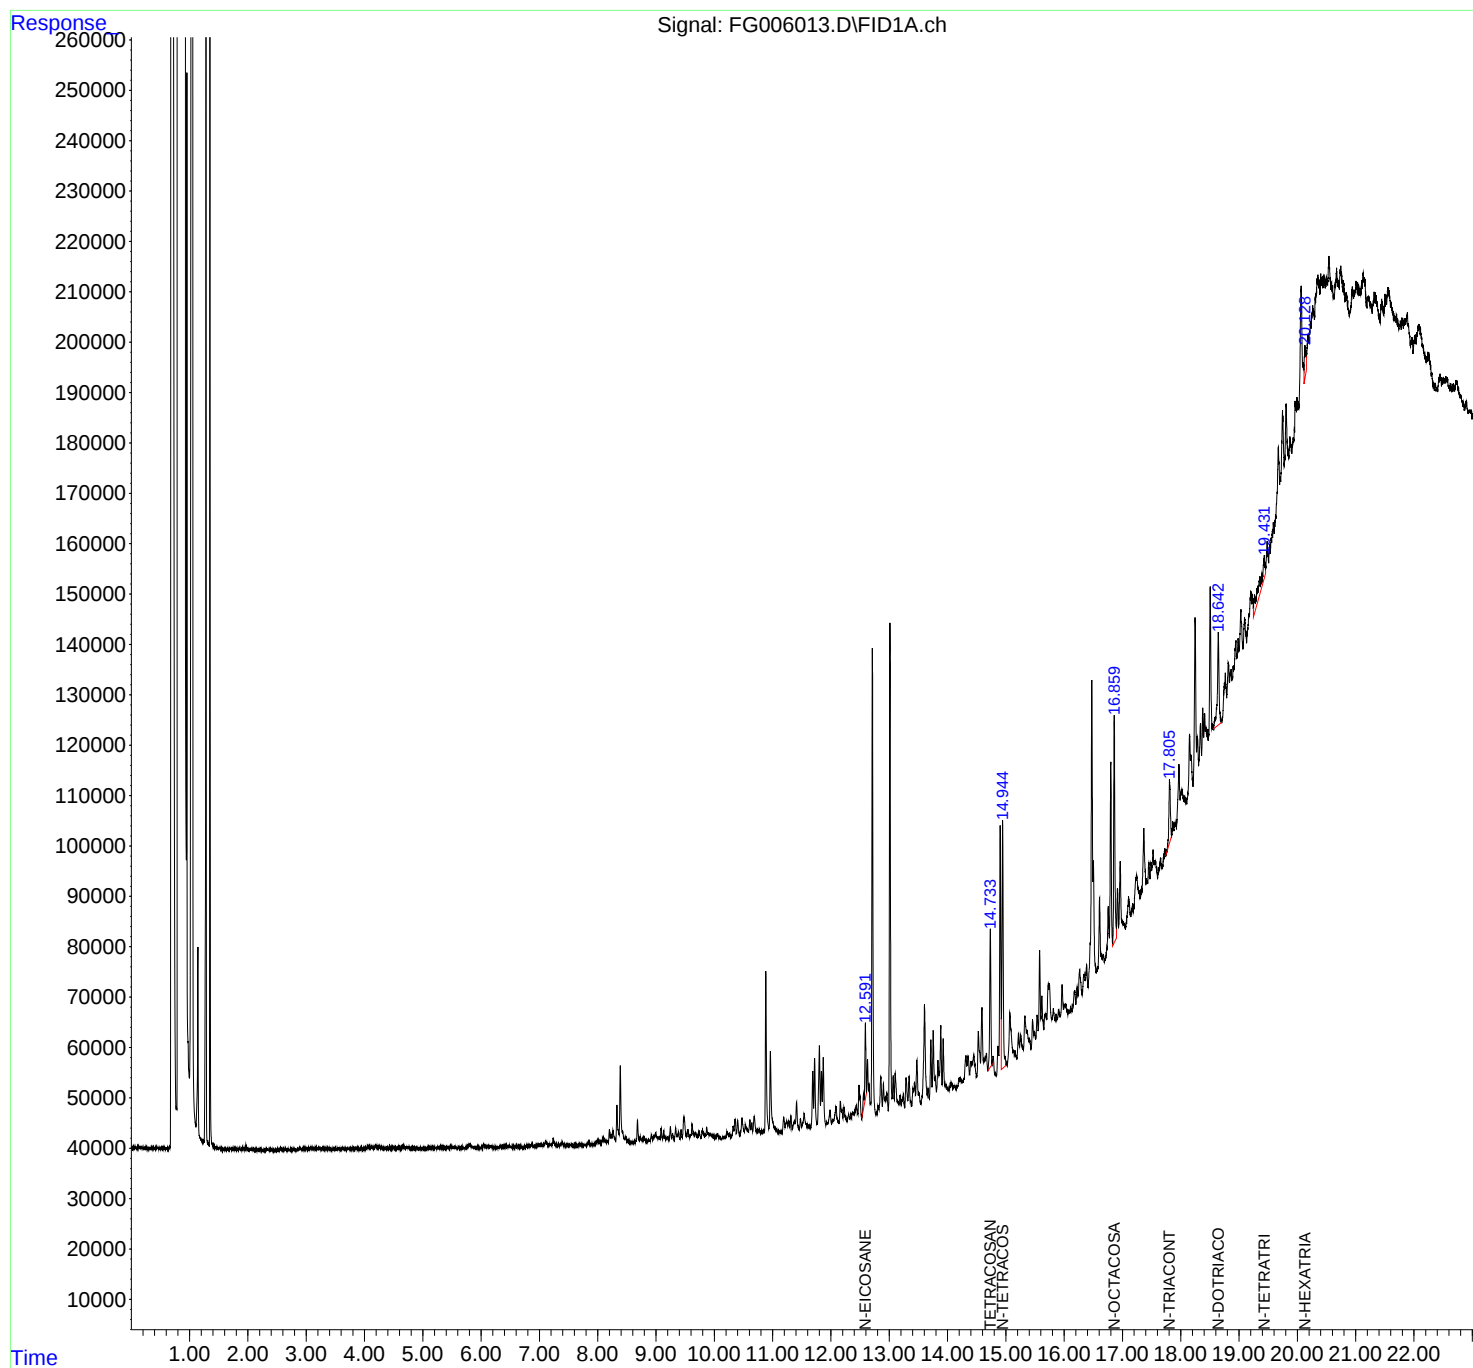


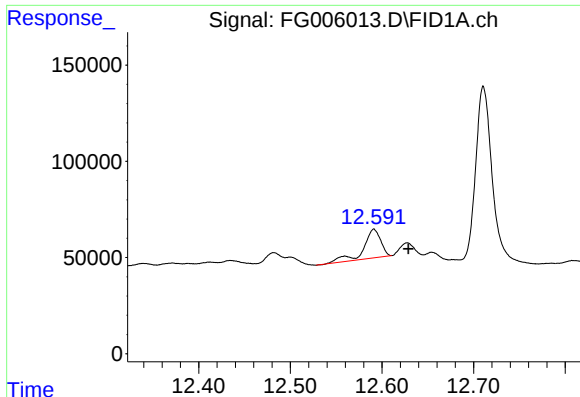

#7 N-EICOSANE


R.T.: 12.591 min
Delta R.T.: -0.037 min
Response: 196418
Conc: 1.45 ug/ml

Instrument :
FID_G
ClientSampleId :
CL-02-091819

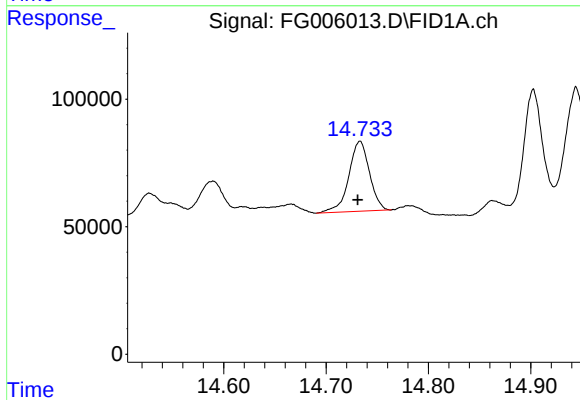


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.733 min
Delta R.T.: 0.002 min
Response: 384269
Conc: 3.42 ug/ml

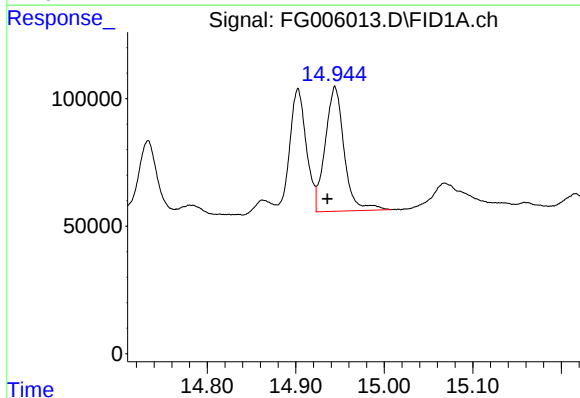


#10 N-TETRACOSANE

R.T.: 14.944 min
Delta R.T.: 0.009 min
Response: 726122
Conc: 5.69 ug/ml

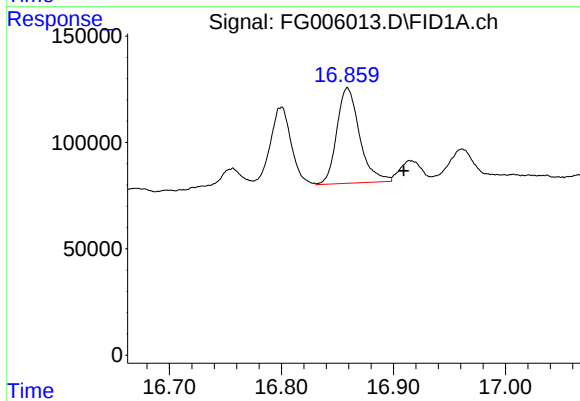

#12 N-OCTACOSANE


R.T.: 16.859 min
Delta R.T.: -0.050 min
Response: 634475
Conc: 5.38 ug/ml

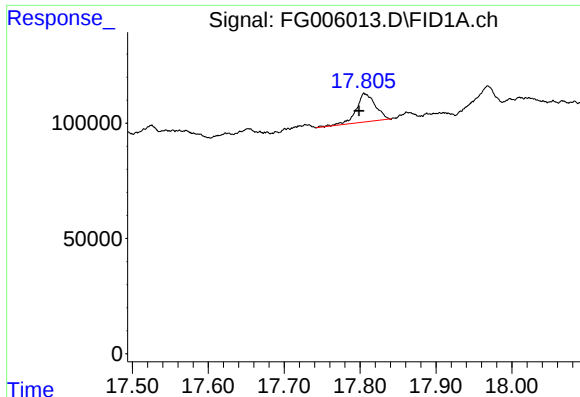

#13 N-TRIACONTANE


R.T.: 17.807 min
Delta R.T.: 0.008 min
Response: 215562
Conc: 1.90 ug/ml

Instrument :
FID_G
ClientSampleId :
CL-02-091819

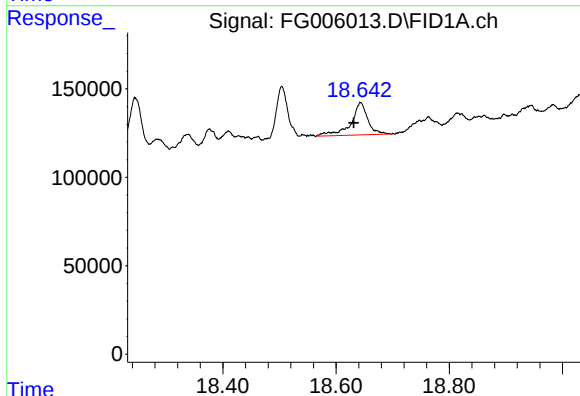


#14 N-DOTRIACONTANE

R.T.: 18.643 min
Delta R.T.: 0.012 min
Response: 374948
Conc: 3.50 ug/ml

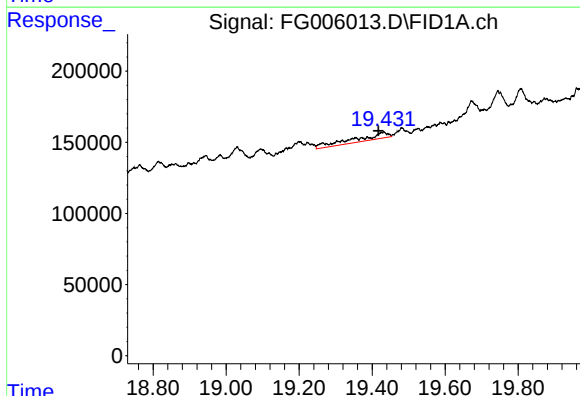

#15 N-TETRATRIACONTANE

R.T.: 19.431 min
Delta R.T.: 0.014 min
Response: 291920
Conc: 2.82 ug/ml

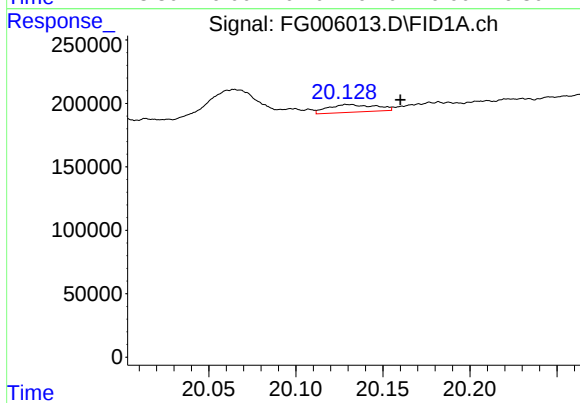

#16 N-HEXATRIACONTANE

R.T.: 20.130 min
Delta R.T.: -0.030 min
Response: 115684
Conc: 1.16 ug/ml