

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG091919\
Data File : FG006016.D
Signal(s) : FID1A.ch
Acq On : 19 Sep 2019 15:53
Operator : DD\AJ
Sample : K4669-04 20X
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
TR-04-091719

Integration File: autoint1.e
Quant Time: Sep 20 01:46:00 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG090719.M
Quant Title :
QLast Update : Mon Sep 09 05:03:58 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
10)	N-TETRACOSANE	14.940	660207	5.177 ug/ml
13)	N-TRIACONTANE	17.813	419404	3.701 ug/ml
15)	N-TETRATRIACONTANE	19.428	124848	1.207 ug/ml
16)	N-HEXATRIACONTANE	20.102f	283606	2.847 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG091919\
Data File : FG006016.D
Signal(s) : FID1A.ch
Acq On : 19 Sep 2019 15:53
Operator : DD\AJ
Sample : K4669-04 20X
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
TR-04-091719

Integration File: autoint1.e
Quant Time: Sep 20 01:46:00 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG090719.M
Quant Title :
QLast Update : Mon Sep 09 05:03:58 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

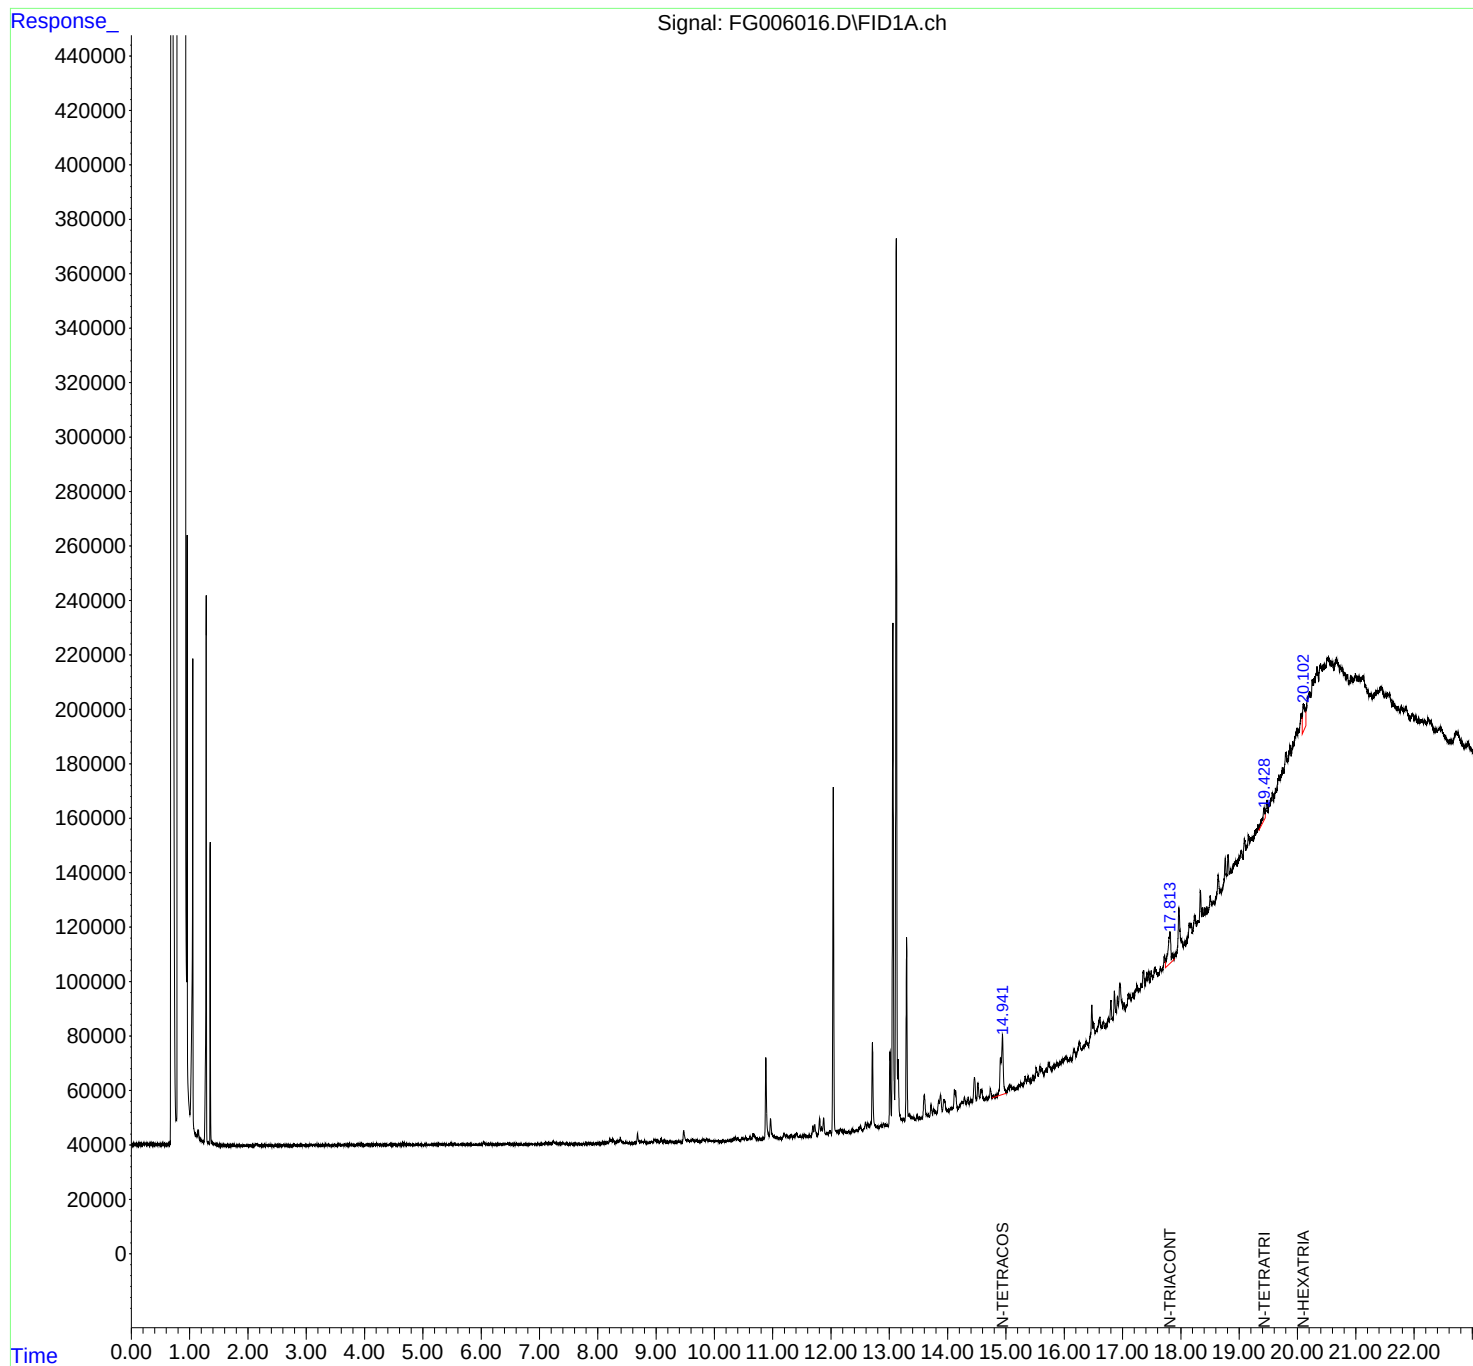


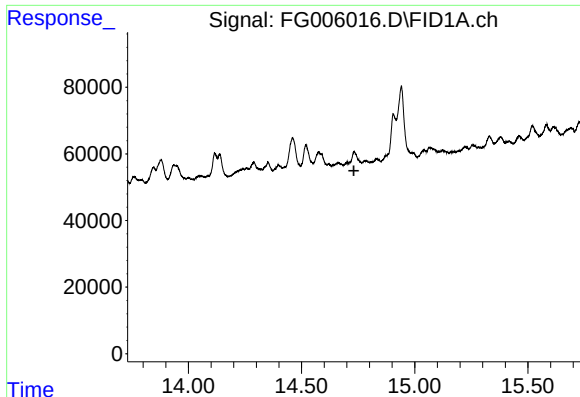

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 0.000 min
Exp R.T.: 14.731 min
Response: 0
Conc: N.D.

Instrument :
FID_G
ClientSampleId :
TR-04-091719

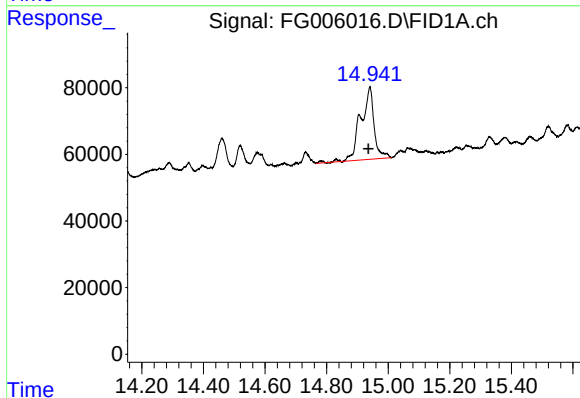


#10 N-TETRACOSANE

R.T.: 14.940 min
Delta R.T.: 0.005 min
Response: 660207
Conc: 5.18 ug/ml

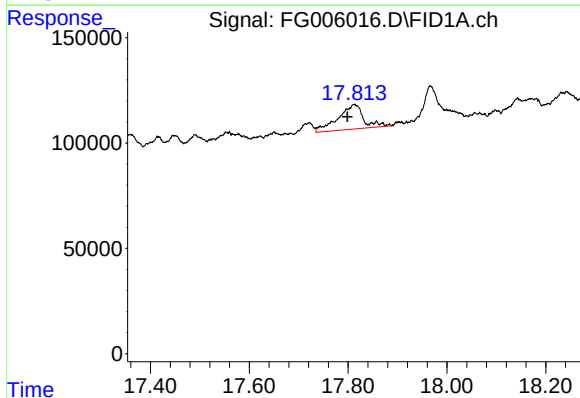


#13 N-TRIACONTANE

R.T.: 17.813 min
Delta R.T.: 0.014 min
Response: 419404
Conc: 3.70 ug/ml

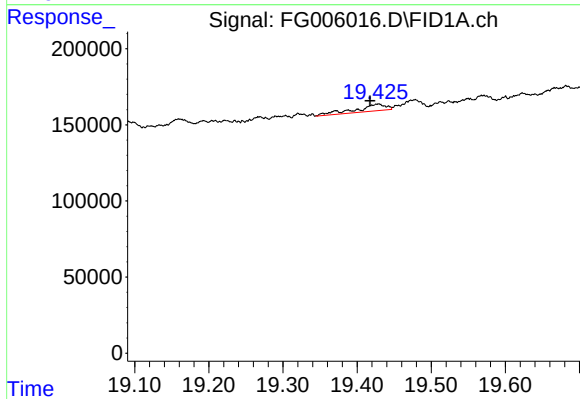

#15 N-TETRATRIACONTANE

R.T.: 19.428 min
Delta R.T.: 0.010 min
Response: 124848
Conc: 1.21 ug/ml

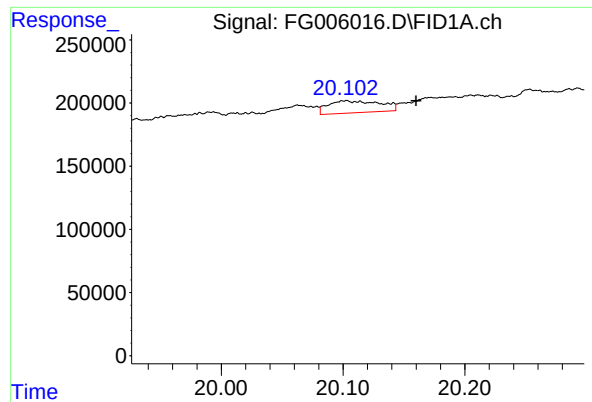

#16 N-HEXATRIACONTANE

R.T.: 20.102 min
Delta R.T.: -0.058 min
Response: 283606
Conc: 2.85 ug/ml

Instrument :
FID_G
ClientSampleId :
TR-04-091719