

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG091919\
Data File : FG006013.D
Signal(s) : FID1A.ch
Acq On : 19 Sep 2019 14:25
Operator : DD\AJ
Sample : K4662-09 5X
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
CL-02-091819

Integration File: autoint1.e
Quant Time: Sep 20 01:45:20 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG090719.M
Quant Title :
QLast Update : Mon Sep 09 05:03:58 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.733	384269	3.420 ug/ml
Target Compounds			

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG091919\
Data File : FG006013.D
Signal(s) : FID1A.ch
Acq On : 19 Sep 2019 14:25
Operator : DD\AJ
Sample : K4662-09 5X
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
CL-02-091819

Integration File: autoint1.e
Quant Time: Sep 20 01:45:20 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG090719.M
Quant Title :
QLast Update : Mon Sep 09 05:03:58 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

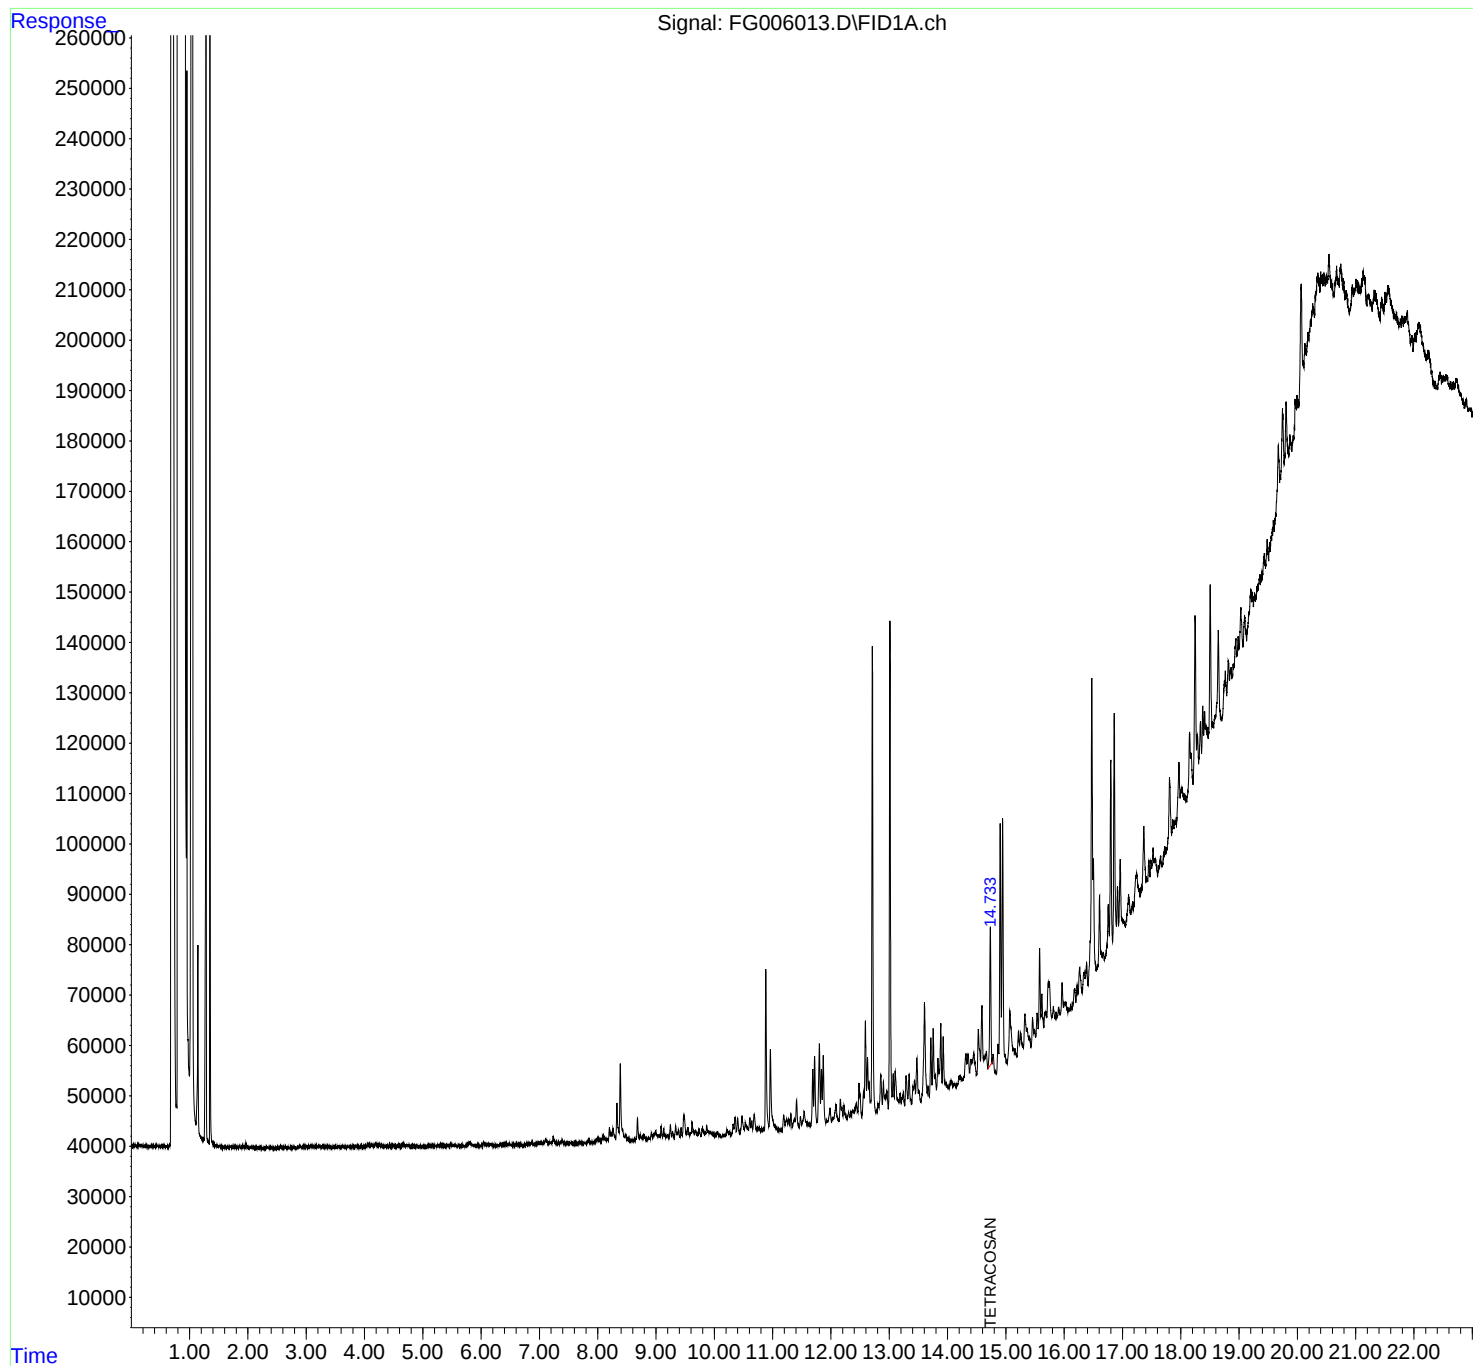

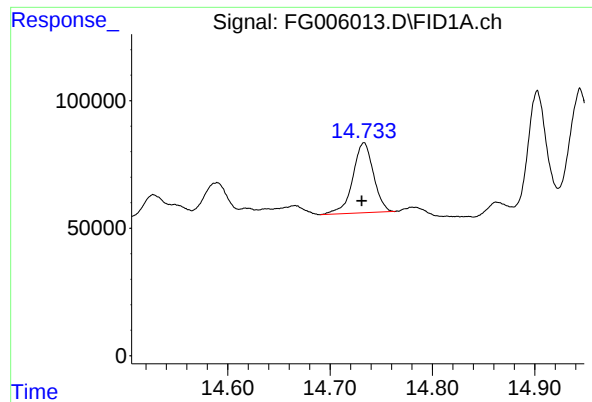

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.733 min
Delta R.T.: 0.002 min
Response: 384269
Conc: 3.42 ug/ml

Instrument :
FID_G
ClientSampleId :
CL-02-091819