

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG091924AL\
Data File : FG014271.D
Signal(s) : FID1A.ch
Acq On : 19 Sep 2024 06:13
Operator : YP\AJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Sep 20 01:11:15 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\Aliphatic EPH 091124.M
Quant Title : GC Extractables
QLast Update : Wed Sep 11 07:16:16 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
14) T	n-Tetracosane (C24)	15.094	176547	1.483 ug/ml
18) T	n-Dotriacontane (C32)	18.836	82762	0.744 ug/ml
20) T	n-Hexatriacontane (C36)	20.360	73844	0.827 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG091924AL\
Data File : FG014271.D
Signal(s) : FID1A.ch
Acq On : 19 Sep 2024 06:13
Operator : YP\AJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Sep 20 01:11:15 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\Aliphatic EPH 091124.M
Quant Title : GC Extractables
QLast Update : Wed Sep 11 07:16:16 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

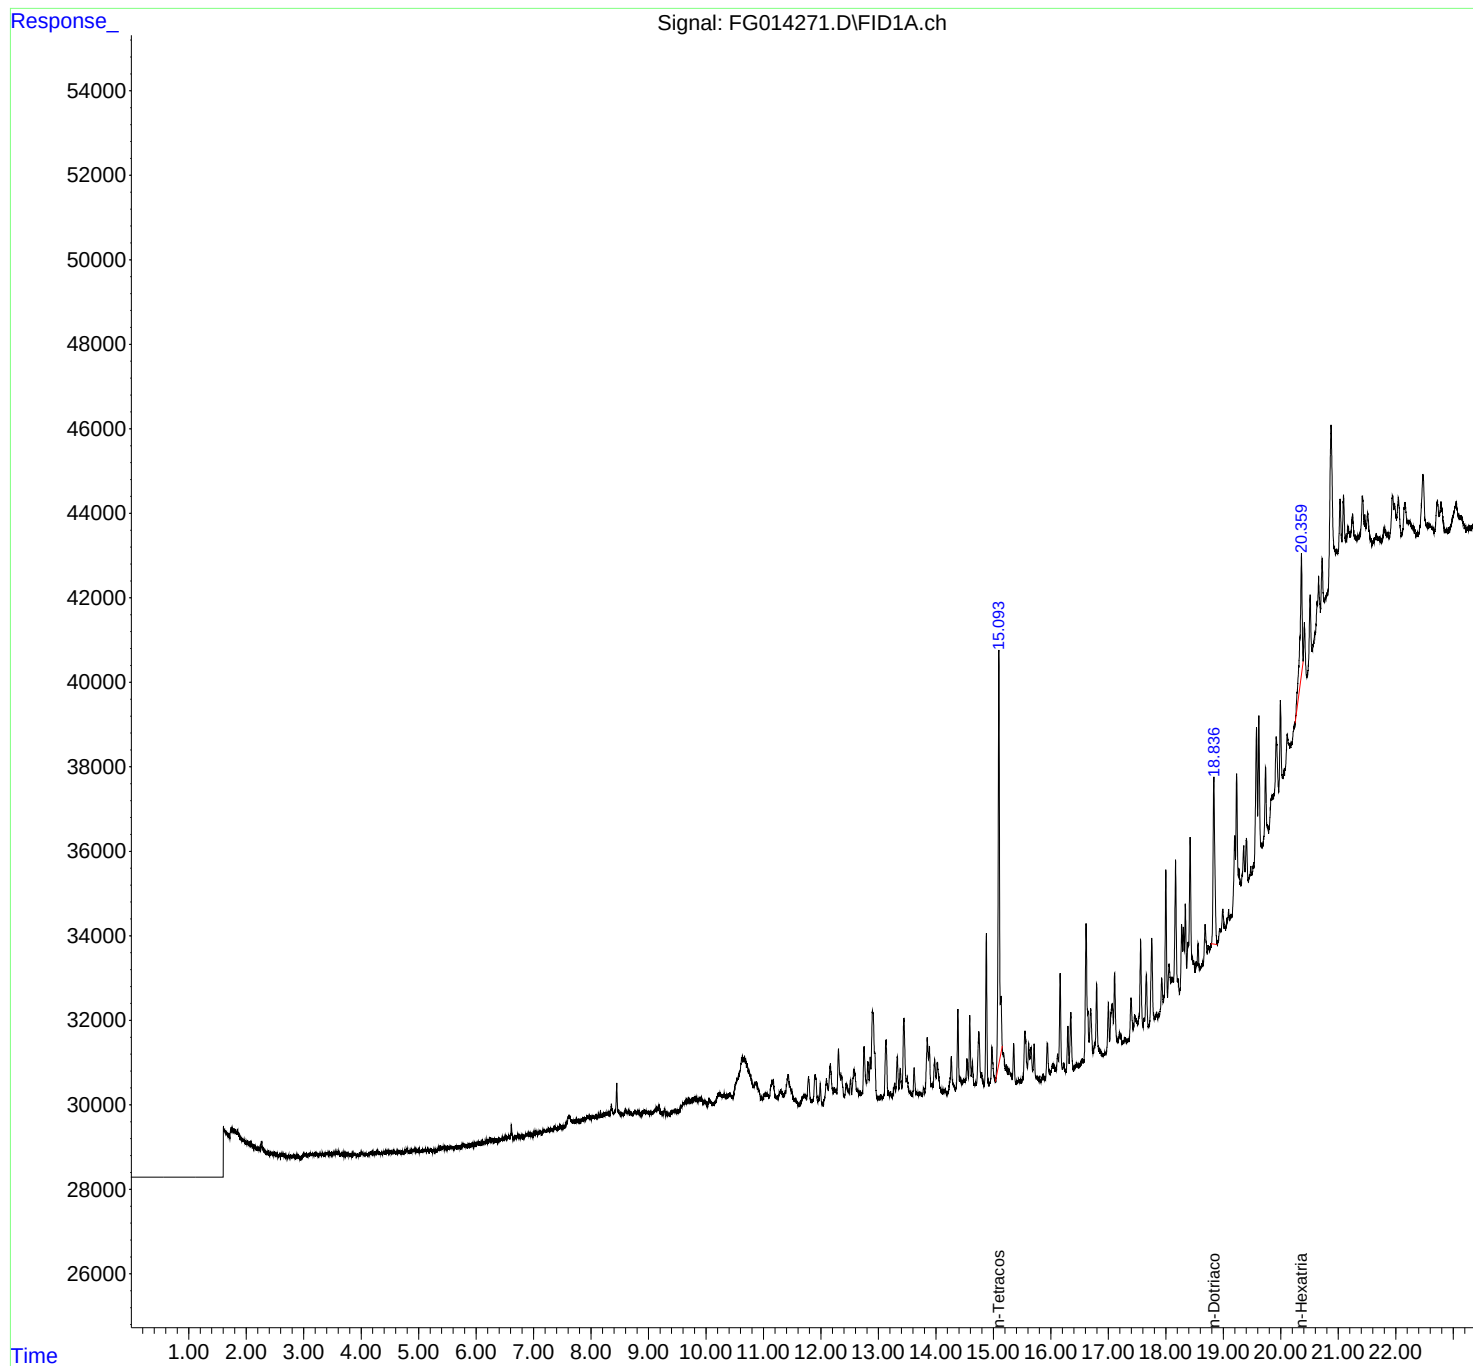


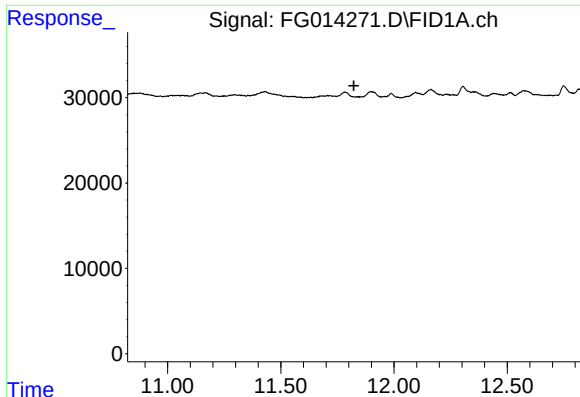

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T. : 11.823 min
Response: 0
Conc: N.D.

Instrument :
FID_G
ClientSampleId :

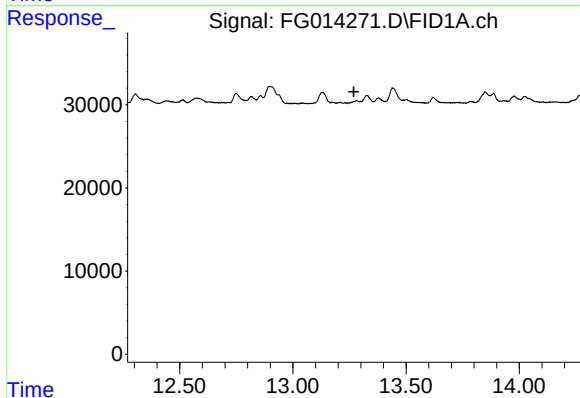


#12 1-chlorooctadecane (SURR)

R.T.: 0.000 min
Exp R.T. : 13.269 min
Response: 0
Conc: N.D.

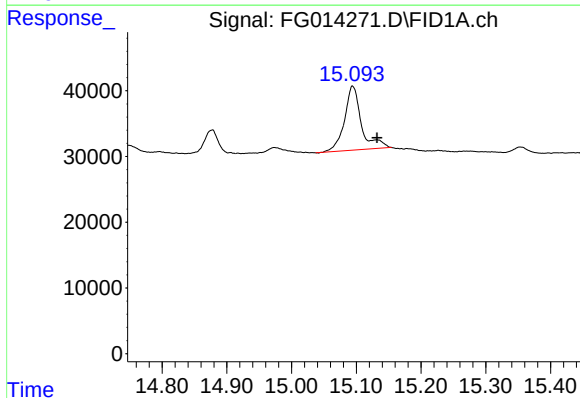


#14 n-Tetracosane (C24)

R.T.: 15.094 min
Delta R.T.: -0.038 min
Response: 176547
Conc: 1.48 ug/ml

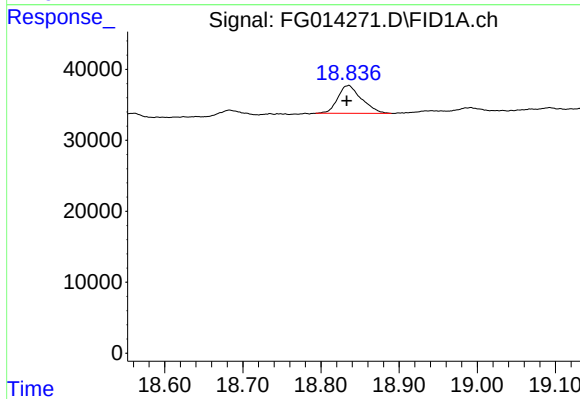

#18 n-Dotriacontane (C32)

R.T.: 18.836 min
Delta R.T.: 0.003 min
Response: 82762
Conc: 0.74 ug/ml

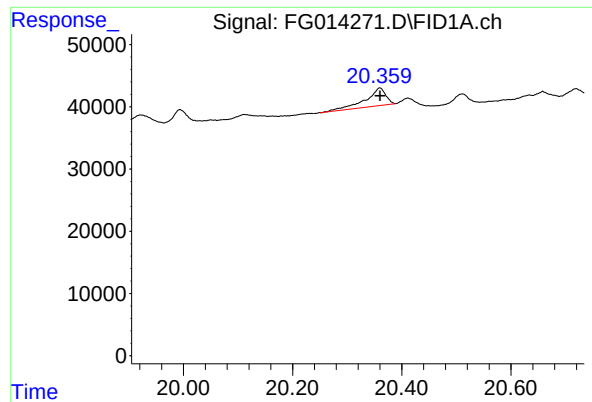

#20 n-Hexatriacontane (C36)

R.T.: 20.360 min
Delta R.T.: 0.000 min
Response: 73844
Conc: 0.83 ug/ml

Instrument :

FID_G

ClientSampleId :