

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG092022\
 Data File : FG010628.D
 Signal(s) : FID1A.ch
 Acq On : 20 Sep 2022 13:40
 Operator : YP\AJ
 Sample : N4702-01
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :
 BU-03-091622

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 09/21/2022
 Supervised By :Ankita Jodhani 09/21/2022

Integration File: Sample.e
 Quant Time: Sep 21 03:56:53 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG082622.M
 Quant Title :
 QLast Update : Fri Aug 26 23:48:05 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.783	2295423	18.756 ug/mlm
Target Compounds			

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG092022\
Data File : FG010628.D
Signal(s) : FID1A.ch
Acq On : 20 Sep 2022 13:40
Operator : YP\AJ
Sample : N4702-01
Misc :
ALS Vial : 7 Sample Multiplier: 1


Instrument :
FID_G
ClientSampleId :
BU-03-091622


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/21/2022
Supervised By :Ankita Jodhani 09/21/2022

Integration File: Sample.e
Quant Time: Sep 21 03:56:53 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG082622.M
Quant Title :
QLast Update : Fri Aug 26 23:48:05 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

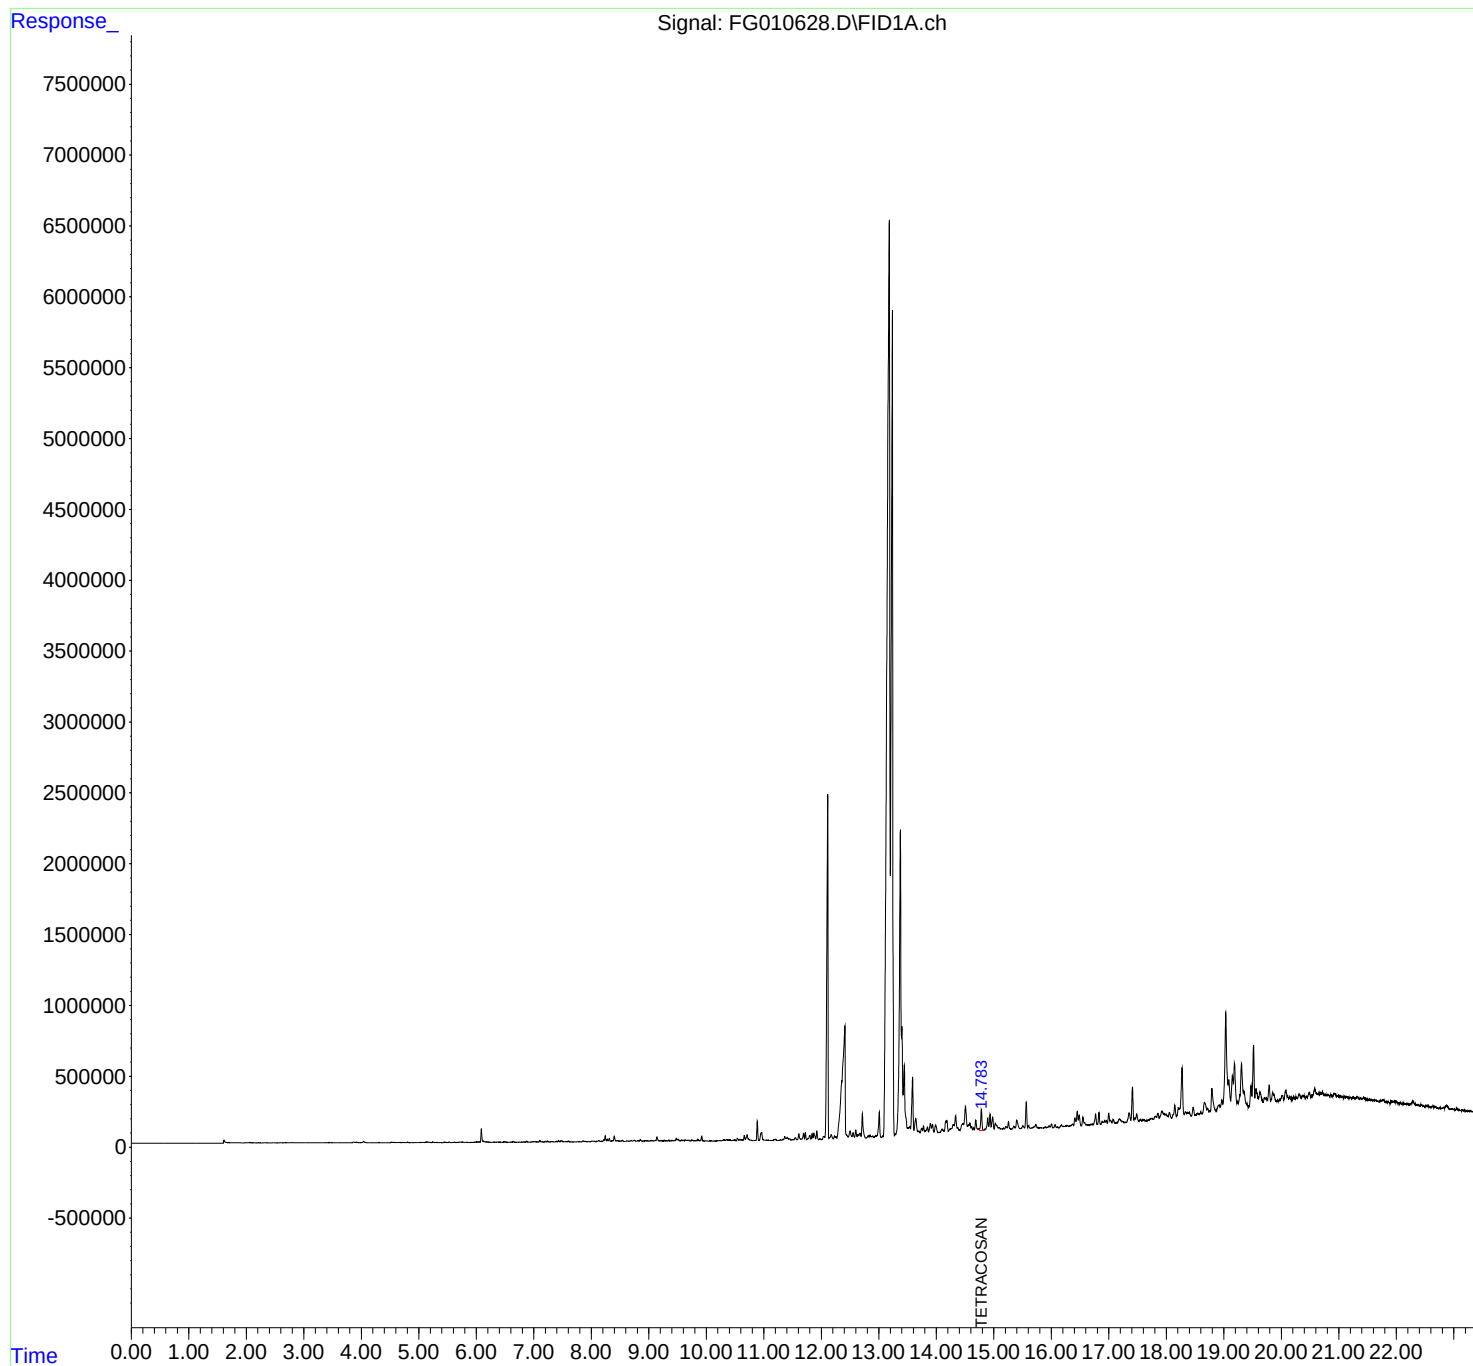

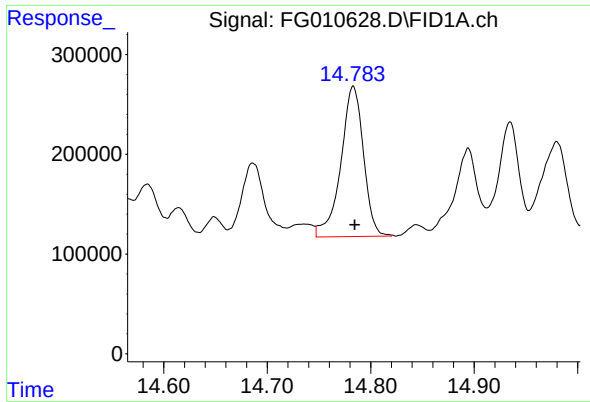

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.783 min
Delta R.T.: -0.002 min
Response: 2295423
Conc: 18.76 ug/ml

Instrument :
FID_G
ClientSampleId :
BU-03-091622

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/21/2022
Supervised By :Ankita Jodhani 09/21/2022