

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG092022\
Data File : FG010629.D
Signal(s) : FID1A.ch
Acq On : 20 Sep 2022 14:19
Operator : YP\AJ
Sample : N4702-01 20X
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
BU-03-091622

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/21/2022
Supervised By :Ankita Jodhani 09/21/2022

Integration File: Sample.e
Quant Time: Sep 21 04:29:22 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG082622.M
Quant Title :
QLast Update : Fri Aug 26 23:48:05 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.778	79846	0.652 ug/mlm
Target Compounds			

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG092022\
Data File : FG010629.D
Signal(s) : FID1A.ch
Acq On : 20 Sep 2022 14:19
Operator : YP\AJ
Sample : N4702-01 20X
Misc :
ALS Vial : 8 Sample Multiplier: 1


Instrument :
FID_G
ClientSampleId :
BU-03-091622


Manual Integrations
APPROVED

Reviewed By : Yogesh Patel 09/21/2022
Supervised By : Ankita Jodhani 09/21/2022

Integration File: Sample.e
Quant Time: Sep 21 04:29:22 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG082622.M
Quant Title :
QLast Update : Fri Aug 26 23:48:05 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

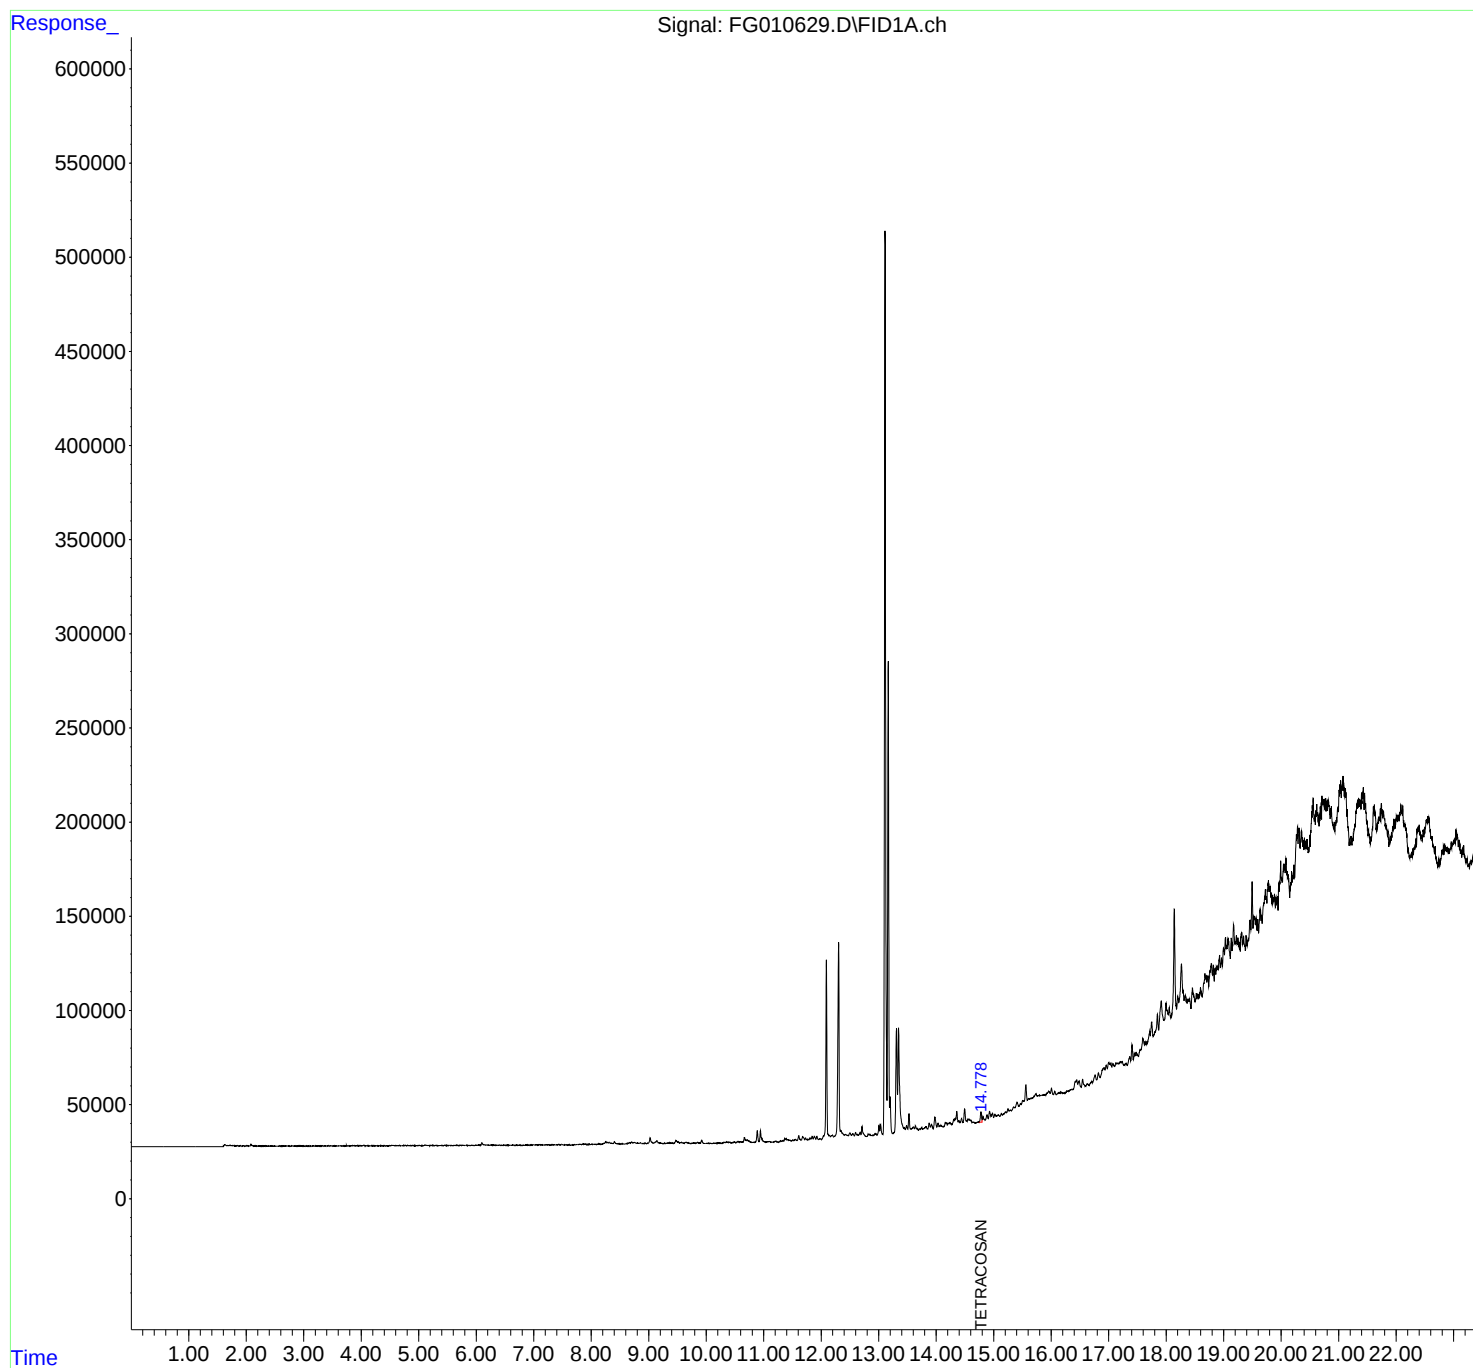

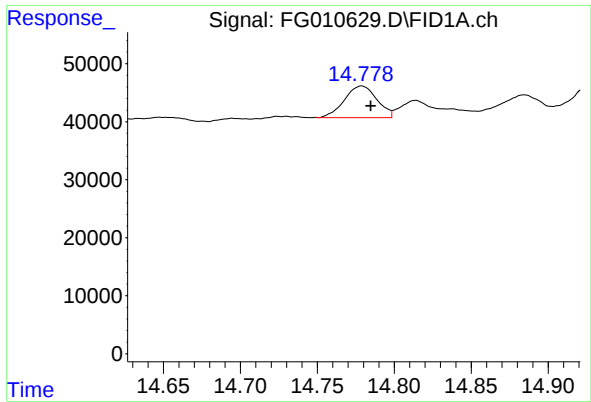

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.778 min
Delta R.T.: -0.006 min
Response: 79846
Conc: 0.65 ug/ml

Instrument :
FID_G
ClientSampleId :
BU-03-091622

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/21/2022
Supervised By :Ankita Jodhani 09/21/2022