

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG092024AR\
Data File : FG014297.D
Signal(s) : FID1A.ch
Acq On : 20 Sep 2024 07:29
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
I.BLK

Integration File: autoint1.e
Quant Time: Sep 21 03:12:28 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\Aromatic EPH 090424.M
Quant Title : GC Extractables
QLast Update : Wed Sep 04 11:28:29 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18µm

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
19) T	Indeno[1,2,3-cd]pyren...	18.428	32115	0.325 ug/ml
20) T	Dibenz[a,h]anthracene...	18.428	32115	0.218 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG092024AR\
Data File : FG014297.D
Signal(s) : FID1A.ch
Acq On : 20 Sep 2024 07:29
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
I.BLK

Integration File: autoint1.e
Quant Time: Sep 21 03:12:28 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\Aromatic EPH 090424.M
Quant Title : GC Extractables
QLast Update : Wed Sep 04 11:28:29 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18µm

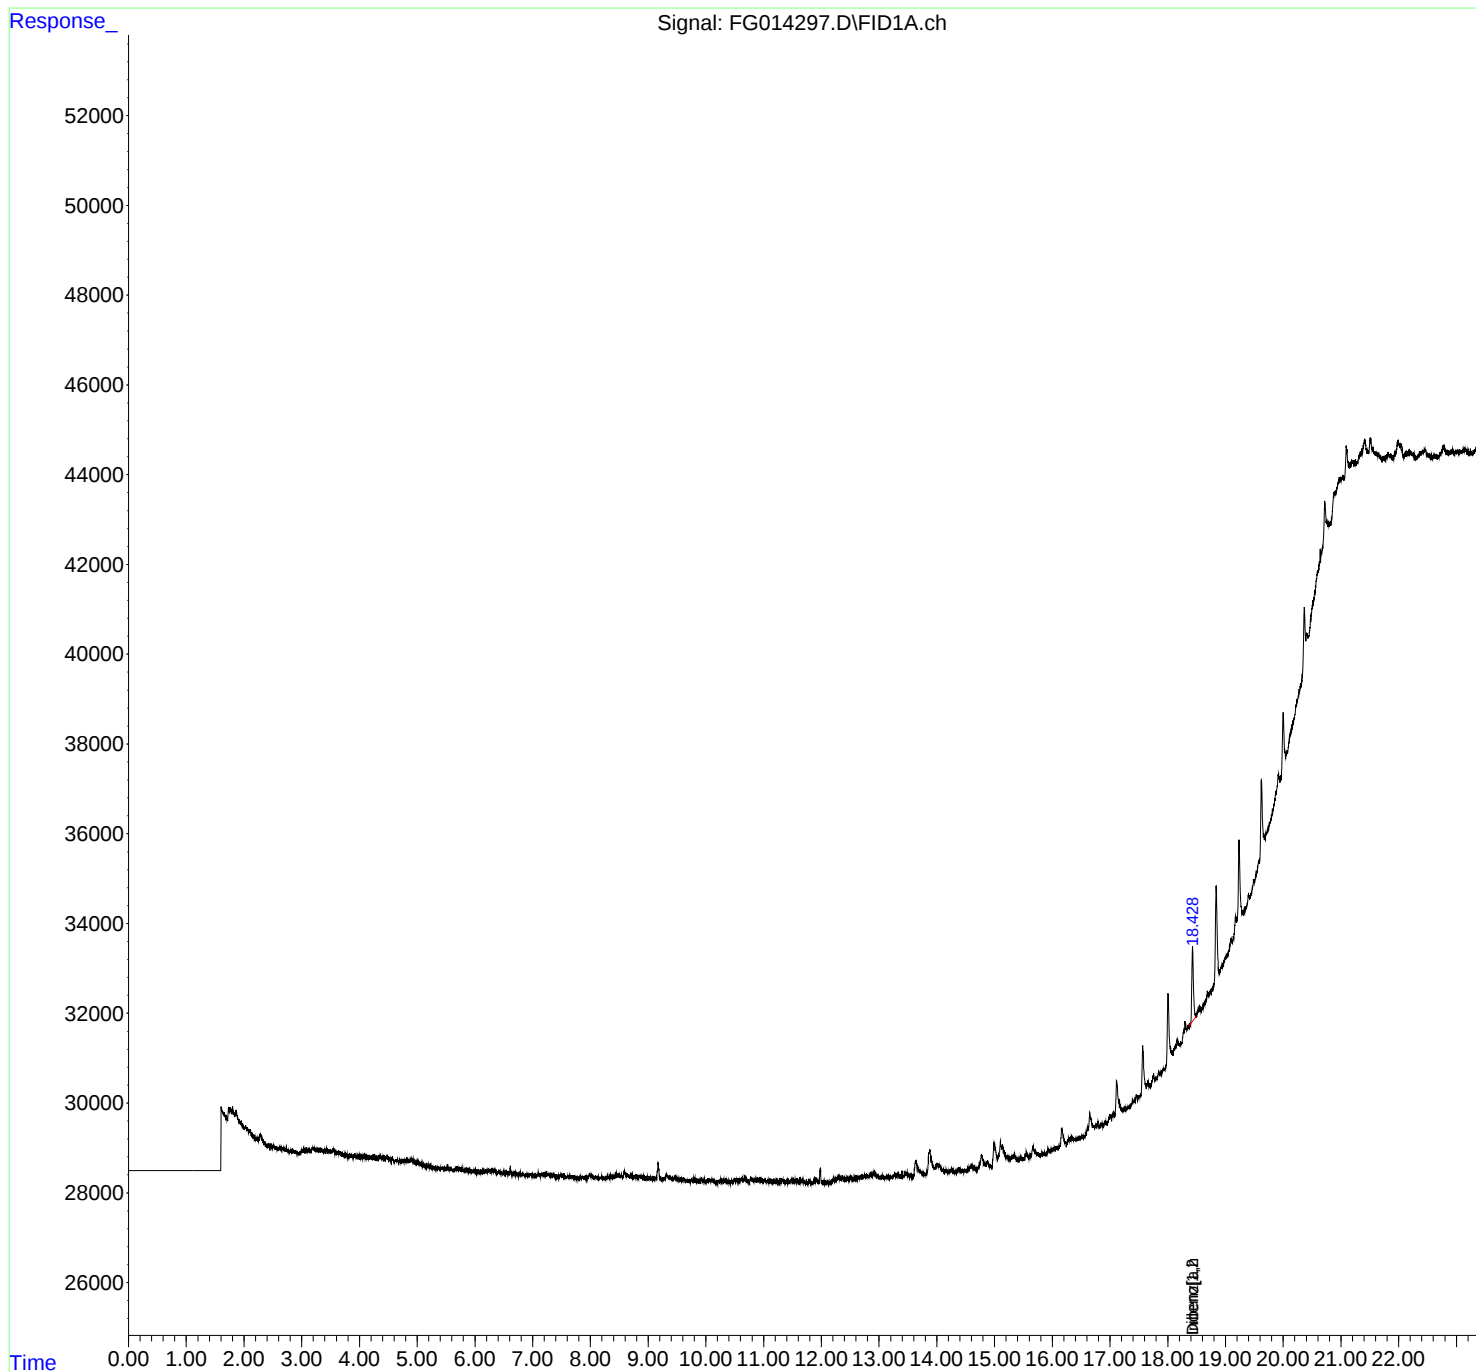


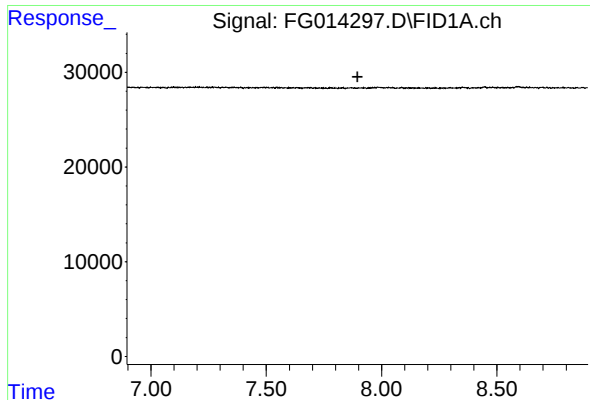

#4 2-Bromonaphthalene (SURR)


R.T.: 0.000 min
Exp R.T.: 7.895 min
Response: 0
Conc: N.D.

Instrument :
FID_G
ClientSampleId :
I.BLK

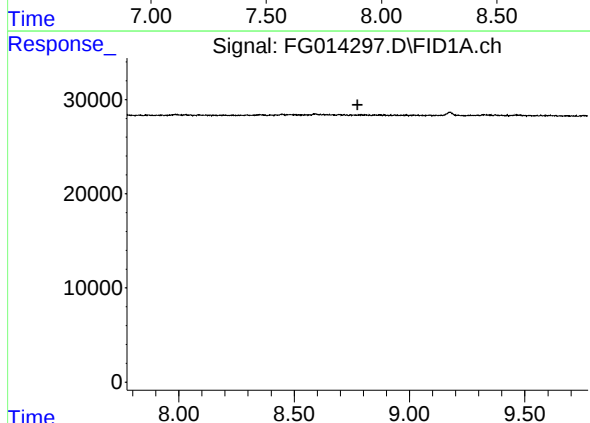


#6 2-Fluorobiphenyl (SURR)

R.T.: 0.000 min
Exp R.T.: 8.775 min
Response: 0
Conc: N.D.

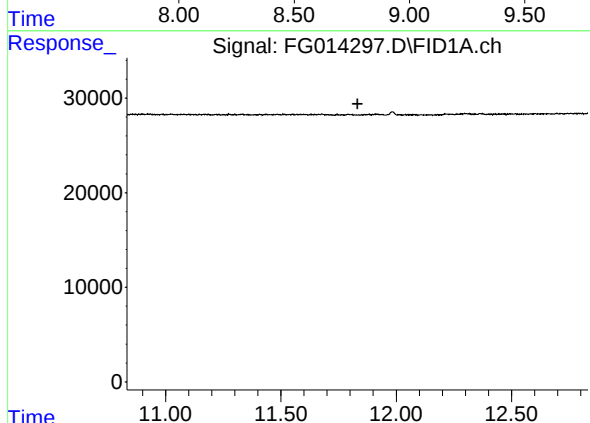


#11 ortho-Terphenyl (SURR)

R.T.: 0.000 min
Exp R.T.: 11.832 min
Response: 0
Conc: N.D.

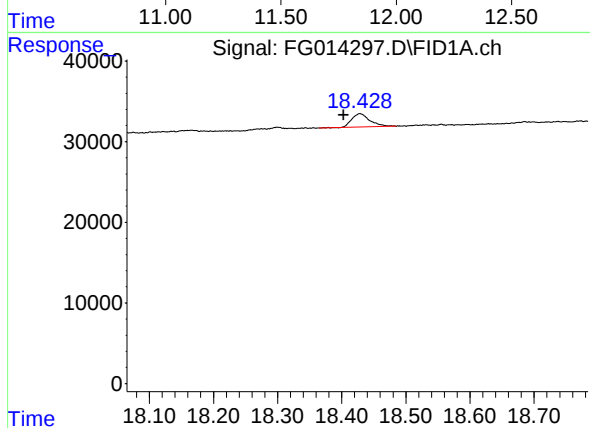

#19 Indeno[1,2,3-cd]pyrene (C35.01)

R.T.: 18.428 min
Delta R.T.: 0.025 min
Response: 32115
Conc: 0.32 ug/ml

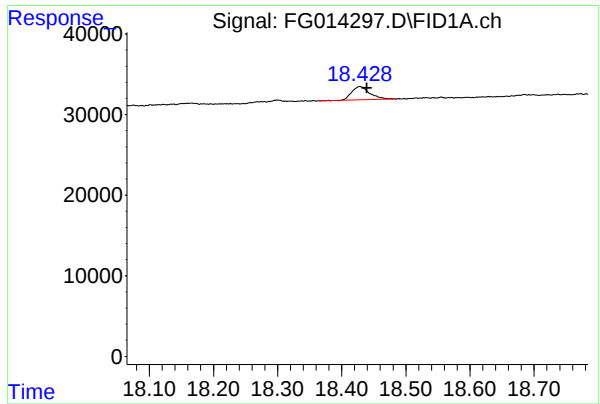

#20 Dibenz[a,h]anthracene (C30.36)

R.T.: 18.428 min

Delta R.T.: -0.011 min

Response: 32115

Conc: 0.22 ug/ml

Instrument :

FID_G

ClientSampleId :

I.BLK