

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG092118\
 Data File : FG002349.D
 Signal(s) : FID1A.ch
 Acq On : 21 Sep 2018 13:12
 Operator : AJ\SJ
 Sample : PB113088BS
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Integration File: Sample.e
 Quant Time: Sep 21 23:36:03 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG083018.M
 Quant Title :
 QLast Update : Thu Aug 30 14:49:31 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.418	2310988	18.318 ug/ml
Target Compounds			
2) N-DECANE	4.180	2526192	21.046 ug/ml
3) N-DODECANE	6.190	2696105	21.424 ug/ml
4) N-TETRADECANE	7.980	2767866	21.084 ug/ml
5) N-HEXADECANE	9.576	2801441	20.582 ug/ml
6) N-OCTADECANE	11.015	2821822	20.089 ug/ml
7) N-EICOSANE	12.323	2798549	19.699 ug/ml
8) N-DOCOSANE	13.519	2768743	19.400 ug/ml
10) N-TETRACOSANE	14.621	2731372	19.106 ug/ml
11) N-HEXACOSANE	15.641	2677323	18.647 ug/ml
12) N-OCTACOSANE	16.590	2645023	18.078 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG092118\
Data File : FG002349.D
Signal(s) : FID1A.ch
Acq On : 21 Sep 2018 13:12
Operator : AJ\SJ
Sample : PB113088BS
Misc :
ALS Vial : 6 Sample Multiplier: 1

Integration File: Sample.e
Quant Time: Sep 21 23:36:03 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG083018.M
Quant Title :
QLast Update : Thu Aug 30 14:49:31 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

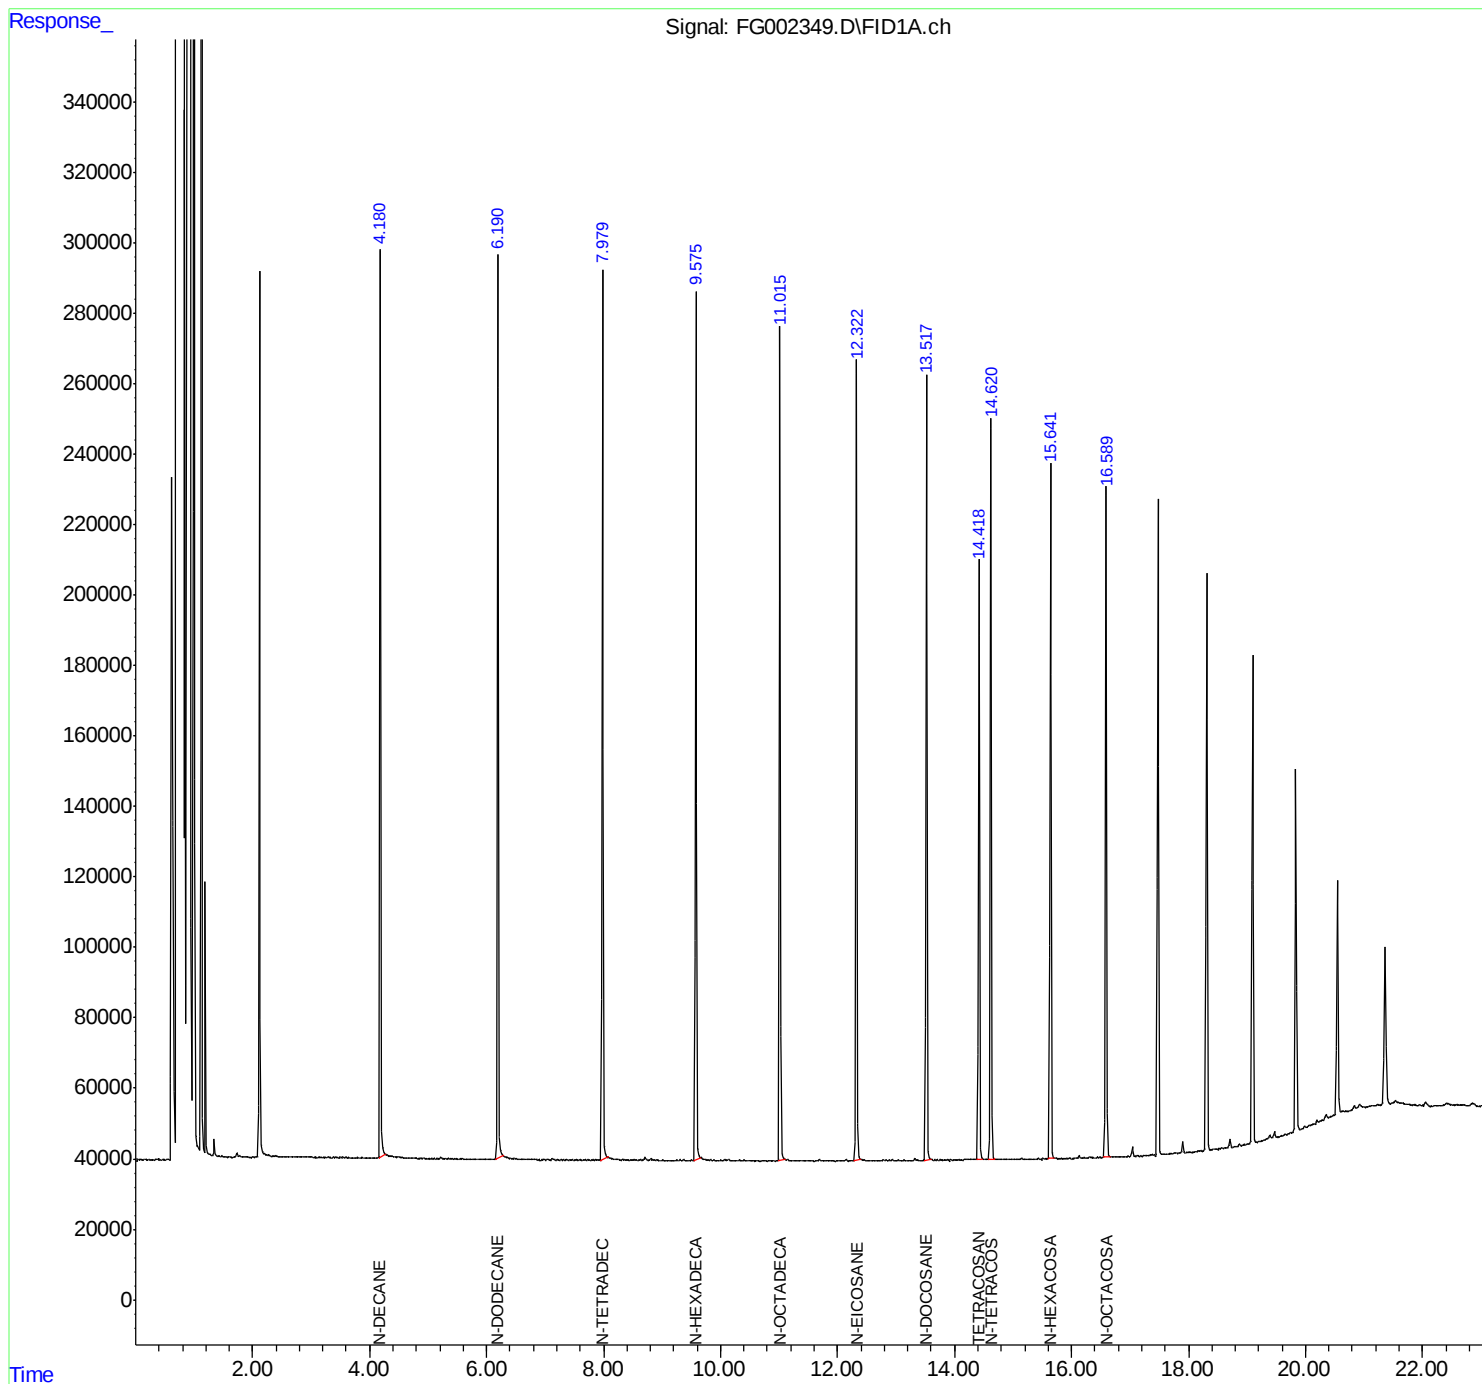

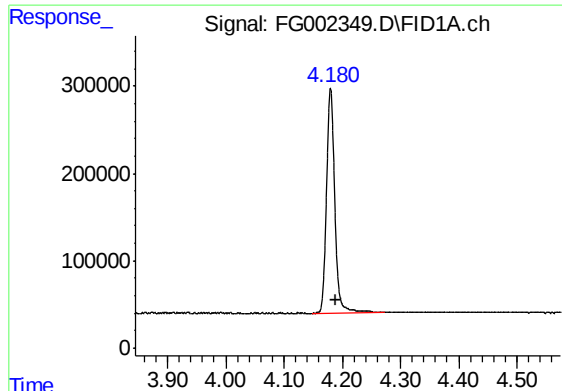


#2 N-DECANE

R.T.: 4.180 min
Delta R.T.: -0.009 min
Response: 2526192
Conc: 21.05 ug/ml

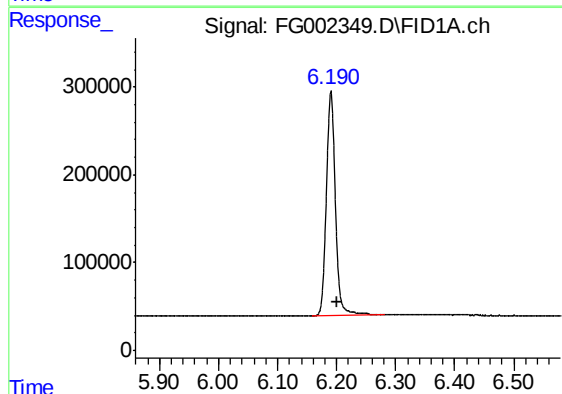


#3 N-DODECANE

R.T.: 6.190 min
Delta R.T.: -0.010 min
Response: 2696105
Conc: 21.42 ug/ml

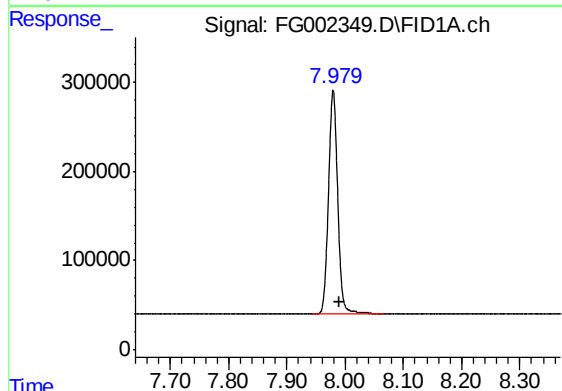


#4 N-TETRADECANE

R.T.: 7.980 min
Delta R.T.: -0.010 min
Response: 2767866
Conc: 21.08 ug/ml

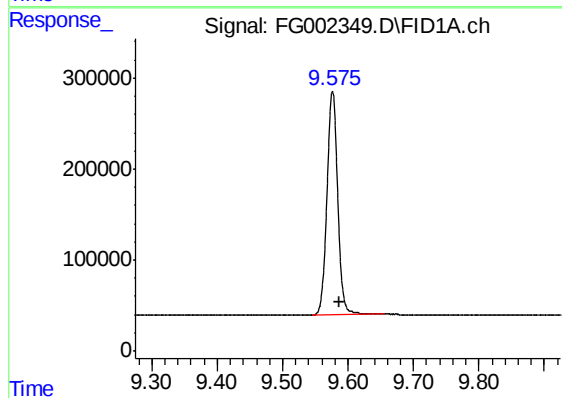


#5 N-HEXADECANE

R.T.: 9.576 min
Delta R.T.: -0.011 min
Response: 2801441
Conc: 20.58 ug/ml

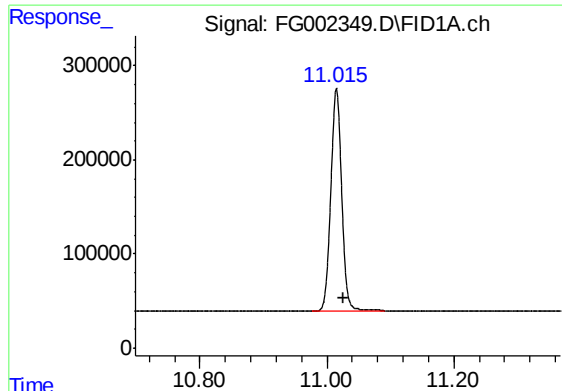


#6 N-OCTADECANE

R.T.: 11.015 min
Delta R.T.: -0.010 min
Response: 2821822
Conc: 20.09 ug/ml

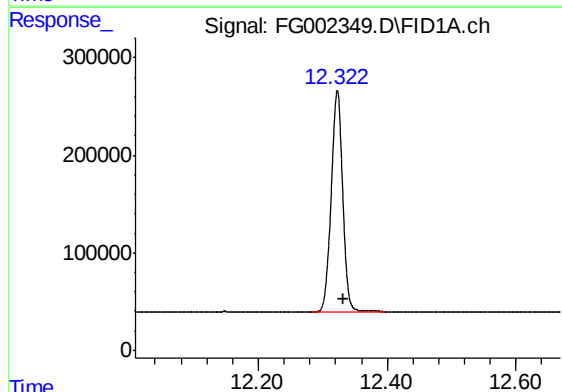


#7 N-EICOSANE

R.T.: 12.323 min
Delta R.T.: -0.009 min
Response: 2798549
Conc: 19.70 ug/ml

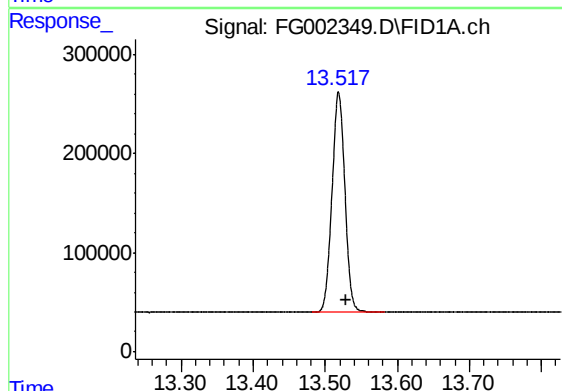


#8 N-DOCOSANE

R.T.: 13.519 min
Delta R.T.: -0.011 min
Response: 2768743
Conc: 19.40 ug/ml

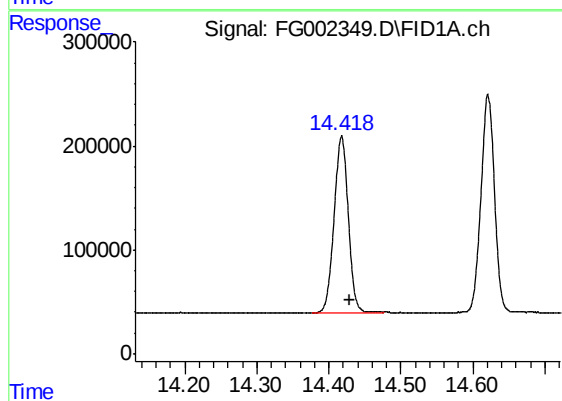


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.418 min
Delta R.T.: -0.011 min
Response: 2310988
Conc: 18.32 ug/ml

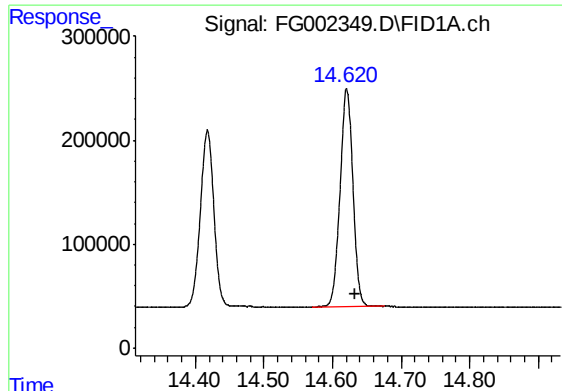


#10 N-TETRACOSANE

R.T.: 14.621 min
Delta R.T.: -0.011 min
Response: 2731372
Conc: 19.11 ug/ml

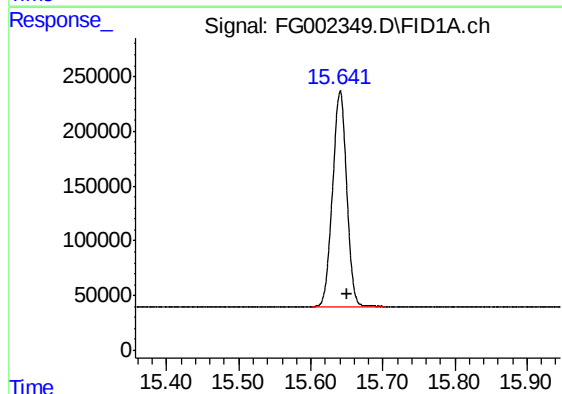

#11 N-HEXACOSANE

R.T.: 15.641 min
Delta R.T.: -0.010 min
Response: 2677323
Conc: 18.65 ug/ml

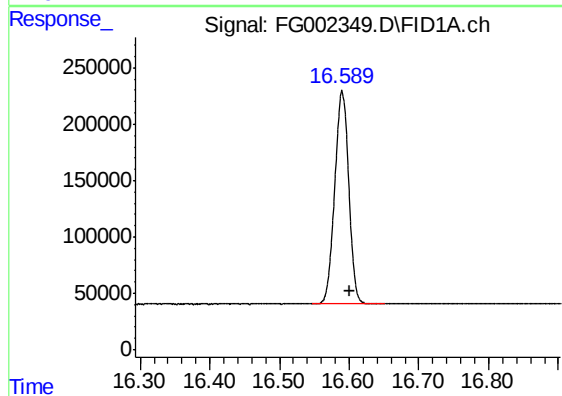

#12 N-OCTACOSANE

R.T.: 16.590 min
Delta R.T.: -0.010 min
Response: 2645023
Conc: 18.08 ug/ml