

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG092322\
Data File : FG010669.D
Signal(s) : FID1A.ch
Acq On : 23 Sep 2022 11:28
Operator : YP\AJ
Sample : RT MARKER
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
RT MARKER

Integration File: autoint1.e
Quant Time: Sep 24 14:30:25 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG082622.M
Quant Title :
QLast Update : Fri Aug 26 23:48:05 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
3) N-DODECANE	6.480	2593281	19.704 ug/ml
12) N-OCTACOSANE	16.947	2382802	18.018 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG092322\
Data File : FG010669.D
Signal(s) : FID1A.ch
Acq On : 23 Sep 2022 11:28
Operator : YP\AJ
Sample : RT MARKER
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
RT MARKER

Integration File: autoint1.e
Quant Time: Sep 24 14:30:25 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG082622.M
Quant Title :
QLast Update : Fri Aug 26 23:48:05 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

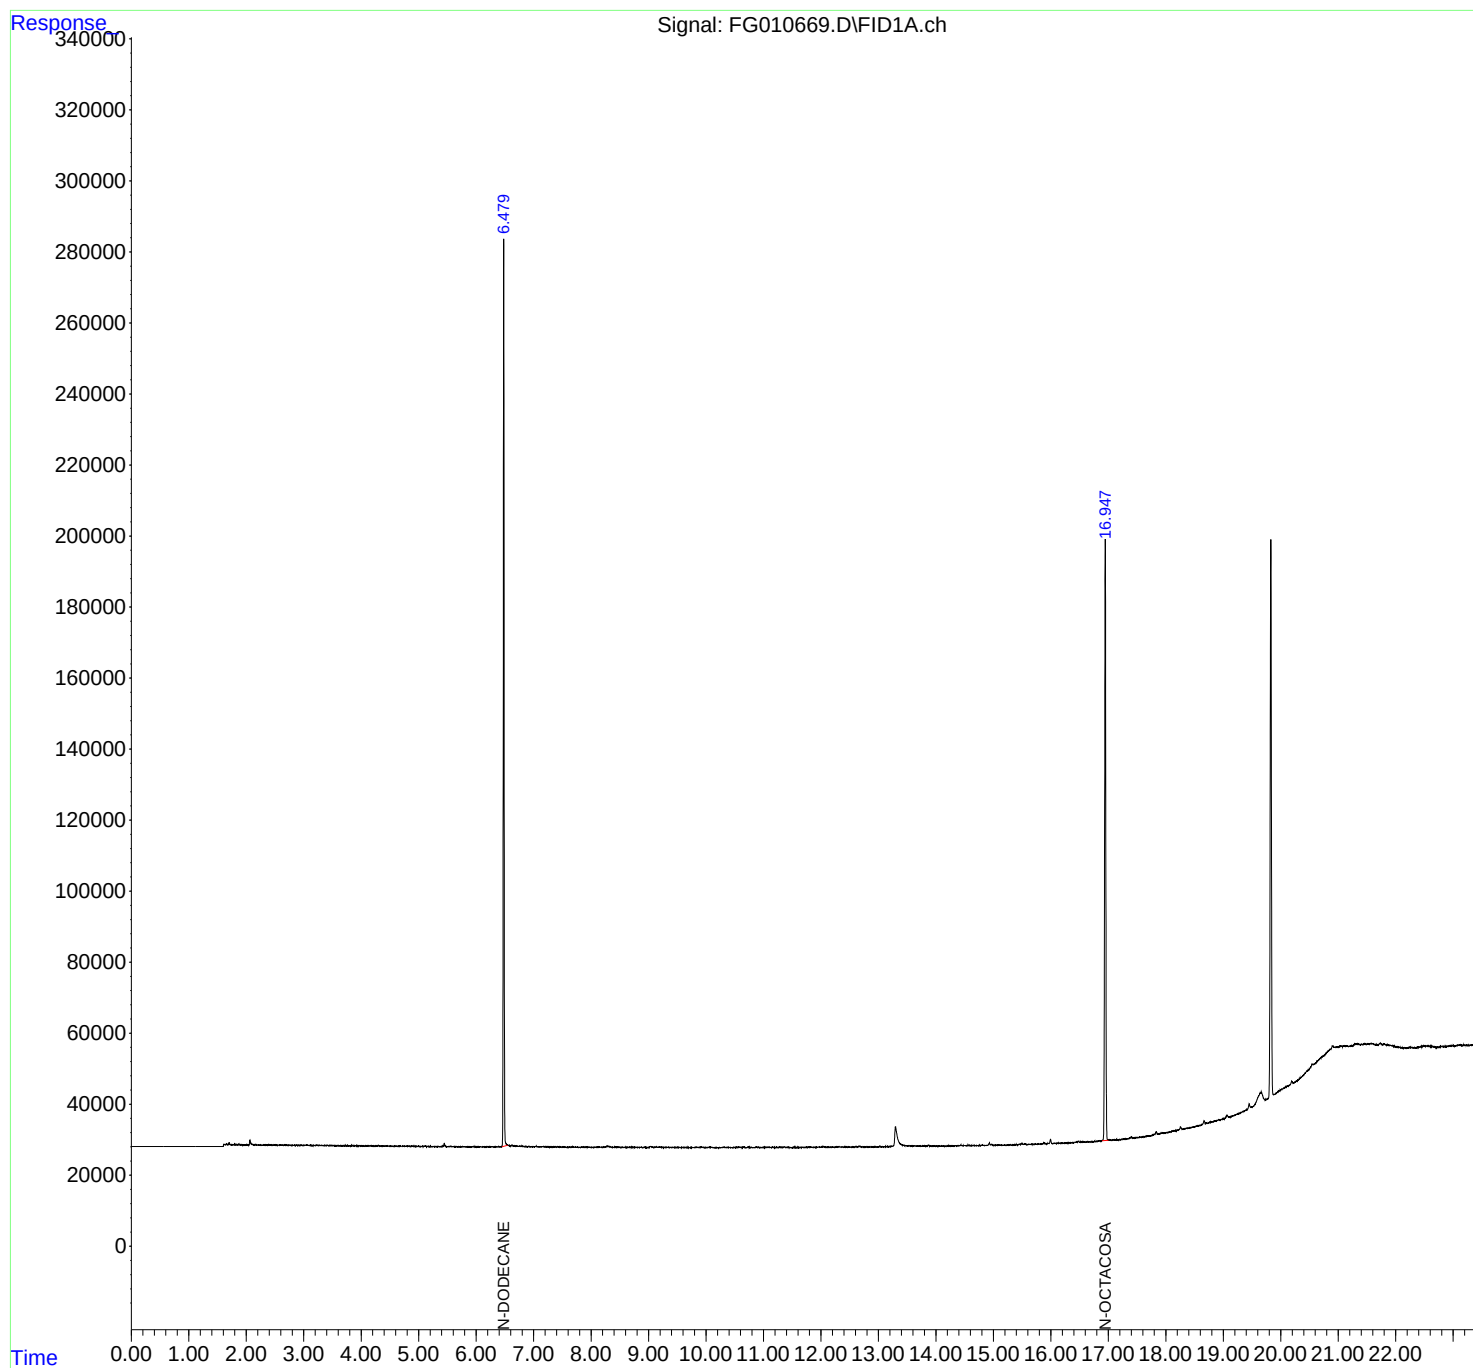


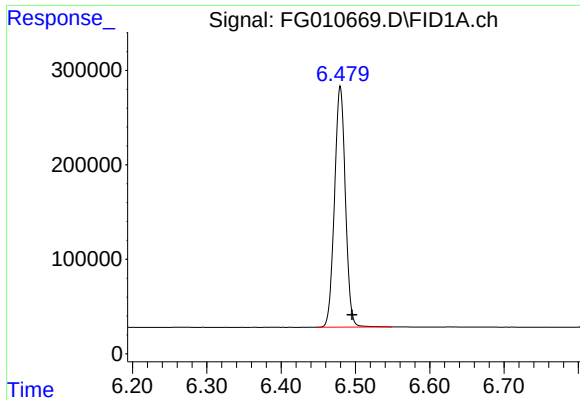

#3 N-DODECANE


R.T.: 6.480 min
Delta R.T.: -0.016 min
Response: 2593281
Conc: 19.70 ug/ml

Instrument :
FID_G
ClientSampleId :
RT MARKER

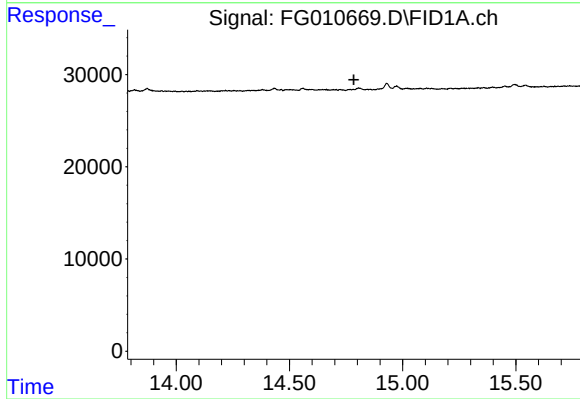

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.785 min
Response: 0
Conc: N.D.

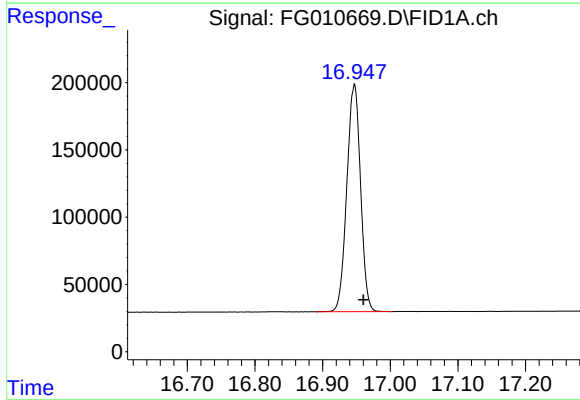

#12 N-OCTACOSANE

R.T.: 16.947 min
Delta R.T.: -0.013 min
Response: 2382802
Conc: 18.02 ug/ml