

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG092518\
 Data File : FG002385.D
 Signal(s) : FID1A.ch
 Acq On : 25 Sep 2018 12:45
 Operator : AJ\SJ
 Sample : J4770-11 25X
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Sep 26 02:31:41 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG083018.M
 Quant Title :
 QLast Update : Thu Aug 30 14:49:31 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
5) N-HEXADECANE	9.573	102984	0.757 ug/ml
6) N-OCTADECANE	11.012	127754	0.910 ug/ml
7) N-EICOSANE	12.319	145806	1.026 ug/ml
8) N-DOCOSANE	13.516	111061	0.778 ug/ml
10) N-TETRACOSANE	14.618	301477	2.109 ug/ml
11) N-HEXACOSANE	15.638	213166	1.485 ug/ml
12) N-OCTACOSANE	16.588	204764	1.399 ug/ml
13) N-TRIACONTANE	17.476	302364	1.993 ug/ml
14) N-DOTRIACONTANE	18.309	251620	1.706 ug/ml
15) N-TETRATRIACONTANE	19.094	186255	1.350 ug/ml
16) N-HEXATRIACONTANE	19.838	88928	0.693 ug/ml
17) N-OCTATRIACONTANE	20.546	95257	0.847 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG092518\
Data File : FG002385.D
Signal(s) : FID1A.ch
Acq On : 25 Sep 2018 12:45
Operator : AJ\SJ
Sample : J4770-11 25X
Misc :
ALS Vial : 5 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Sep 26 02:31:41 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG083018.M
Quant Title :
QLast Update : Thu Aug 30 14:49:31 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

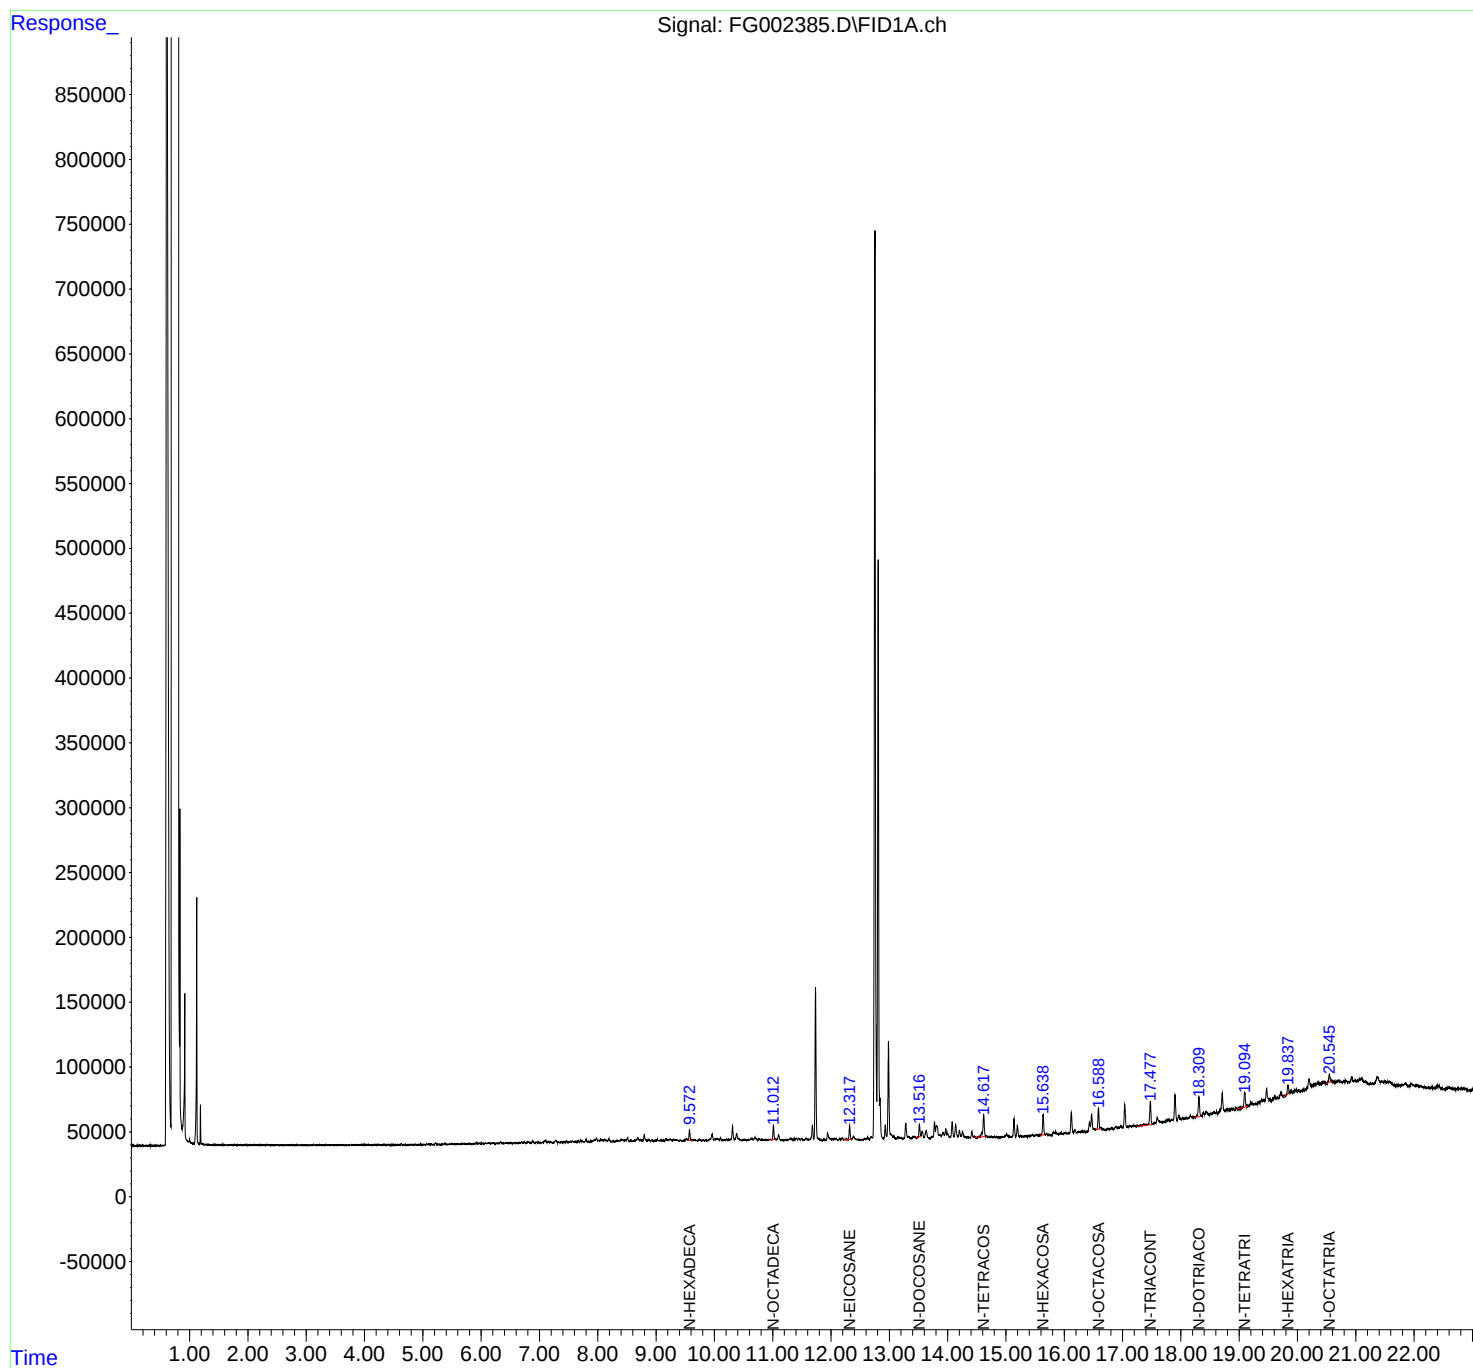

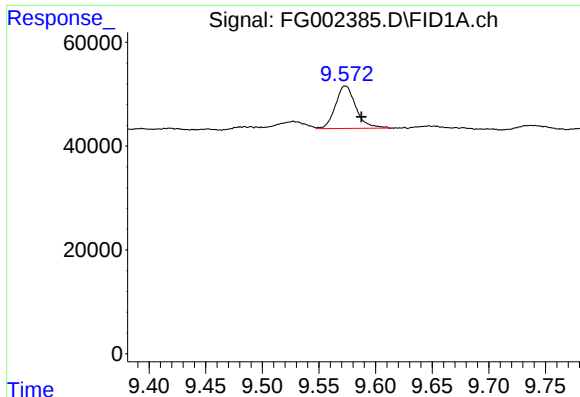


#5 N-HEXADECANE

R.T.: 9.573 min
Delta R.T.: -0.014 min
Response: 102984
Conc: 0.76 ug/ml

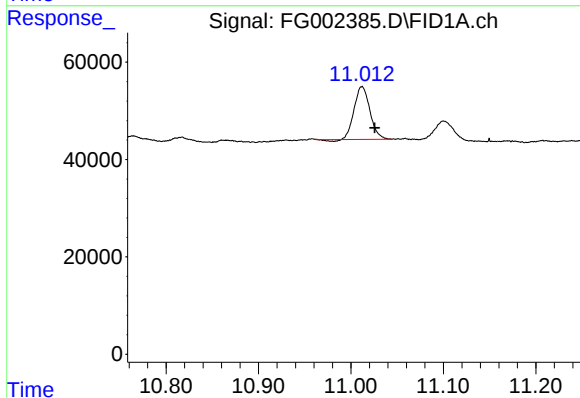


#6 N-OCTADECANE

R.T.: 11.012 min
Delta R.T.: -0.014 min
Response: 127754
Conc: 0.91 ug/ml

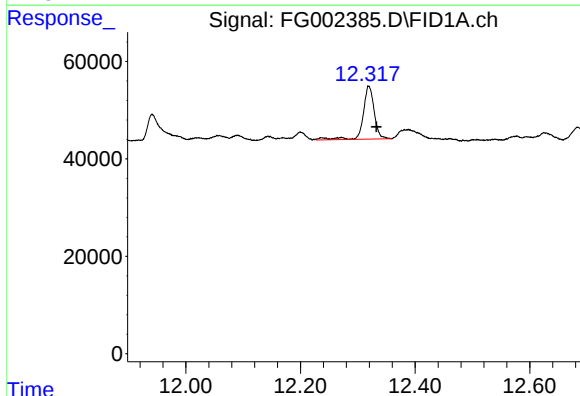


#7 N-EICOSANE

R.T.: 12.319 min
Delta R.T.: -0.013 min
Response: 145806
Conc: 1.03 ug/ml

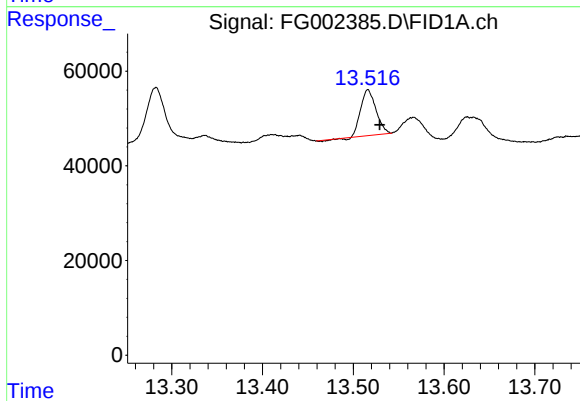


#8 N-DOCOSANE

R.T.: 13.516 min
Delta R.T.: -0.013 min
Response: 111061
Conc: 0.78 ug/ml

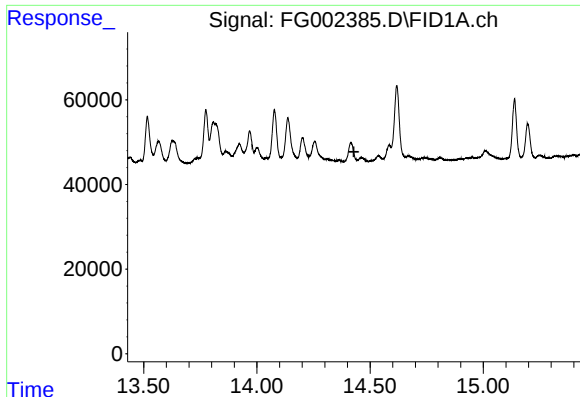


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T.: 14.429 min
Response: 0
Conc: N.D.

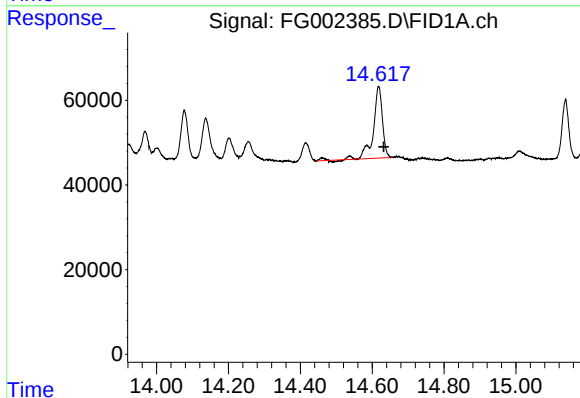


#10 N-TETRACOSANE

R.T.: 14.618 min
Delta R.T.: -0.014 min
Response: 301477
Conc: 2.11 ug/ml

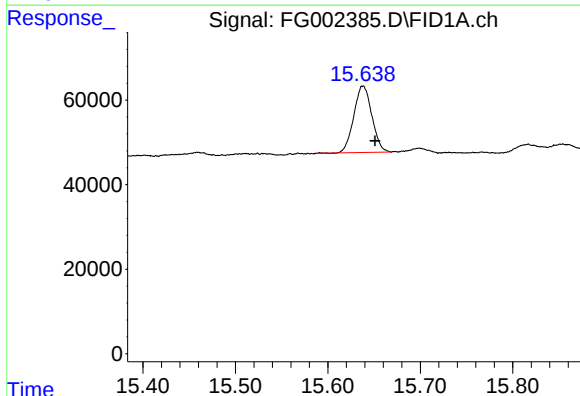


#11 N-HEXACOSANE

R.T.: 15.638 min
Delta R.T.: -0.013 min
Response: 213166
Conc: 1.48 ug/ml

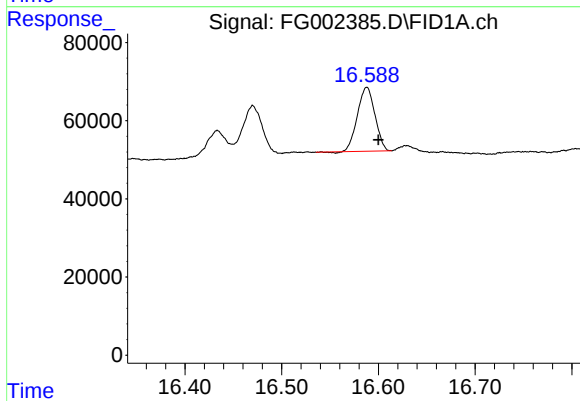


#12 N-OCTACOSANE

R.T.: 16.588 min
Delta R.T.: -0.012 min
Response: 204764
Conc: 1.40 ug/ml

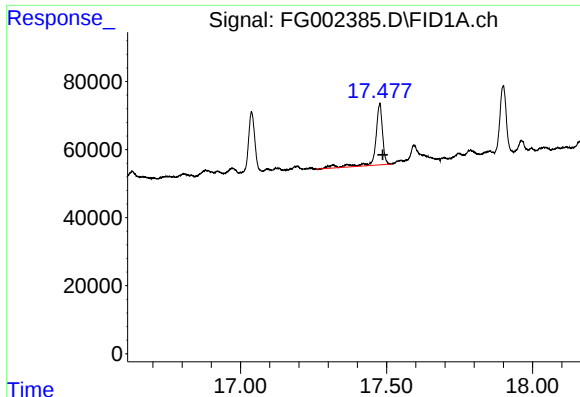


#13 N-TRIACONTANE

R.T.: 17.476 min
Delta R.T.: -0.010 min
Response: 302364
Conc: 1.99 ug/ml

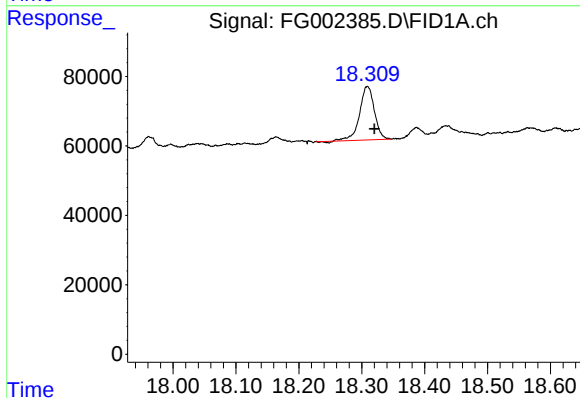


#14 N-DOTRIACONTANE

R.T.: 18.309 min
Delta R.T.: -0.011 min
Response: 251620
Conc: 1.71 ug/ml

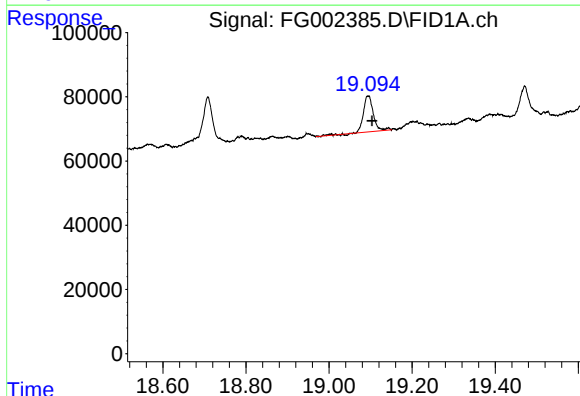


#15 N-TETRATRIACONTANE

R.T.: 19.094 min
Delta R.T.: -0.010 min
Response: 186255
Conc: 1.35 ug/ml

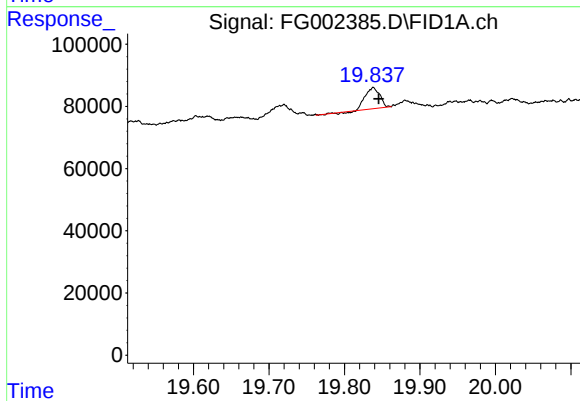

#16 N-HEXATRIACONTANE

R.T.: 19.838 min
Delta R.T.: -0.008 min
Response: 88928
Conc: 0.69 ug/ml

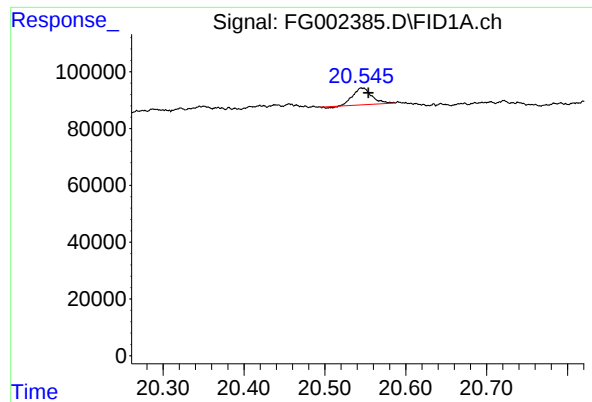

#17 N-OCTATRIACONTANE

R.T.: 20.546 min
Delta R.T.: -0.007 min
Response: 95257
Conc: 0.85 ug/ml