

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG092622\
Data File : FG010682.D
Signal(s) : FID1A.ch
Acq On : 26 Sep 2022 13:38
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
I.BLK

Integration File: autoint1.e
Quant Time: Sep 26 17:33:42 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG092622.M
Quant Title :
QLast Update : Mon Sep 26 16:36:10 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
9) S	TETRACOSANE-d50 (SURR...	14.766	2125085	17.943 ug/ml
Target Compounds				
16)	N-HEXATRIACONTANE	20.121f	7313	0.058 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG092622\
Data File : FG010682.D
Signal(s) : FID1A.ch
Acq On : 26 Sep 2022 13:38
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
I.BLK

Integration File: autoint1.e
Quant Time: Sep 26 17:33:42 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG092622.M
Quant Title :
QLast Update : Mon Sep 26 16:36:10 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

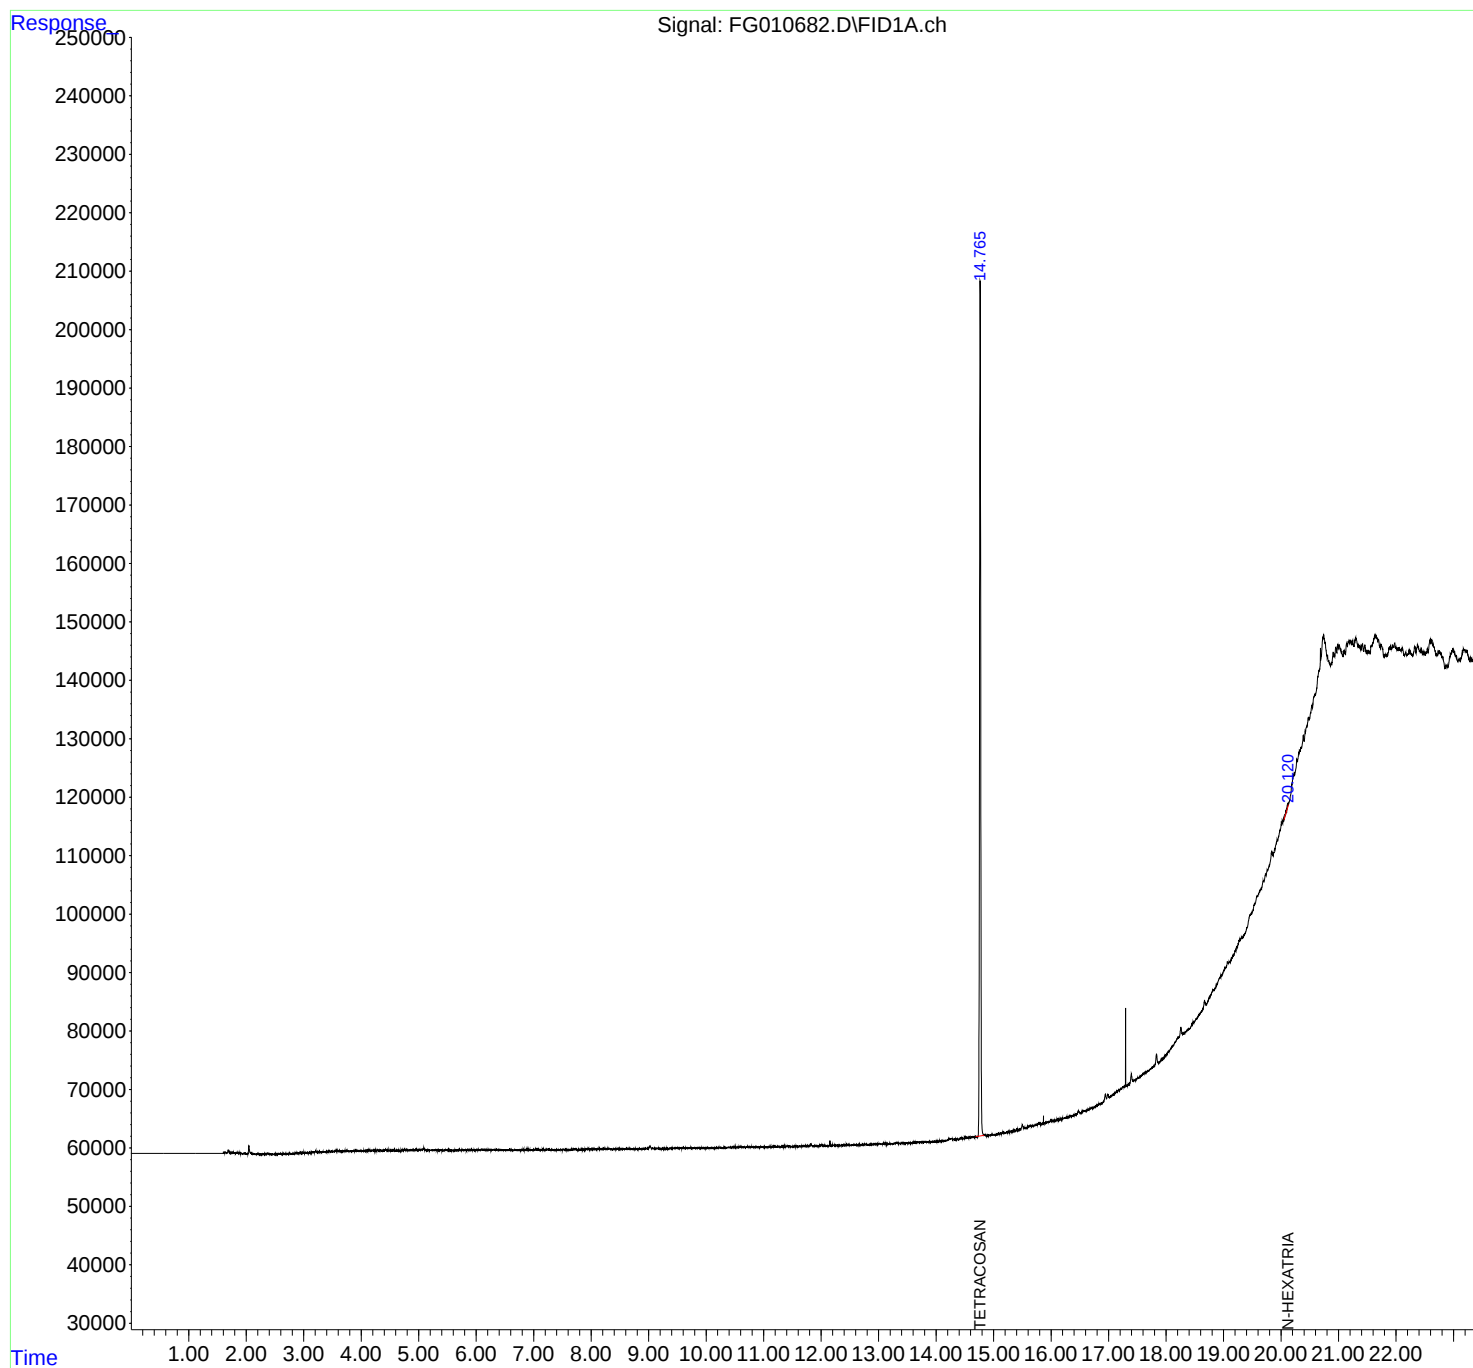


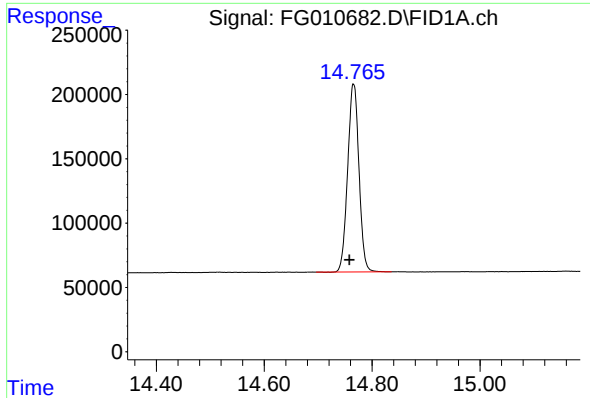

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.766 min
Delta R.T.: 0.008 min
Response: 2125085
Conc: 17.94 ug/ml

Instrument :
FID_G
ClientSampleId :
I.BLK

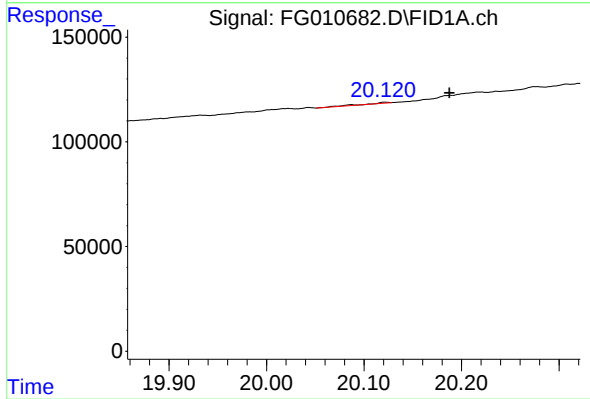

#16 N-HEXATRIACONTANE

R.T.: 20.121 min
Delta R.T.: -0.067 min
Response: 7313
Conc: 0.06 ug/ml