

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG092719\
 Data File : FG006075.D
 Signal(s) : FID1A.ch
 Acq On : 27 Sep 2019 18:49
 Operator : DD\AJ
 Sample : K5076-02
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Sep 27 23:40:26 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG090719.M
 Quant Title :
 QLast Update : Mon Sep 09 05:03:58 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.719	2033700	18.102 ug/ml
Target Compounds			
4) N-TETRADECANE	8.318f	257182	1.824 ug/ml
12) N-OCTACOSANE	16.899	354435	3.006 ug/ml
13) N-TRIACONTANE	17.790	458436	4.046 ug/ml
14) N-DOTRIACONTANE	18.625	276378	2.582 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG092719\
Data File : FG006075.D
Signal(s) : FID1A.ch
Acq On : 27 Sep 2019 18:49
Operator : DD\AJ
Sample : K5076-02
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Sep 27 23:40:26 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG090719.M
Quant Title :
QLast Update : Mon Sep 09 05:03:58 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

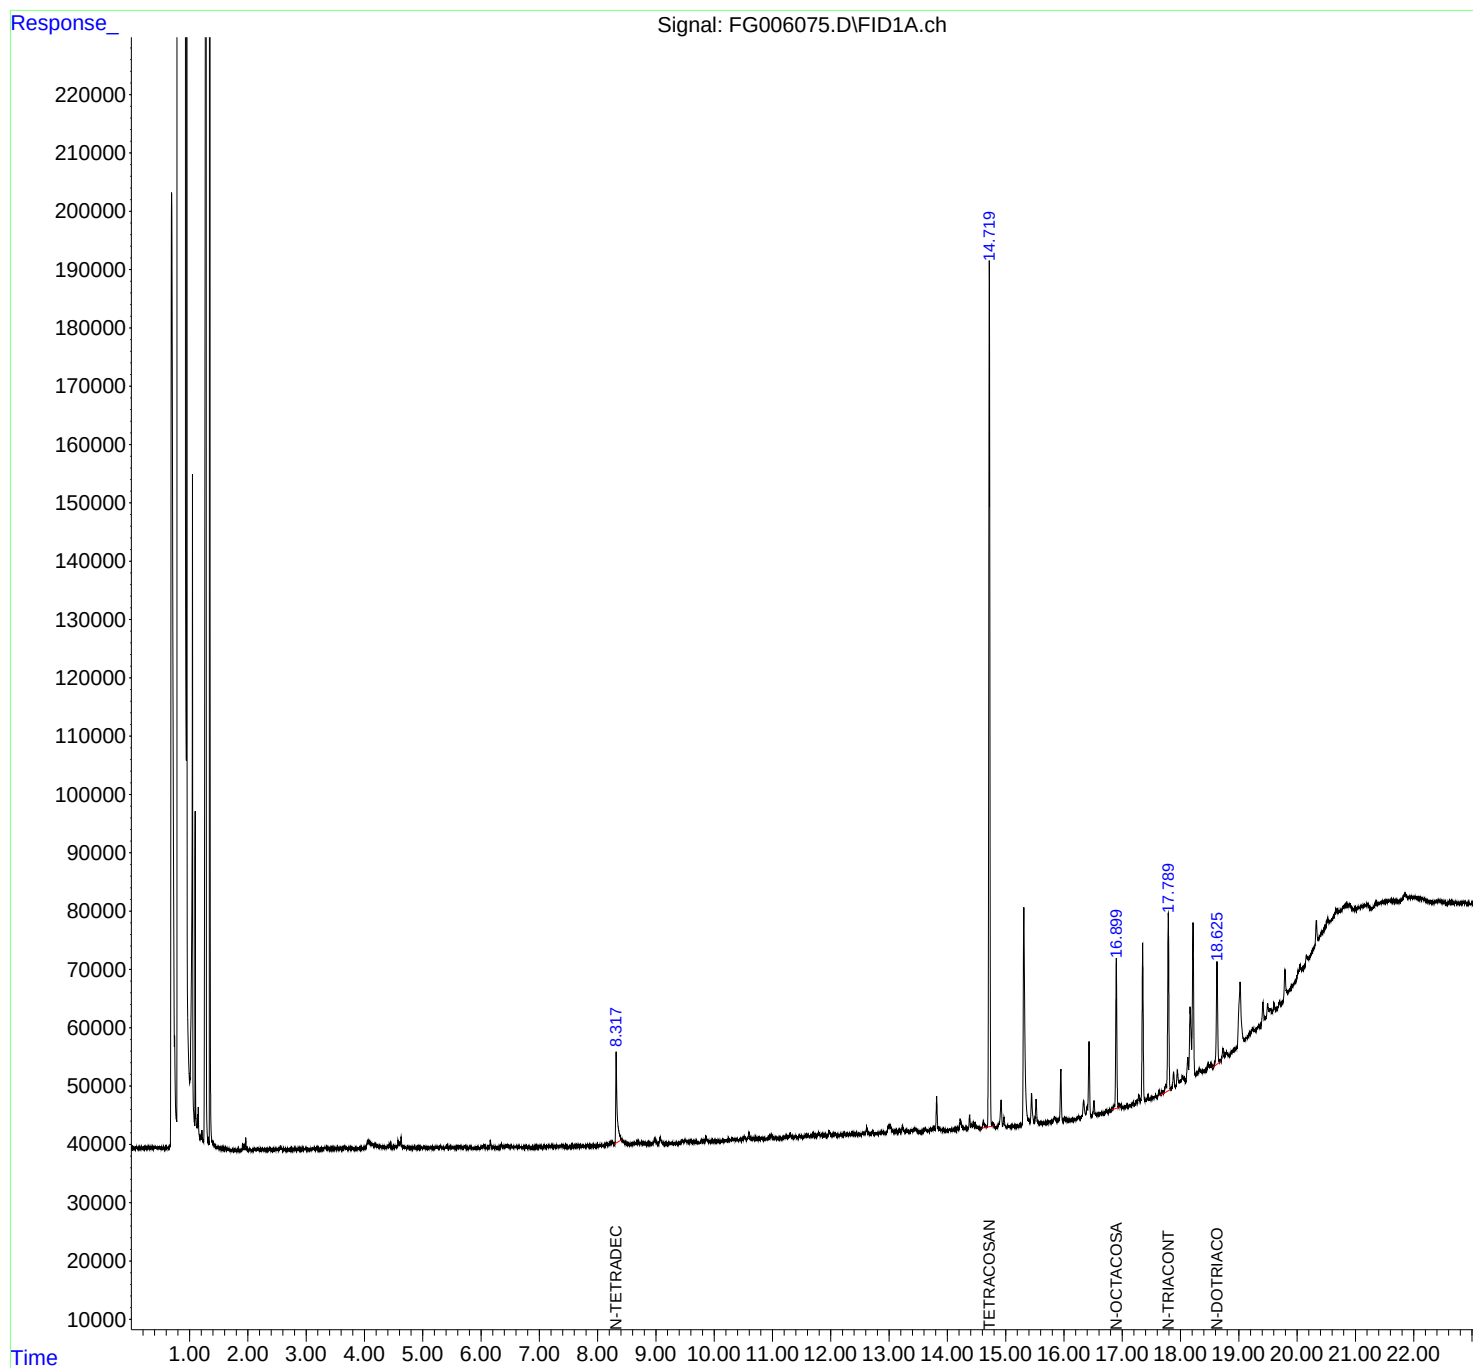


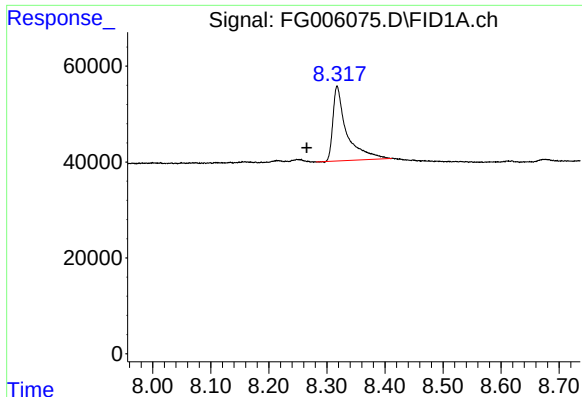

#4 N-TETRADECANE


R.T.: 8.318 min
Delta R.T.: 0.053 min
Response: 257182
Conc: 1.82 ug/ml

Instrument :
FID_G
ClientSampleId :

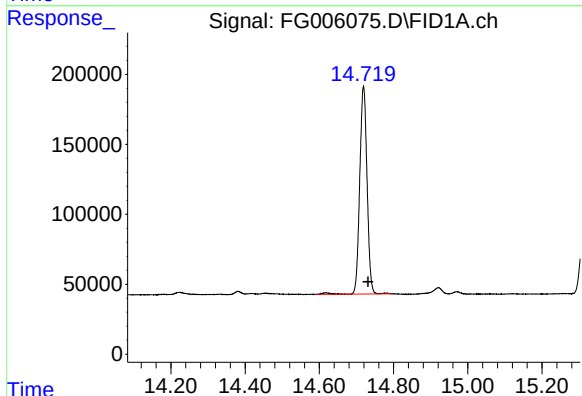


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.719 min
Delta R.T.: -0.012 min
Response: 2033700
Conc: 18.10 ug/ml

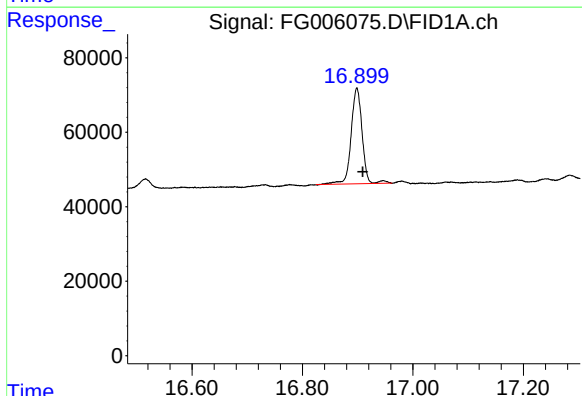


#12 N-OCTACOSANE

R.T.: 16.899 min
Delta R.T.: -0.011 min
Response: 354435
Conc: 3.01 ug/ml

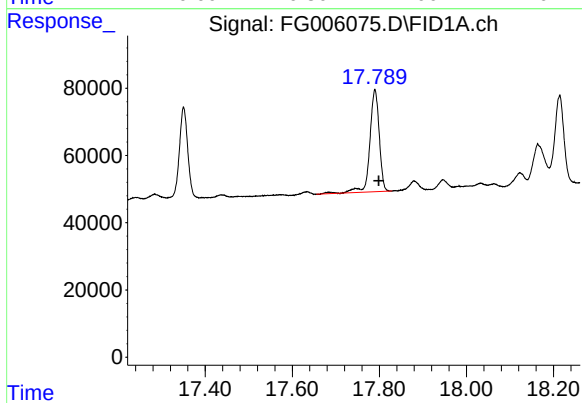

#13 N-TRIACONTANE

R.T.: 17.790 min
Delta R.T.: -0.009 min
Response: 458436
Conc: 4.05 ug/ml

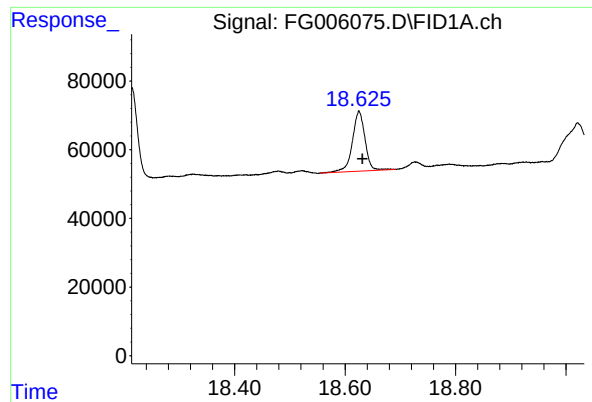

#14 N-DOTRIACONTANE

R.T.: 18.625 min
Delta R.T.: -0.006 min
Response: 276378
Conc: 2.58 ug/ml

Instrument :
FID_G
ClientSampleId :