

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG092719\
 Data File : FG006079.D
 Signal(s) : FID1A.ch
 Acq On : 27 Sep 2019 20:48
 Operator : DD\AJ
 Sample : K5076-06
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :
 SIMW-04-20190926

Integration File: autoint1.e
 Quant Time: Sep 27 23:41:23 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG090719.M
 Quant Title :
 QLast Update : Mon Sep 09 05:03:58 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.720	2010752	17.897 ug/ml
Target Compounds			
3) N-DODECANE	6.450	333625	2.356 ug/ml
4) N-TETRADECANE	8.316f	265639	1.884 ug/ml
6) N-OCTADECANE	11.383f	315557	2.301 ug/ml
10) N-TETRACOSANE	14.921	446775	3.503 ug/ml
11) N-HEXACOSANE	15.945	733407	5.985 ug/ml
12) N-OCTACOSANE	16.897	1218897	10.336 ug/ml
13) N-TRIACONTANE	17.788	1291134	11.395 ug/ml
14) N-DOTRIACONTANE	18.622	742219	6.935 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG092719\
Data File : FG006079.D
Signal(s) : FID1A.ch
Acq On : 27 Sep 2019 20:48
Operator : DD\AJ
Sample : K5076-06
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
SIMW-04-20190926

Integration File: autoint1.e
Quant Time: Sep 27 23:41:23 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG090719.M
Quant Title :
QLast Update : Mon Sep 09 05:03:58 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

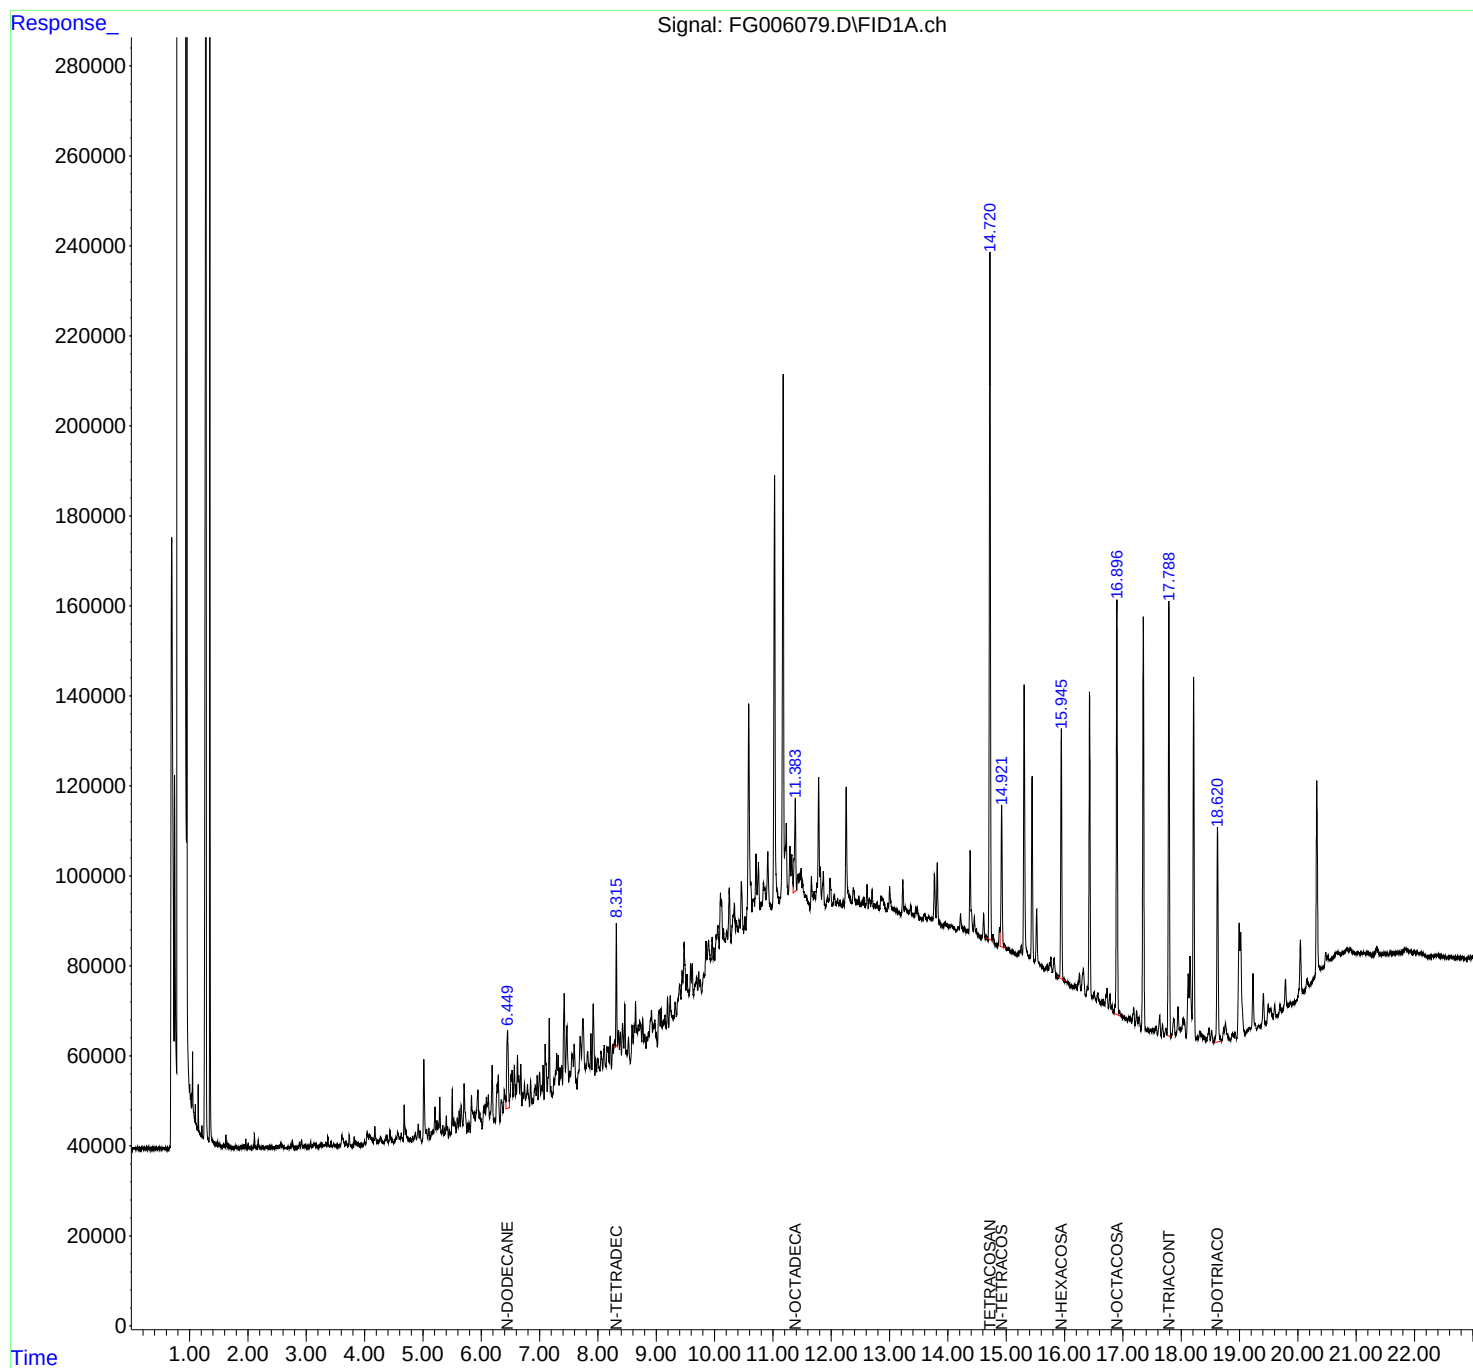


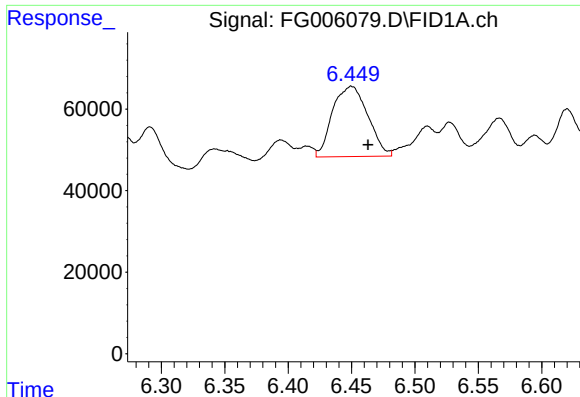

#3 N-DODECANE


R.T.: 6.450 min
Delta R.T.: -0.013 min
Response: 333625
Conc: 2.36 ug/ml

Instrument :
FID_G
ClientSampleId :
SIMW-04-20190926

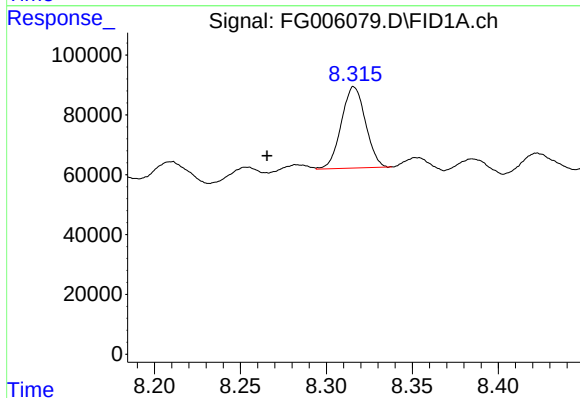


#4 N-TETRADECANE

R.T.: 8.316 min
Delta R.T.: 0.051 min
Response: 265639
Conc: 1.88 ug/ml

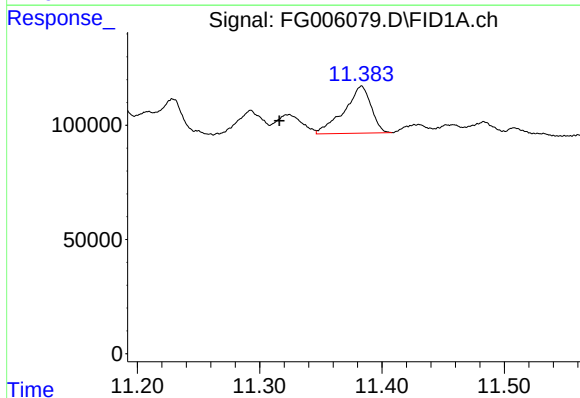


#6 N-OCTADECANE

R.T.: 11.383 min
Delta R.T.: 0.067 min
Response: 315557
Conc: 2.30 ug/ml

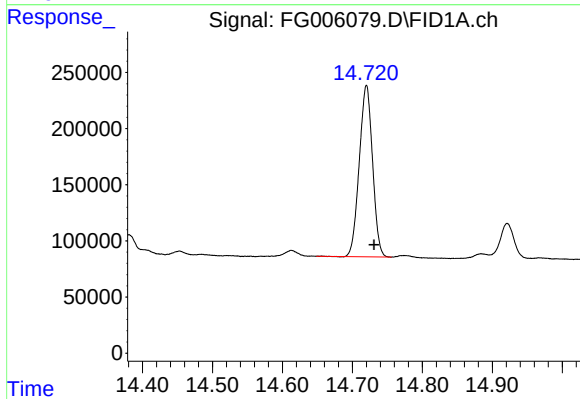

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.720 min
Delta R.T.: -0.011 min
Response: 2010752
Conc: 17.90 ug/ml

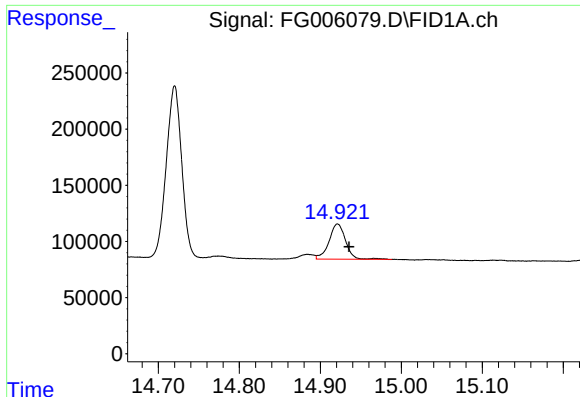

#10 N-TETRACOSANE


R.T.: 14.921 min
Delta R.T.: -0.014 min
Response: 446775
Conc: 3.50 ug/ml

Instrument :
FID_G
ClientSampleId :
SIMW-04-20190926

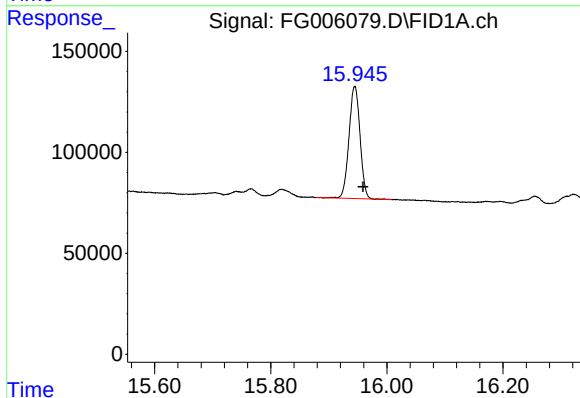


#11 N-HEXACOSANE

R.T.: 15.945 min
Delta R.T.: -0.014 min
Response: 733407
Conc: 5.98 ug/ml

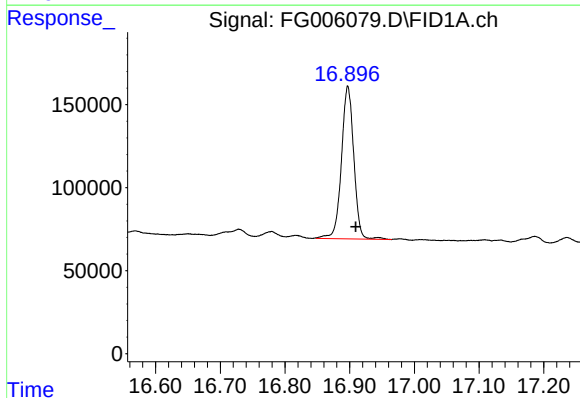


#12 N-OCTACOSANE

R.T.: 16.897 min
Delta R.T.: -0.012 min
Response: 1218897
Conc: 10.34 ug/ml

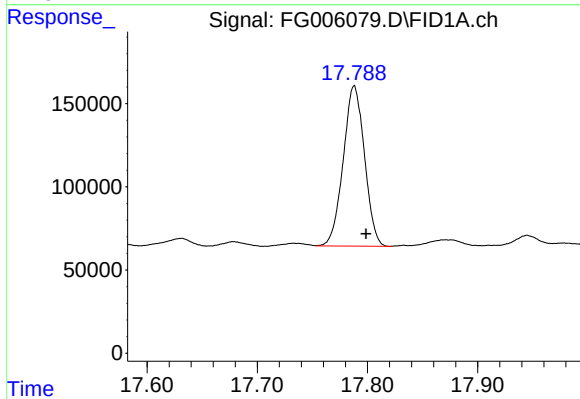

#13 N-TRIACONTANE

R.T.: 17.788 min
Delta R.T.: -0.011 min
Response: 1291134
Conc: 11.39 ug/ml

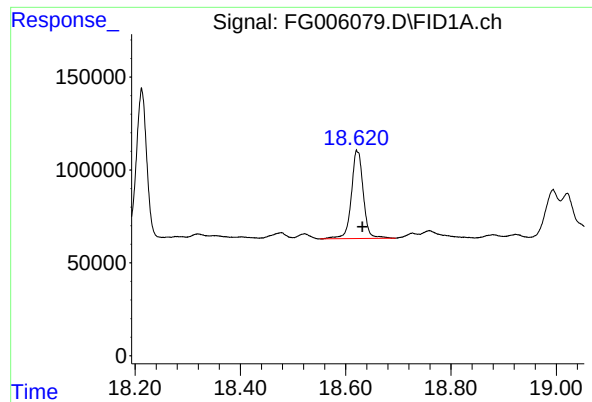

#14 N-DOTRIACONTANE

R.T.: 18.622 min
Delta R.T.: -0.009 min
Response: 742219
Conc: 6.93 ug/ml

Instrument :
FID_G
ClientSampleId :
SIMW-04-20190926