

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG092719\
 Data File : FG006080.D
 Signal(s) : FID1A.ch
 Acq On : 27 Sep 2019 21:17
 Operator : DD\AJ
 Sample : K5076-07
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :
 MW-3-20190926

Integration File: autoint1.e
 Quant Time: Sep 27 23:41:36 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG090719.M
 Quant Title :
 QLast Update : Mon Sep 09 05:03:58 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.718	1872039	16.663 ug/ml
Target Compounds			
4) N-TETRADECANE	8.319f	229874	1.630 ug/ml
8) N-DOCOSANE	13.816	164792	1.253 ug/ml
10) N-TETRACOSANE	14.921	444780	3.488 ug/ml
11) N-HEXACOSANE	15.945	654317	5.339 ug/ml
12) N-OCTACOSANE	16.897	870116	7.379 ug/ml
13) N-TRIACONTANE	17.786	889764	7.853 ug/ml
14) N-DOTRIACONTANE	18.621	420273	3.927 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG092719\
Data File : FG006080.D
Signal(s) : FID1A.ch
Acq On : 27 Sep 2019 21:17
Operator : DD\AJ
Sample : K5076-07
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
MW-3-20190926

Integration File: autoint1.e
Quant Time: Sep 27 23:41:36 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG090719.M
Quant Title :
QLast Update : Mon Sep 09 05:03:58 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

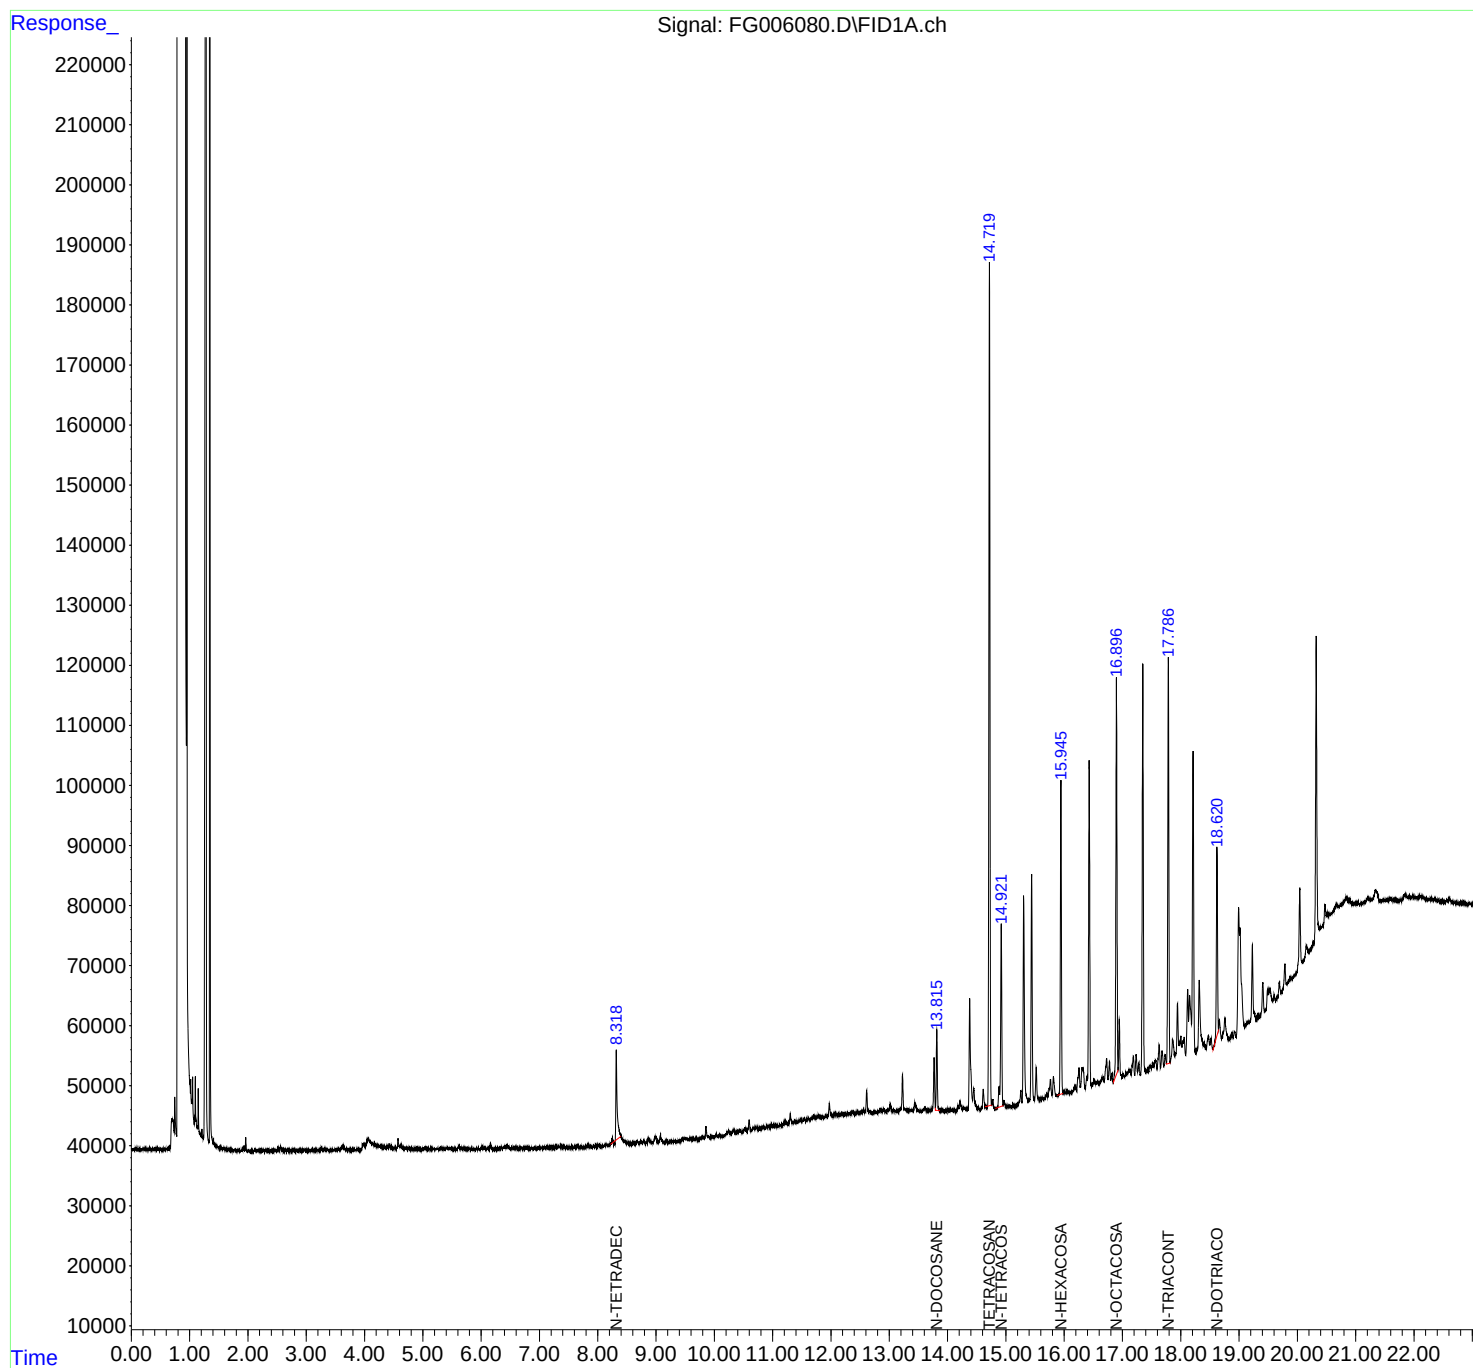


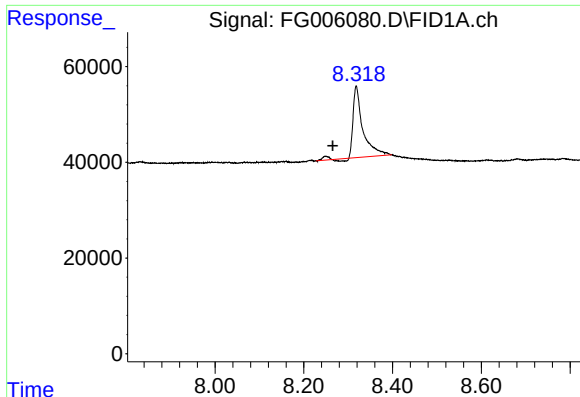

#4 N-TETRADECANE


R.T.: 8.319 min
Delta R.T.: 0.053 min
Response: 229874
Conc: 1.63 ug/ml

Instrument :
FID_G
ClientSampleId :
MW-3-20190926

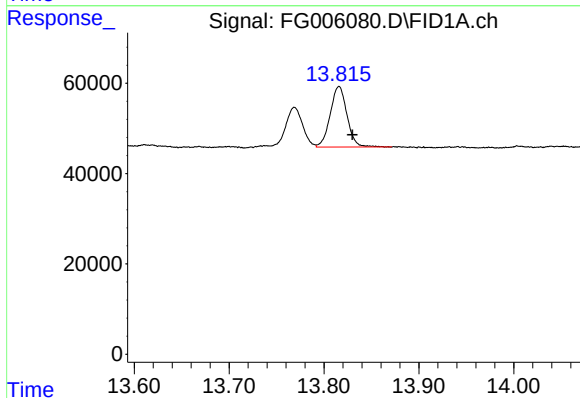


#8 N-DOCOSANE

R.T.: 13.816 min
Delta R.T.: -0.014 min
Response: 164792
Conc: 1.25 ug/ml

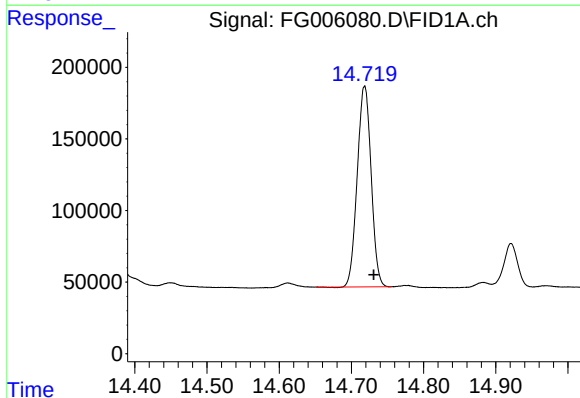


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.718 min
Delta R.T.: -0.013 min
Response: 1872039
Conc: 16.66 ug/ml

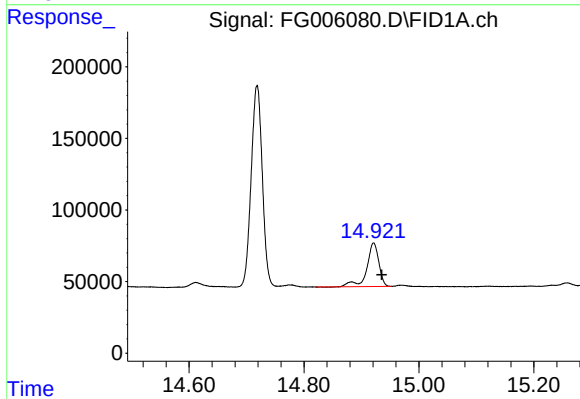

#10 N-TETRACOSANE


R.T.: 14.921 min
Delta R.T.: -0.014 min
Response: 444780
Conc: 3.49 ug/ml

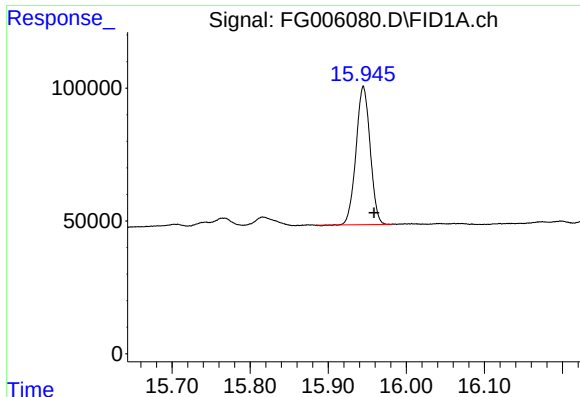

#11 N-HEXACOSANE


R.T.: 15.945 min
Delta R.T.: -0.014 min
Response: 654317
Conc: 5.34 ug/ml

Instrument :
FID_G
ClientSampleId :
MW-3-20190926

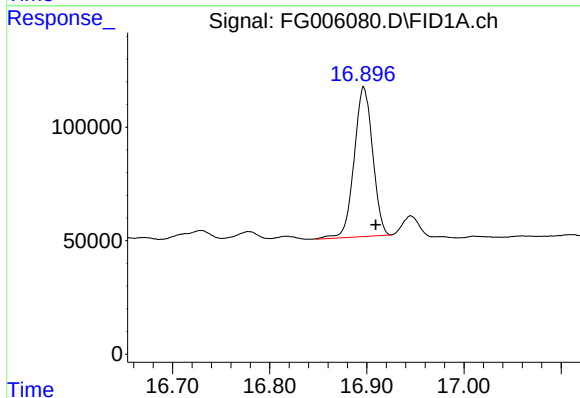


#12 N-OCTACOSANE

R.T.: 16.897 min
Delta R.T.: -0.012 min
Response: 870116
Conc: 7.38 ug/ml

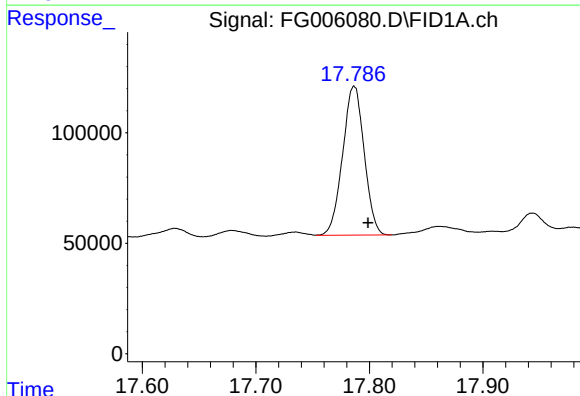

#13 N-TRIACONTANE

R.T.: 17.786 min
Delta R.T.: -0.012 min
Response: 889764
Conc: 7.85 ug/ml

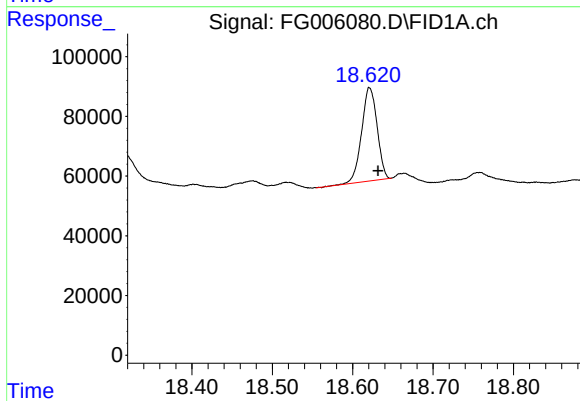

#14 N-DOTRIACONTANE

R.T.: 18.621 min
Delta R.T.: -0.010 min
Response: 420273
Conc: 3.93 ug/ml