

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG092719\
Data File : FG006078.D
Signal(s) : FID1A.ch
Acq On : 27 Sep 2019 20:18
Operator : DD\AJ
Sample : K5076-05
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
SIMW-02-20190926-A

Integration File: autoint1.e
Quant Time: Sep 27 23:41:11 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG090719.M
Quant Title :
QLast Update : Mon Sep 09 05:03:58 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.719	2148272	19.121 ug/ml

Target Compounds

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG092719\
Data File : FG006078.D
Signal(s) : FID1A.ch
Acq On : 27 Sep 2019 20:18
Operator : DD\AJ
Sample : K5076-05
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
SIMW-02-20190926-A

Integration File: autoint1.e
Quant Time: Sep 27 23:41:11 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG090719.M
Quant Title :
QLast Update : Mon Sep 09 05:03:58 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

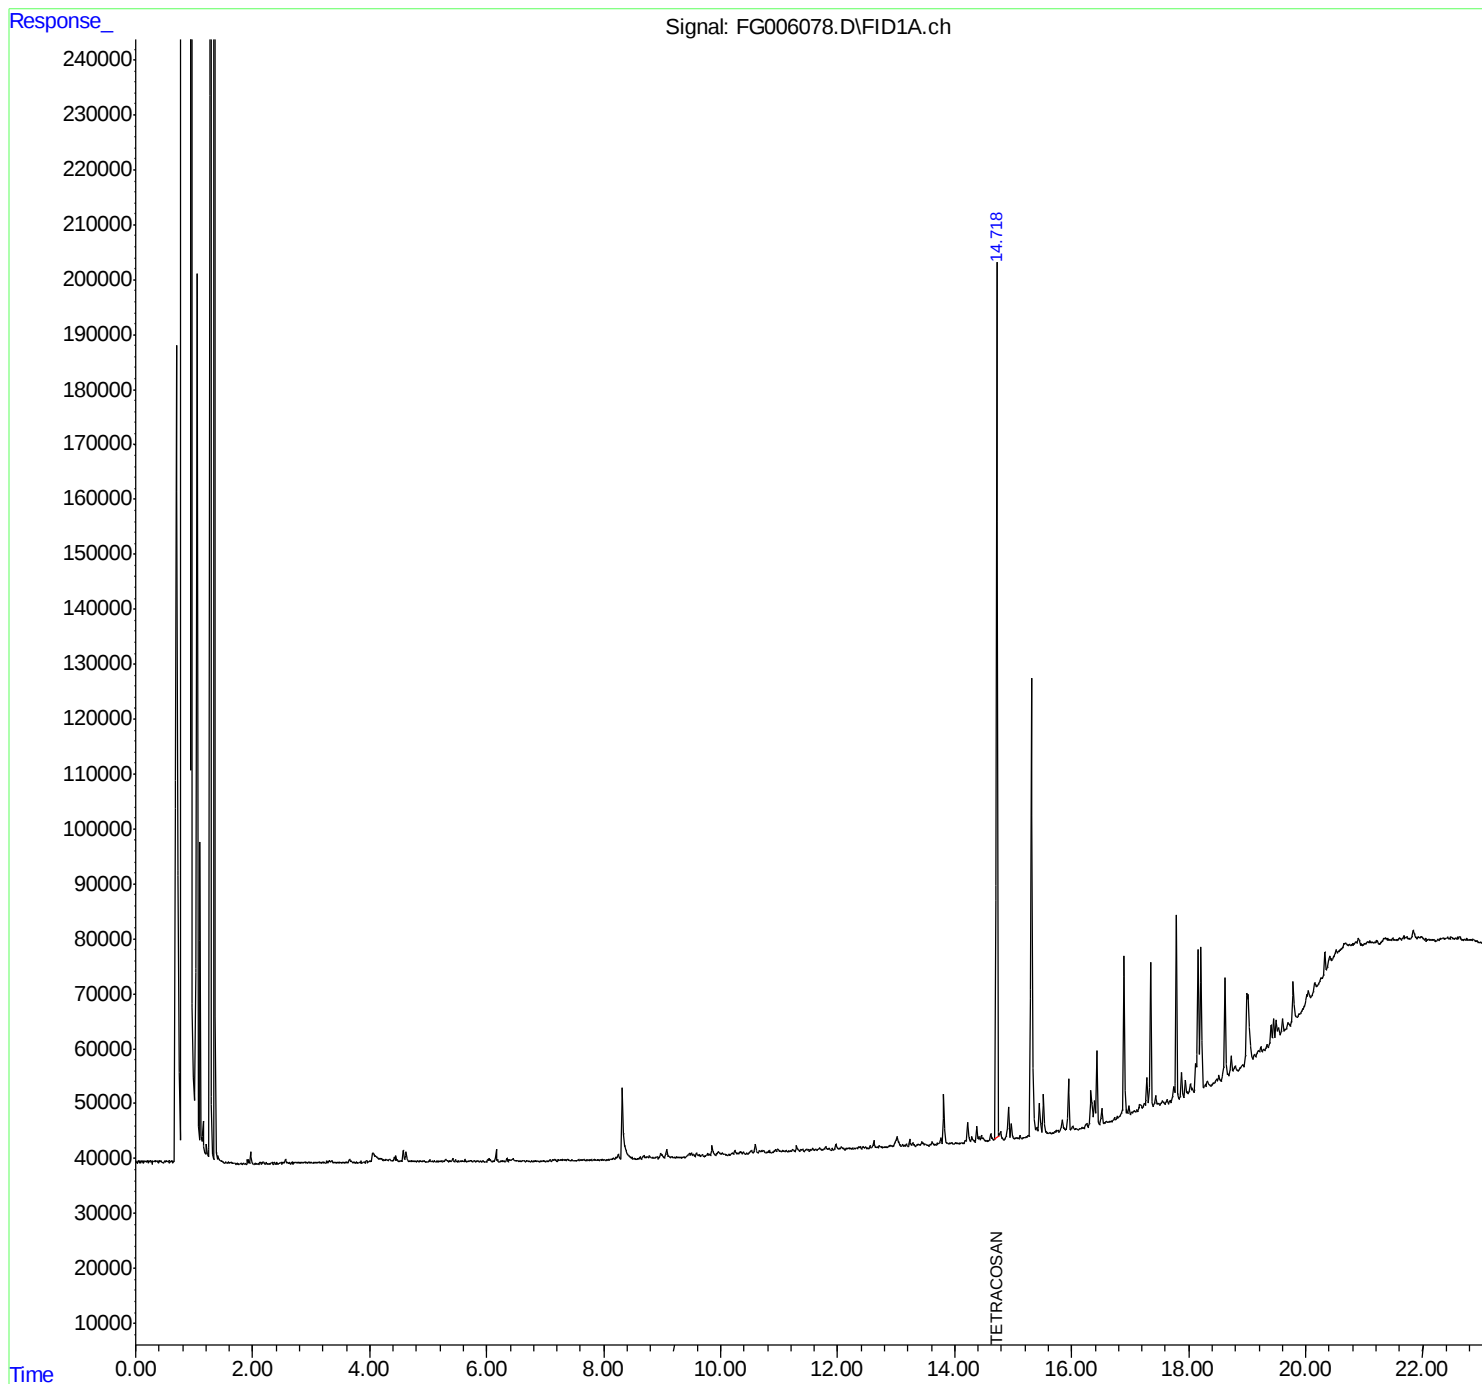

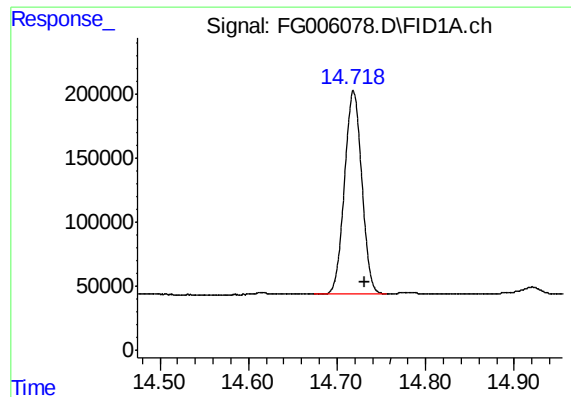

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.719 min
Delta R.T.: -0.012 min
Response: 2148272
Conc: 19.12 ug/ml

Instrument :
FID_G
ClientSampleId :
SIMW-02-20190926-A