

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG092722\
 Data File : FG010692.D
 Signal(s) : FID1A.ch
 Acq On : 27 Sep 2022 12:40
 Operator : YP\AJ
 Sample : RT MARKER
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :
 RT MARKER

Integration File: autoint1.e
 Quant Time: Sep 28 02:02:49 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG092622.M
 Quant Title :
 QLast Update : Mon Sep 26 16:36:10 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds			
3) N-DODECANE	6.461	2593672	20.151 ug/ml
12) N-OCTACOSANE	16.933	2825662	21.102 ug/ml
13) N-TRIACONTANE	17.821	87584	0.658 ug/ml
14) N-DOTRIACONTANE	18.654	140143	1.061 ug/ml
15) N-TETRATRIACONTANE	19.439	118215	0.898 ug/ml
16) N-HEXATRIACONTANE	20.182	90261	0.711 ug/ml
17) N-OCTATRIACONTANE	20.892	57809	0.457 ug/ml
18) N-TETRACONTANE	21.784f	280864	2.121 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG092722\
Data File : FG010692.D
Signal(s) : FID1A.ch
Acq On : 27 Sep 2022 12:40
Operator : YP\AJ
Sample : RT MARKER
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
RT MARKER

Integration File: autoint1.e
Quant Time: Sep 28 02:02:49 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG092622.M
Quant Title :
QLast Update : Mon Sep 26 16:36:10 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

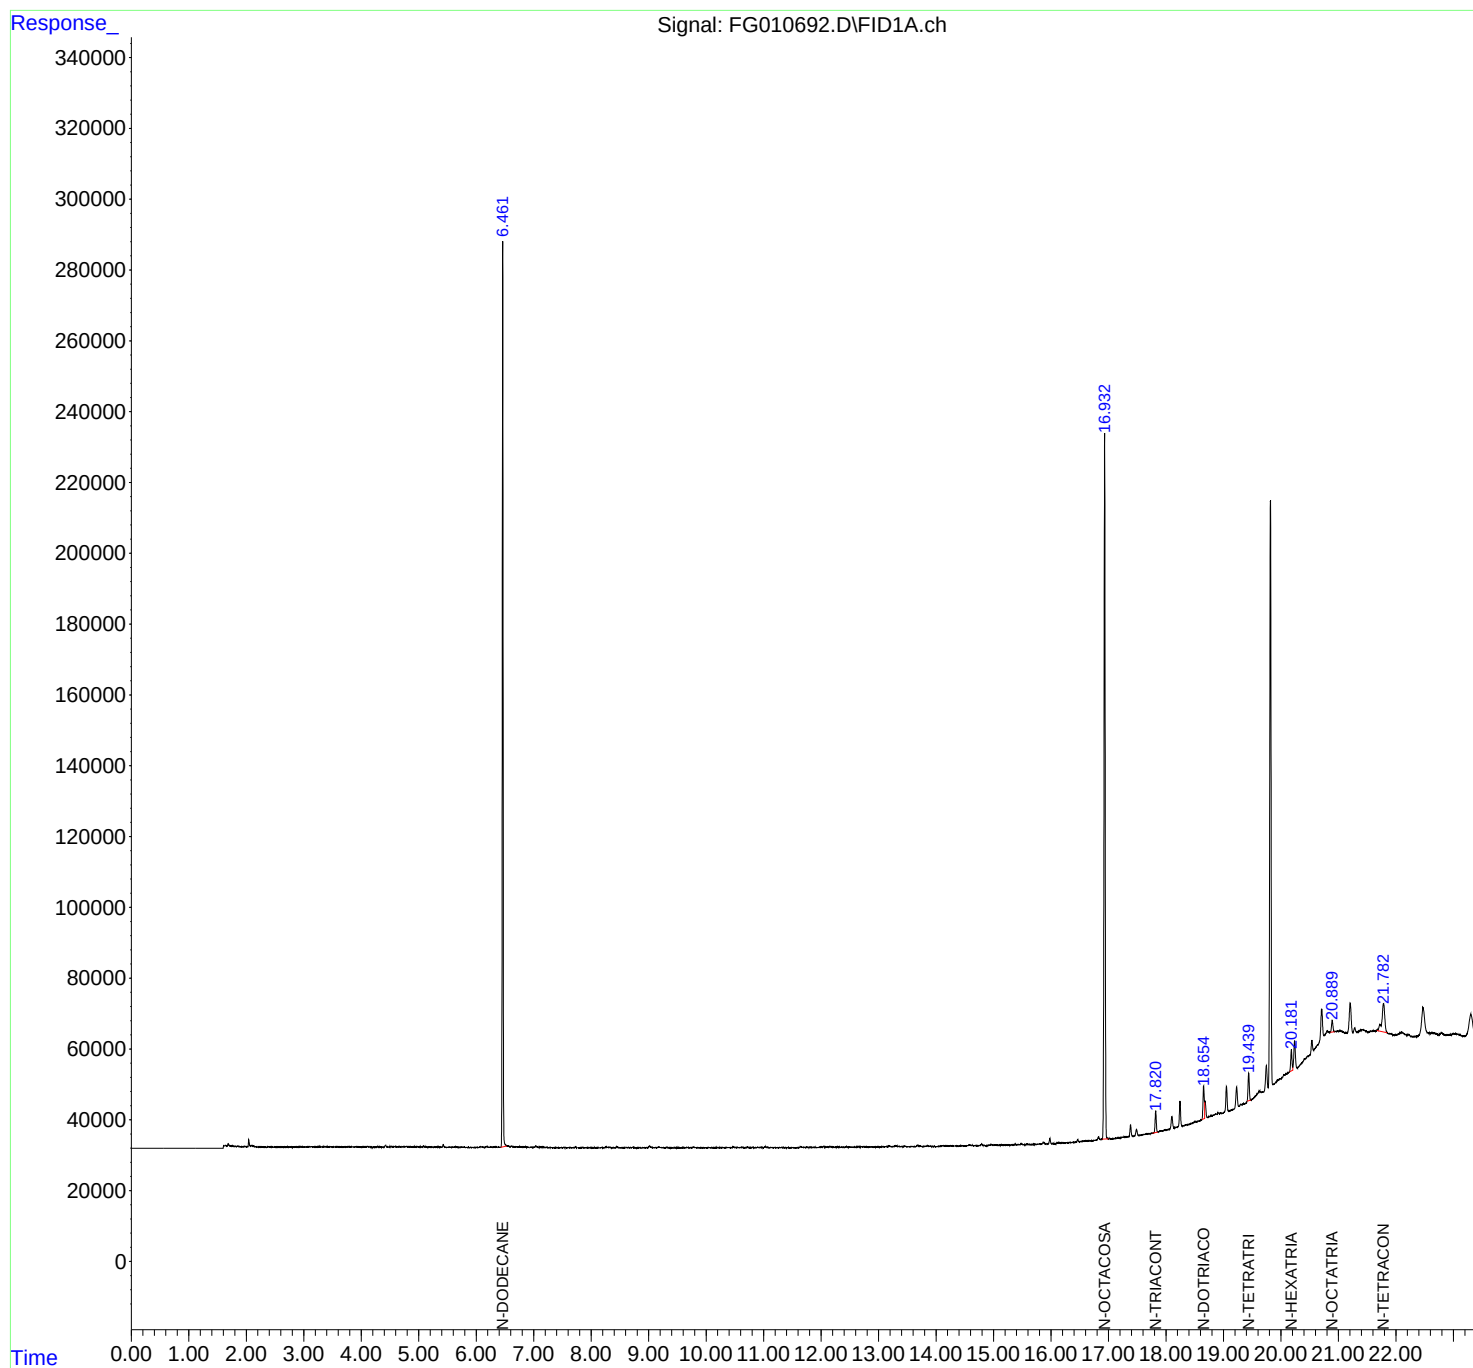


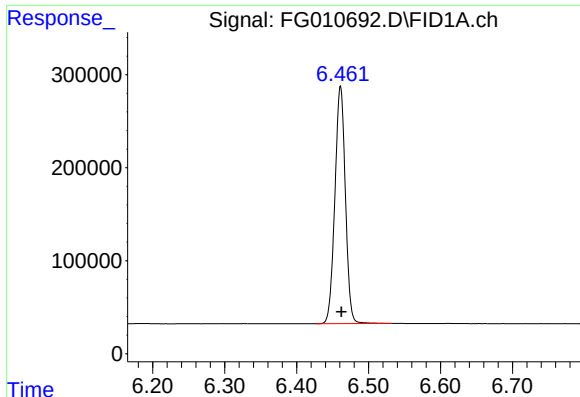

#3 N-DODECANE


R.T.: 6.461 min
Delta R.T.: -0.001 min
Response: 2593672
Conc: 20.15 ug/ml

Instrument :
FID_G
ClientSampleId :
RT MARKER

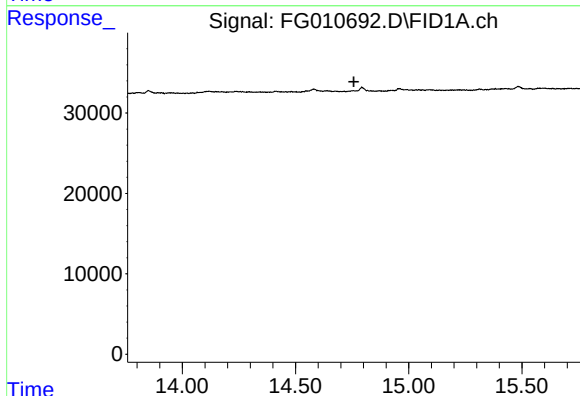


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.758 min
Response: 0
Conc: N.D.

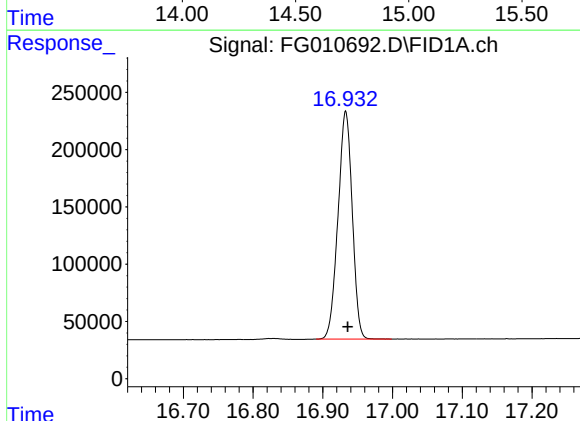


#12 N-OCTACOSANE

R.T.: 16.933 min
Delta R.T.: -0.003 min
Response: 2825662
Conc: 21.10 ug/ml

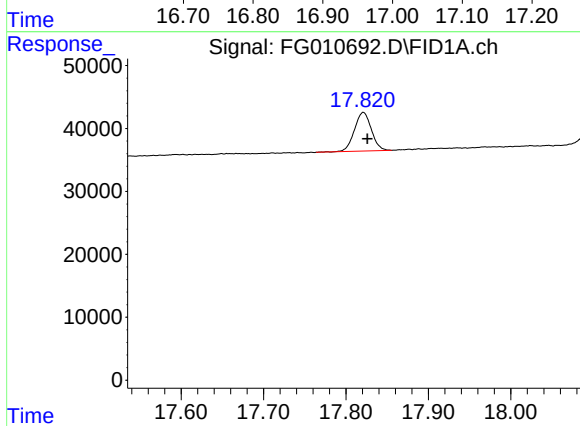

#13 N-TRIACONTANE


R.T.: 17.821 min
Delta R.T.: -0.005 min
Response: 87584
Conc: 0.66 ug/ml

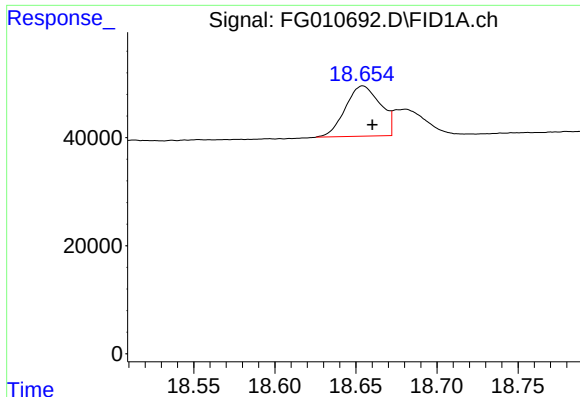

#14 N-DOTRIACONTANE


R.T.: 18.654 min
Delta R.T.: -0.006 min
Response: 140143
Conc: 1.06 ug/ml

Instrument :
FID_G
ClientSampleId :
RT MARKER

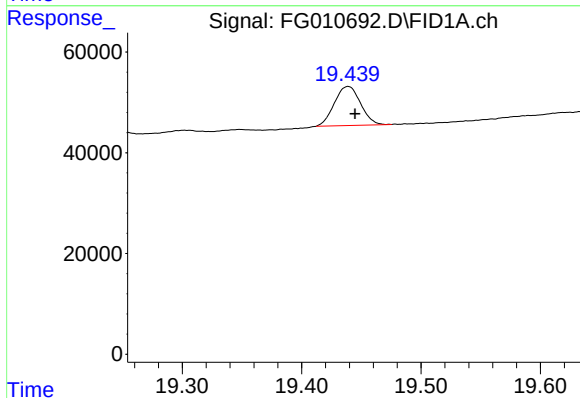


#15 N-TETRATRIACONTANE

R.T.: 19.439 min
Delta R.T.: -0.006 min
Response: 118215
Conc: 0.90 ug/ml

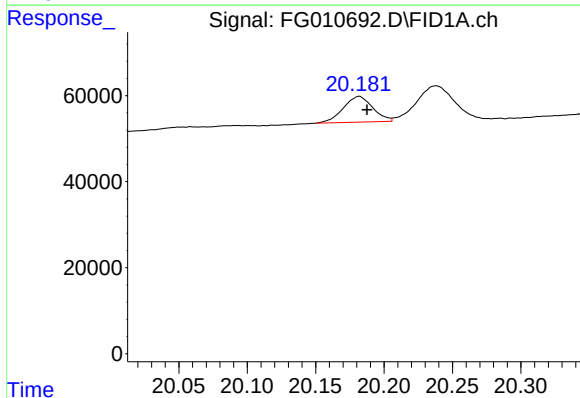


#16 N-HEXATRIACONTANE

R.T.: 20.182 min
Delta R.T.: -0.006 min
Response: 90261
Conc: 0.71 ug/ml

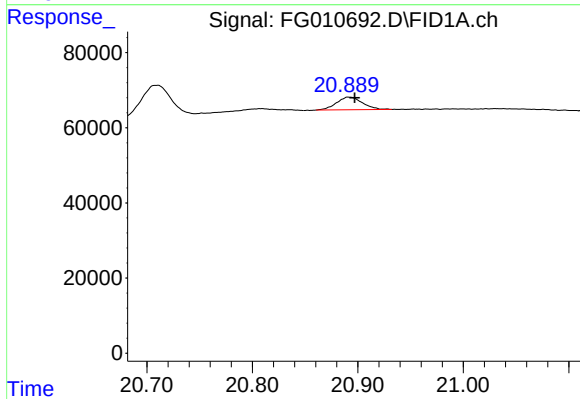

#17 N-OCTATRIACONTANE

R.T.: 20.892 min
Delta R.T.: -0.005 min
Response: 57809
Conc: 0.46 ug/ml

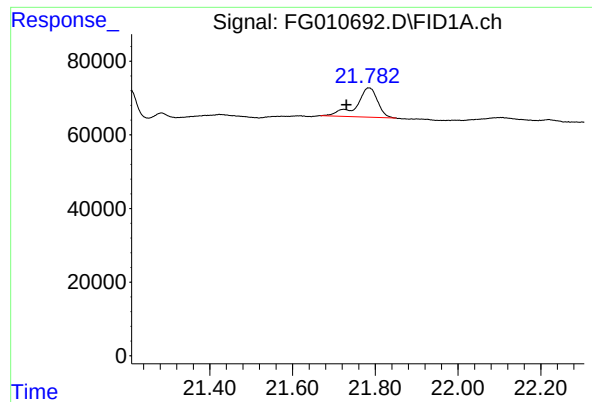

#18 N-TETRACONTANE

R.T.: 21.784 min
Delta R.T.: 0.054 min
Response: 280864
Conc: 2.12 ug/ml

Instrument :
FID_G
ClientSampleId :
RT MARKER