

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG092722\
Data File : FG010692.D
Signal(s) : FID1A.ch
Acq On : 27 Sep 2022 12:40
Operator : YP\AJ
Sample : RT MARKER
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
RT MARKER

Integration File: autoint1.e
Quant Time: Sep 28 02:02:49 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG092622.M
Quant Title :
QLast Update : Mon Sep 26 16:36:10 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
3)	N-DODECANE	6.461	2593672	20.151 ug/ml
12)	N-OCTACOSANE	16.933	2825662	21.102 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG092722\
Data File : FG010692.D
Signal(s) : FID1A.ch
Acq On : 27 Sep 2022 12:40
Operator : YP\AJ
Sample : RT MARKER
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
RT MARKER

Integration File: autoint1.e
Quant Time: Sep 28 02:02:49 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG092622.M
Quant Title :
QLast Update : Mon Sep 26 16:36:10 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

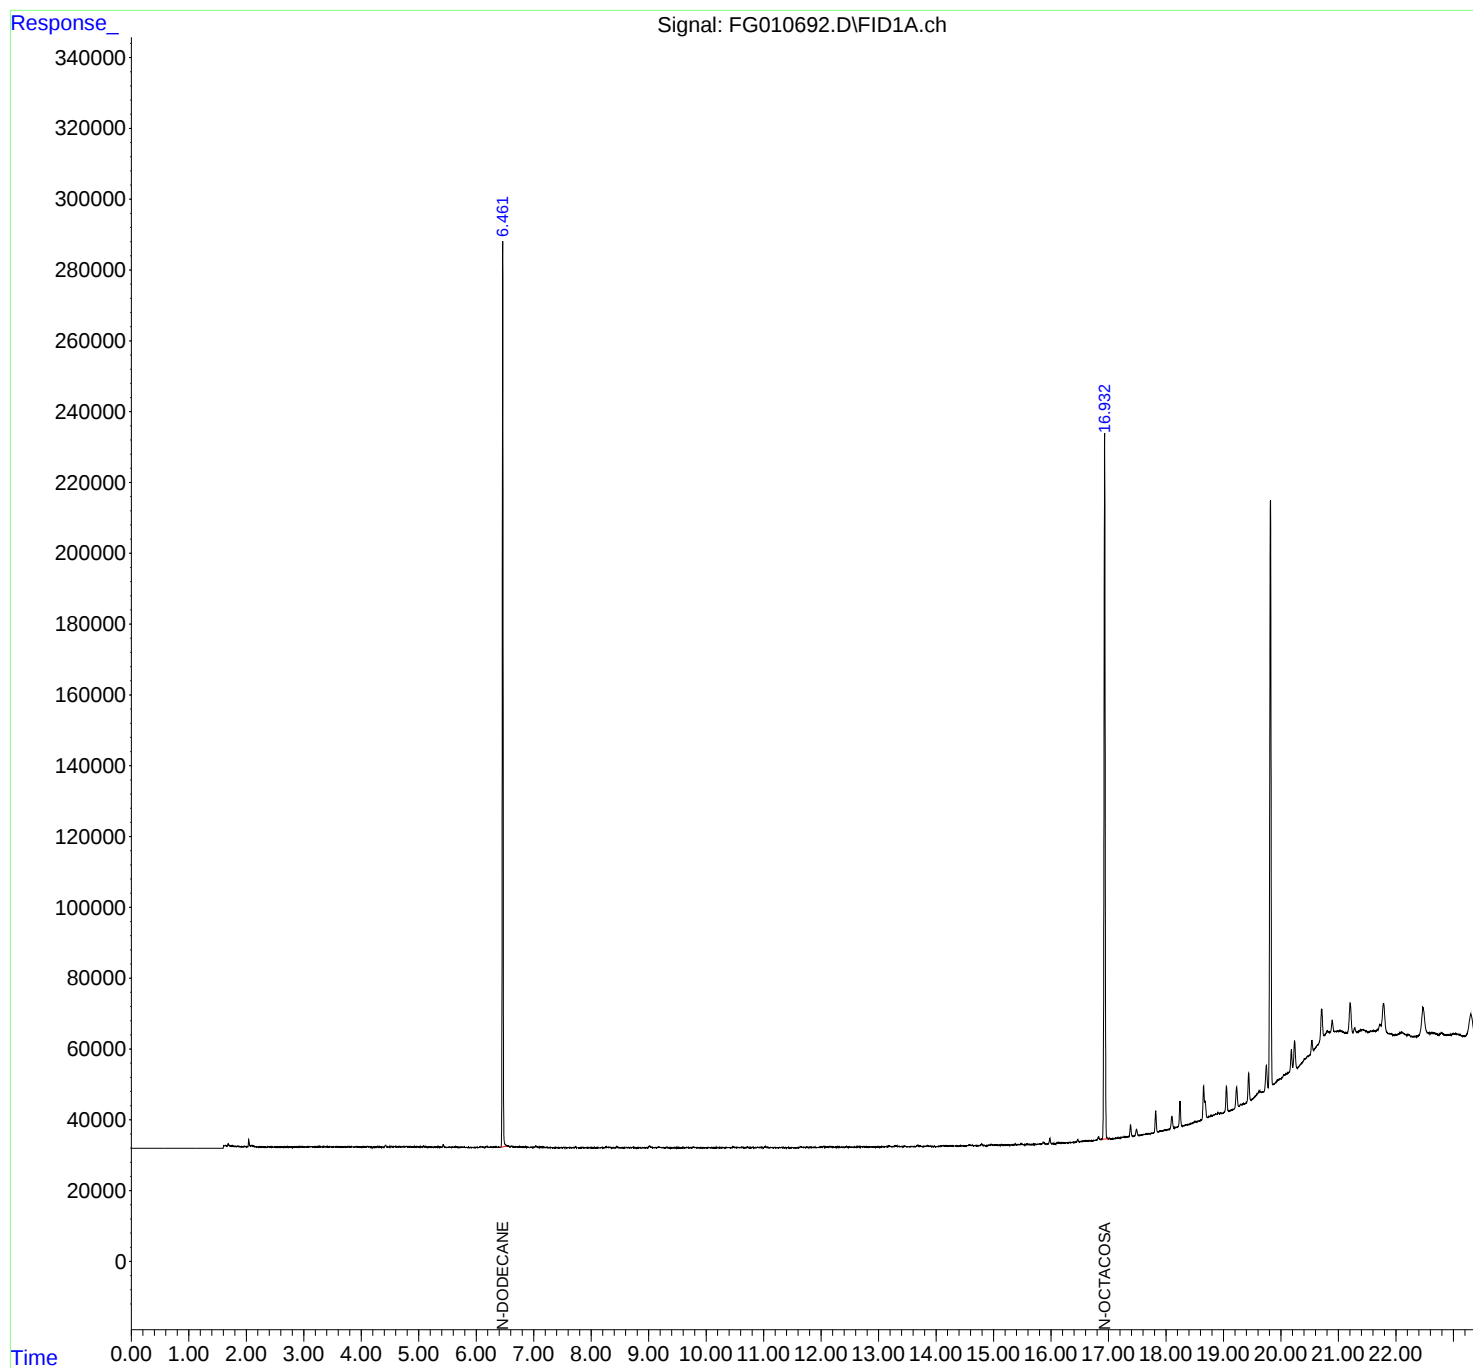


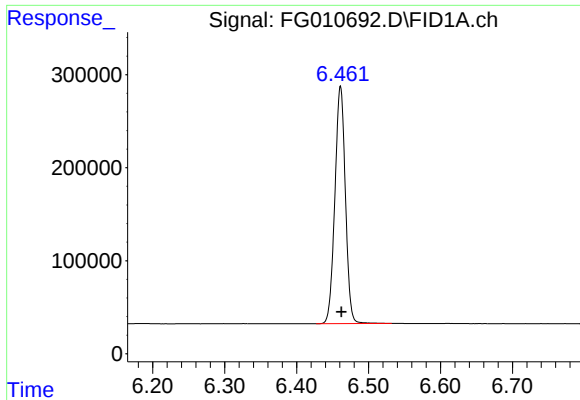

#3 N-DODECANE


R.T.: 6.461 min
Delta R.T.: -0.001 min
Response: 2593672
Conc: 20.15 ug/ml

Instrument :
FID_G
ClientSampleId :
RT MARKER

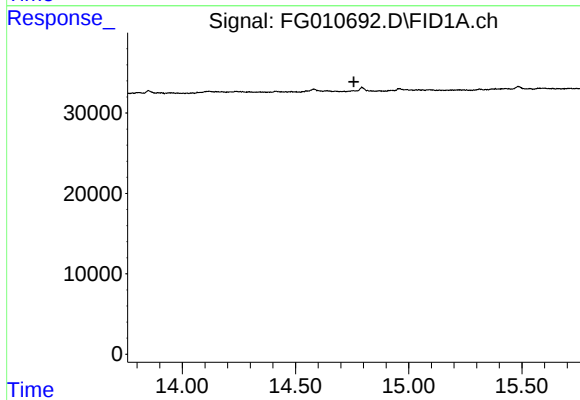

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.758 min
Response: 0
Conc: N.D.

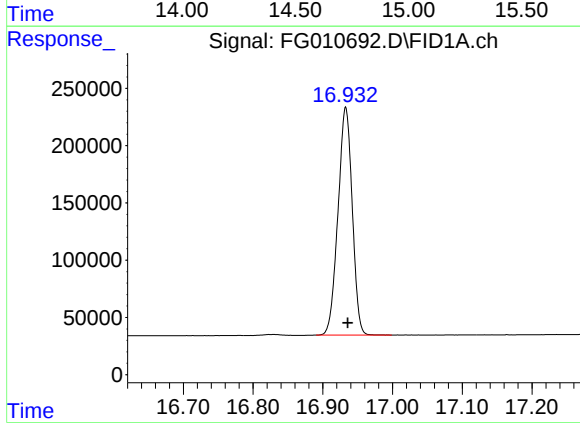

#12 N-OCTACOSANE

R.T.: 16.933 min
Delta R.T.: -0.003 min
Response: 2825662
Conc: 21.10 ug/ml