

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG092922\
Data File : FG010714.D
Signal(s) : FID1A.ch
Acq On : 29 Sep 2022 13:43
Operator : YP\AJ
Sample : N4785-19
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
RR-DIES-WP

Integration File: autoint1.e
Quant Time: Sep 29 18:17:52 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG092822.M
Quant Title :
QLast Update : Thu Sep 29 02:21:49 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.748	2327186	19.182 ug/ml

Target Compounds

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG092922\
Data File : FG010714.D
Signal(s) : FID1A.ch
Acq On : 29 Sep 2022 13:43
Operator : YP\AJ
Sample : N4785-19
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
RR-DIES-WP

Integration File: autoint1.e
Quant Time: Sep 29 18:17:52 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG092822.M
Quant Title :
QLast Update : Thu Sep 29 02:21:49 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

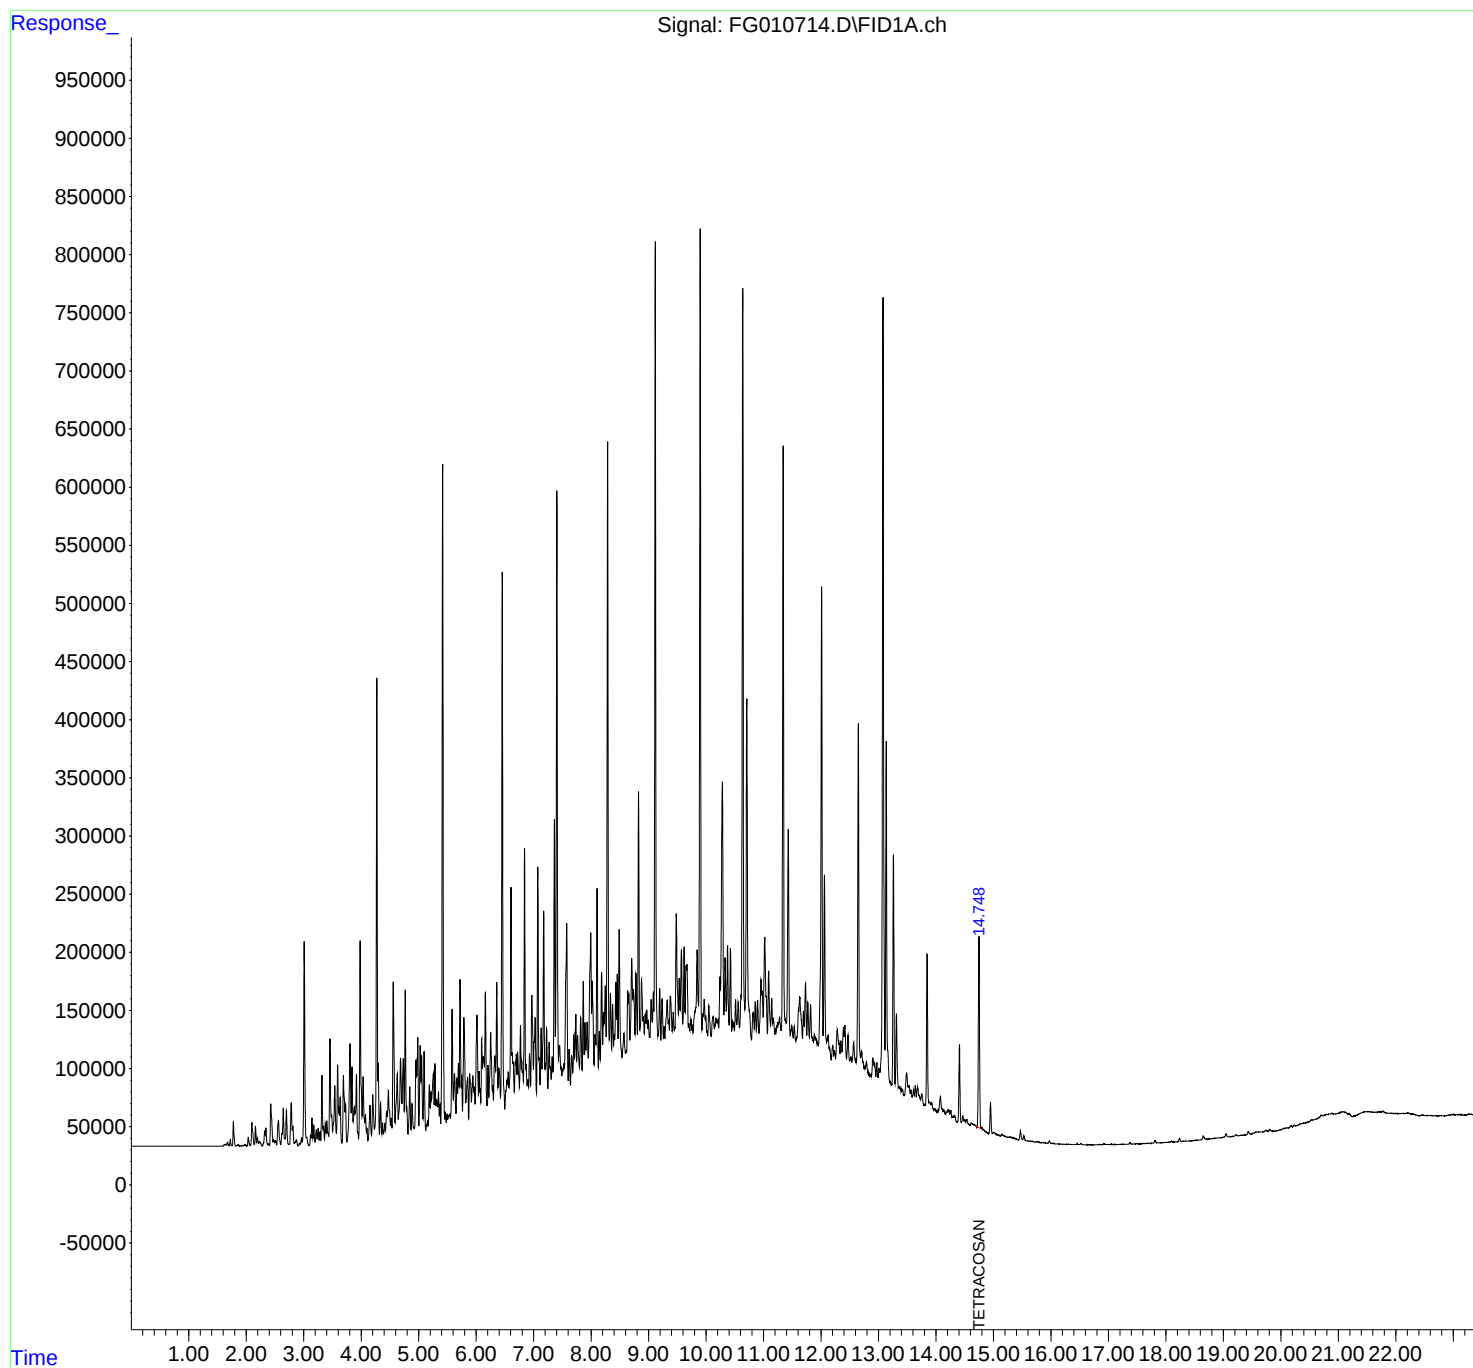

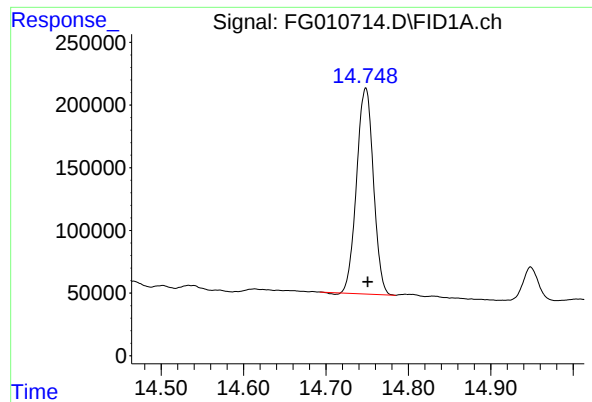

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.748 min
Delta R.T.: -0.002 min
Response: 2327186
Conc: 19.18 ug/ml

Instrument :

FID_G

ClientSampleId :

RR-DIES-WP