

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG092923\
Data File : FG012956.D
Signal(s) : FID1A.ch
Acq On : 29 Sep 2023 16:14
Operator : YP\AJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Sep 30 03:44:57 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG092123.M
Quant Title :
QLast Update : Fri Sep 22 02:14:31 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
14) N-DOTRIACONTANE	18.976	119724	1.076 ug/ml
15) N-TETRATRIACONTANE	19.764	84571	0.896 ug/ml
16) N-HEXATRIACONTANE	20.499	65336	0.884 ug/ml
17) N-OCTATRIACONTANE	21.210	11901	0.180 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG092923\
Data File : FG012956.D
Signal(s) : FID1A.ch
Acq On : 29 Sep 2023 16:14
Operator : YP\AJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Sep 30 03:44:57 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG092123.M
Quant Title :
QLast Update : Fri Sep 22 02:14:31 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

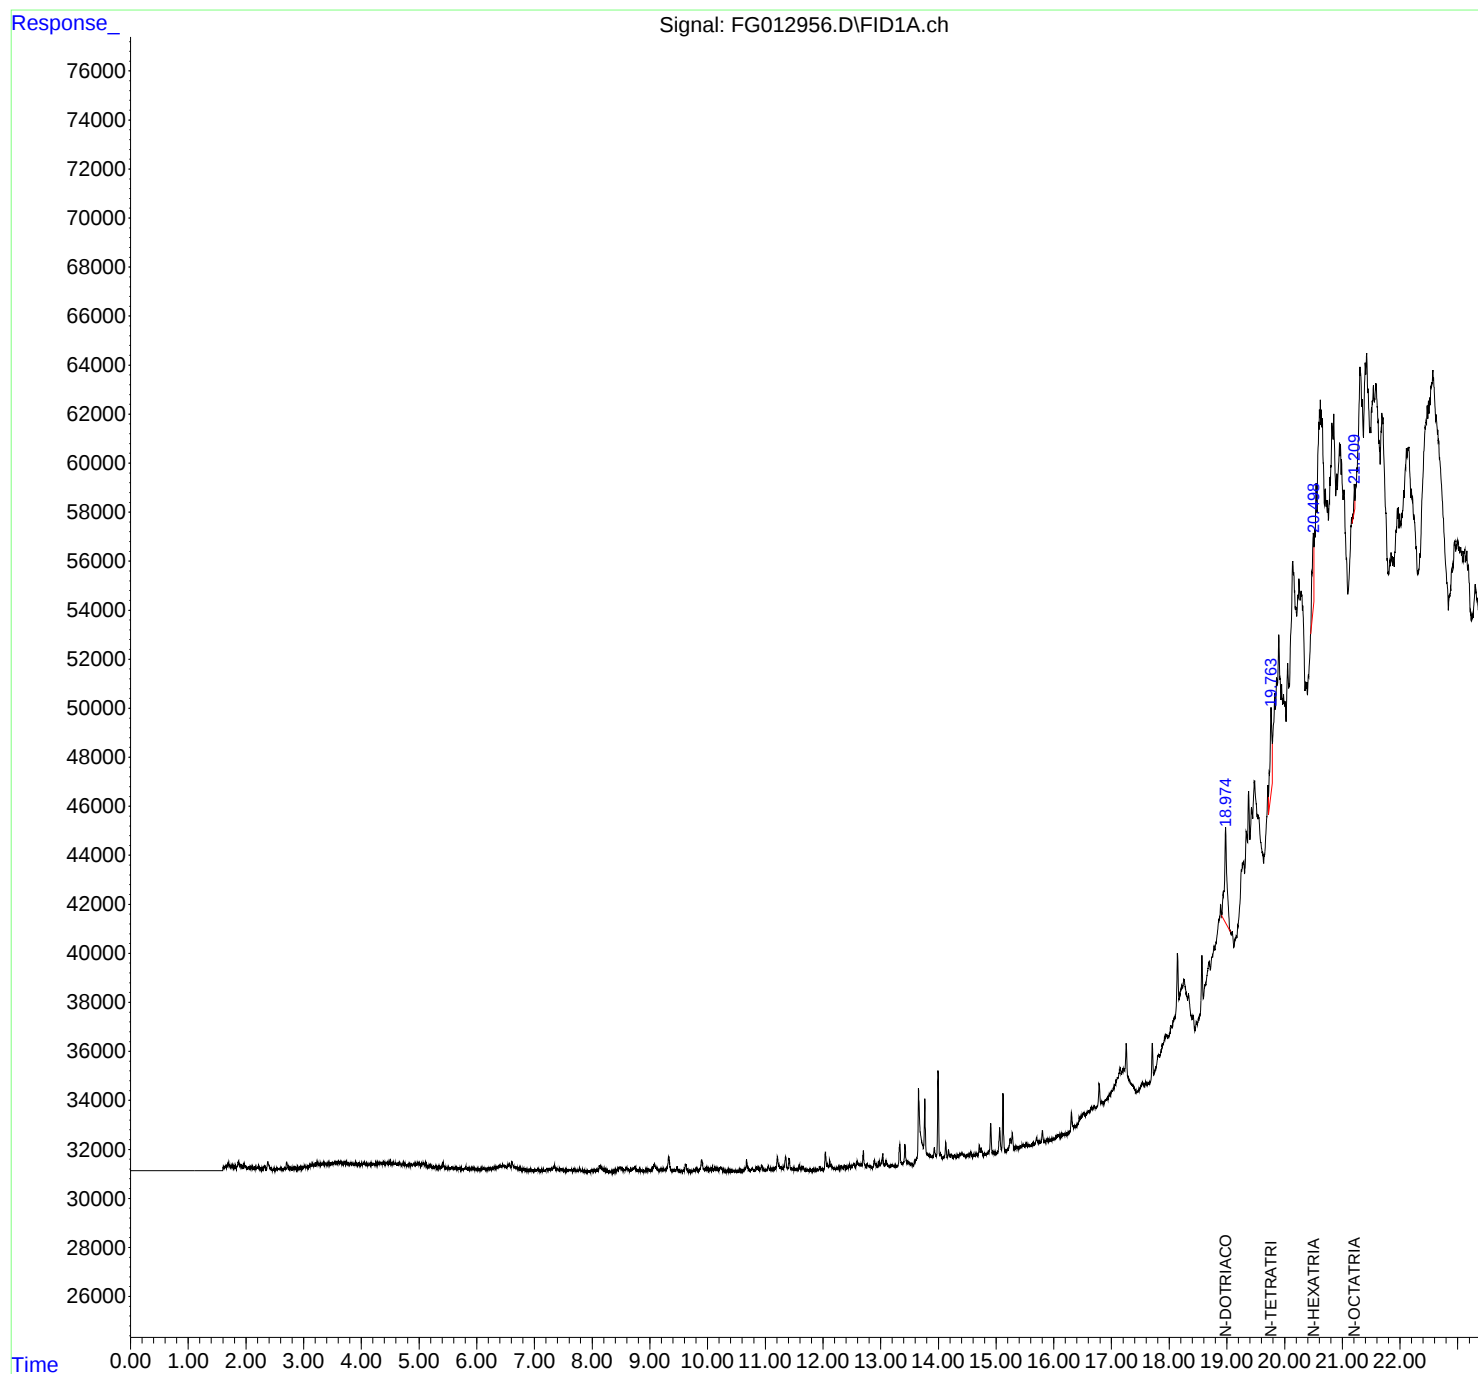


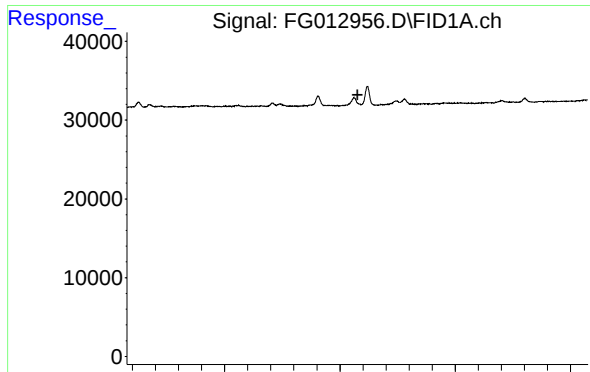

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 0.000 min
Exp R.T.: 15.076 min
Response: 0
Conc: N.D.

Instrument :
FID_G
ClientSampleId :

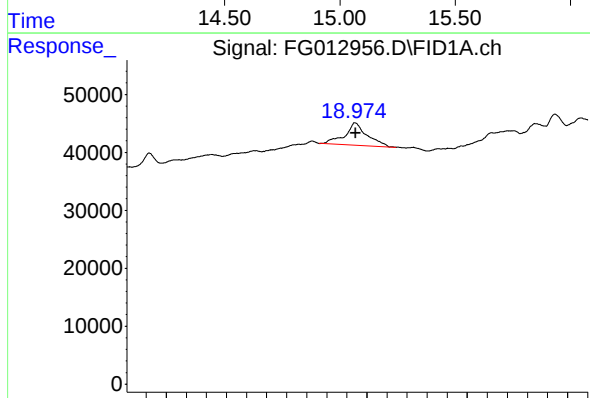


#14 N-DOTRIACONTANE

R.T.: 18.976 min
Delta R.T.: -0.001 min
Response: 119724
Conc: 1.08 ug/ml

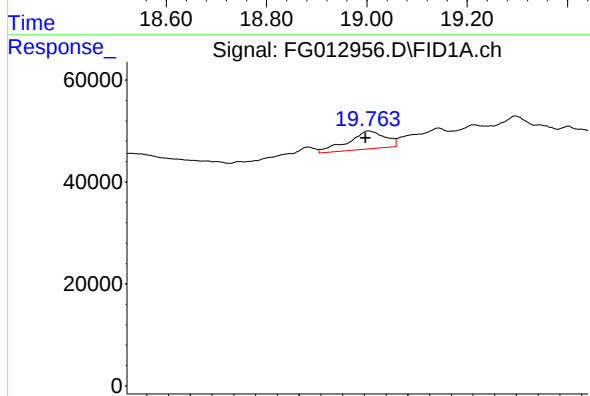


#15 N-TETRATRIACONTANE

R.T.: 19.764 min
Delta R.T.: 0.003 min
Response: 84571
Conc: 0.90 ug/ml

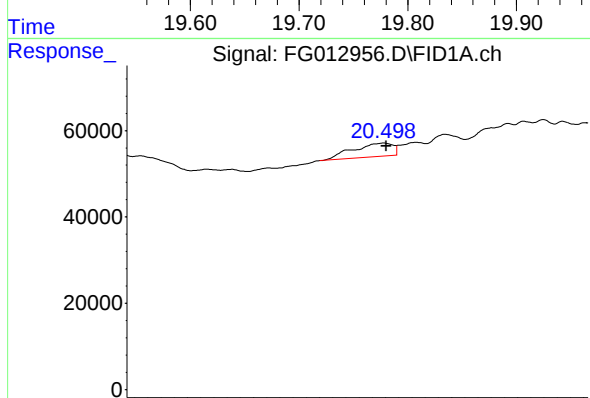

#16 N-HEXATRIACONTANE

R.T.: 20.499 min
Delta R.T.: -0.002 min
Response: 65336
Conc: 0.88 ug/ml

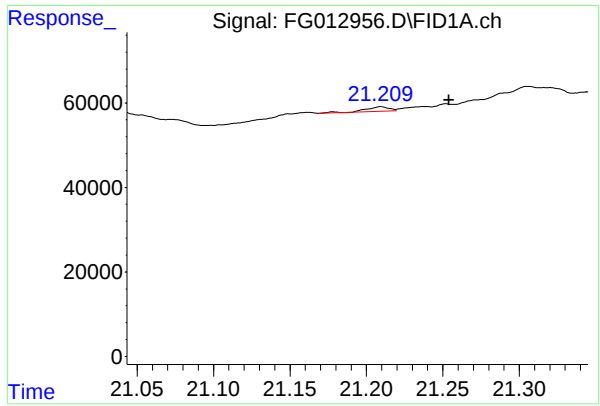

#17 N-OCTATRIACONTANE

R.T.: 21.210 min
Delta R.T.: -0.044 min
Response: 11901
Conc: 0.18 ug/ml

Instrument :
FID_G
ClientSampleId :