

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG093019\
 Data File : FG006088.D
 Signal(s) : FID1A.ch
 Acq On : 30 Sep 2019 12:08
 Operator : DD\AJ
 Sample : K5076-06 2X
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :
 SIMW-04-20190926

Integration File: autoint1.e
 Quant Time: Oct 01 02:15:59 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG090719.M
 Quant Title :
 QLast Update : Mon Sep 09 05:03:58 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.720	1050816	9.353 ug/ml
Target Compounds			
4) N-TETRADECANE	8.317f	156351	1.109 ug/ml
10) N-TETRACOSANE	14.923	301383	2.363 ug/ml
11) N-HEXACOSANE	15.948	390001	3.183 ug/ml
12) N-OCTACOSANE	16.902	651926	5.528 ug/ml
13) N-TRIACONTANE	17.792	758722	6.696 ug/ml
14) N-DOTRIACONTANE	18.630	449348	4.198 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG093019\
Data File : FG006088.D
Signal(s) : FID1A.ch
Acq On : 30 Sep 2019 12:08
Operator : DD\AJ
Sample : K5076-06 2X
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
SIMW-04-20190926

Integration File: autoint1.e
Quant Time: Oct 01 02:15:59 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG090719.M
Quant Title :
QLast Update : Mon Sep 09 05:03:58 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

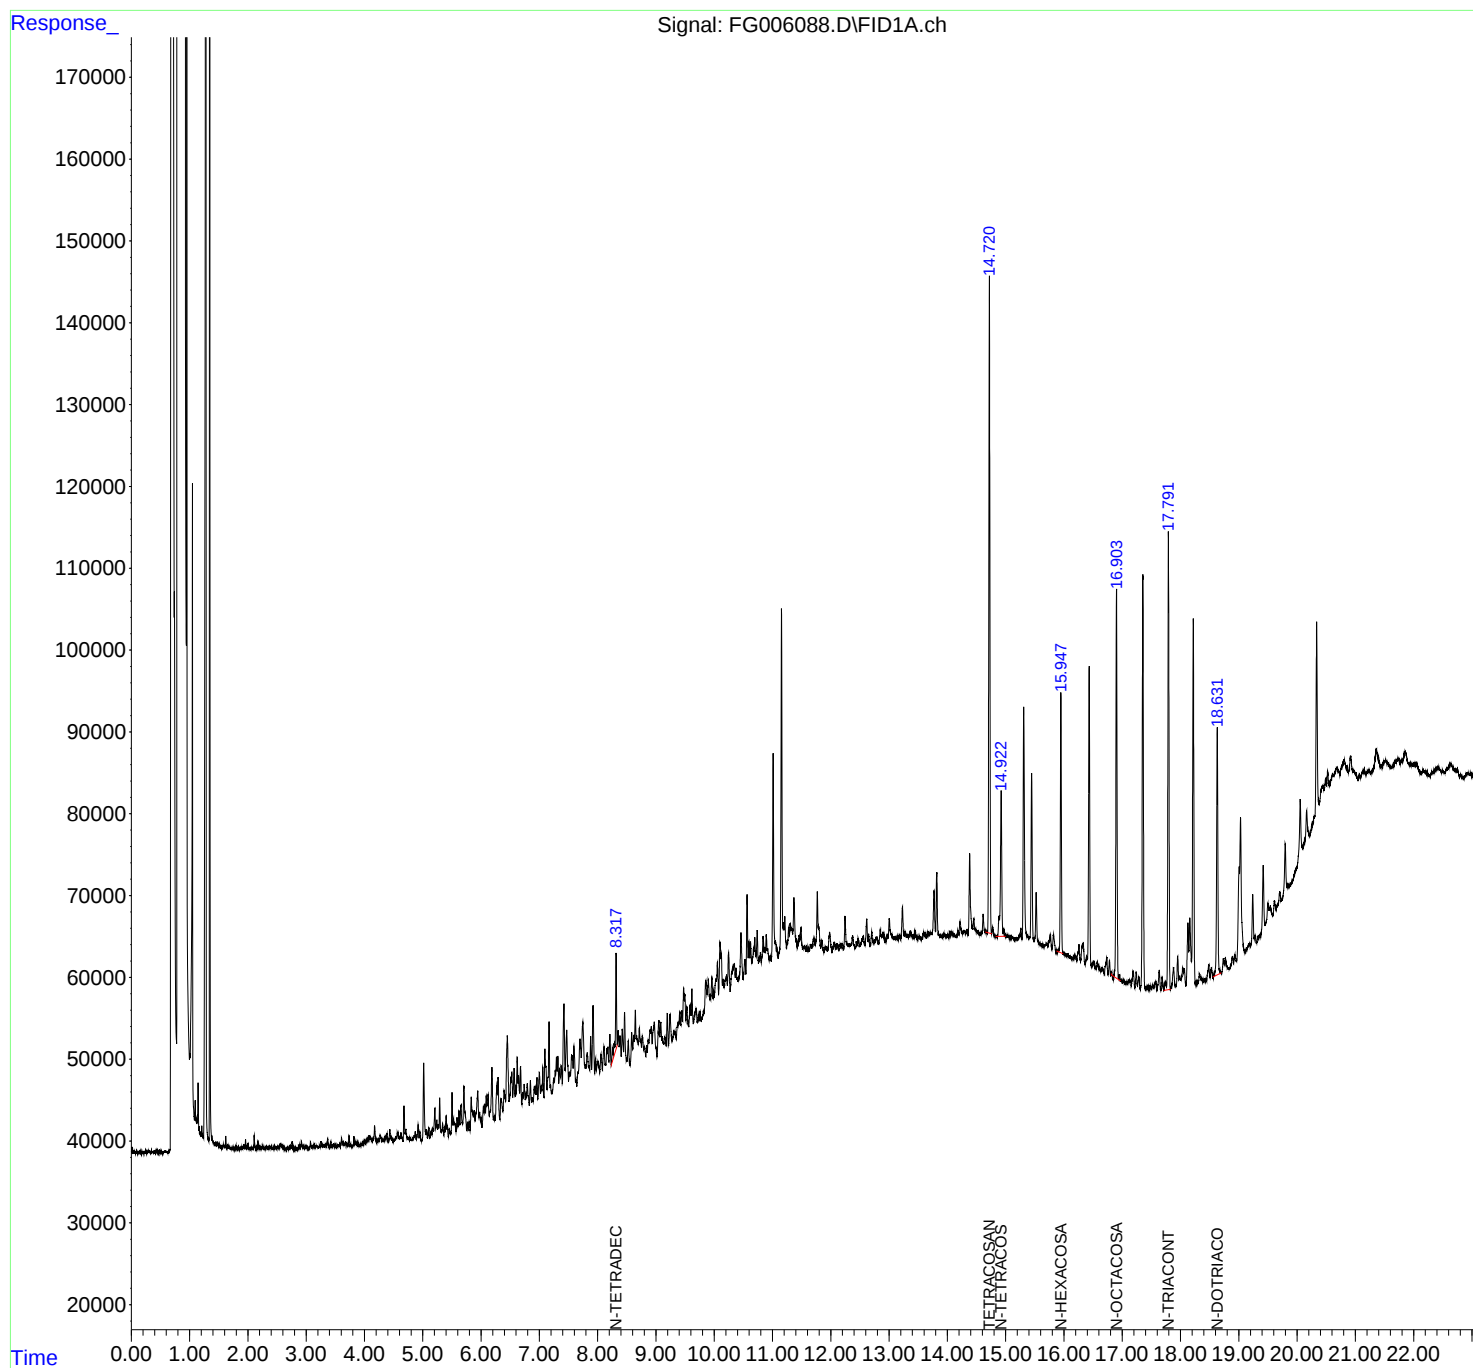


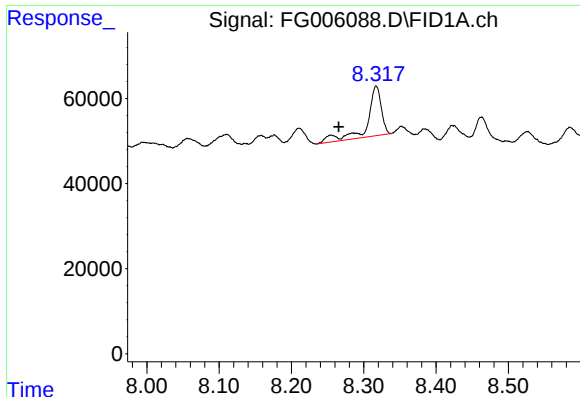

#4 N-TETRADECANE


R.T.: 8.317 min
Delta R.T.: 0.052 min
Response: 156351
Conc: 1.11 ug/ml

Instrument :
FID_G
ClientSampleId :
SIMW-04-20190926

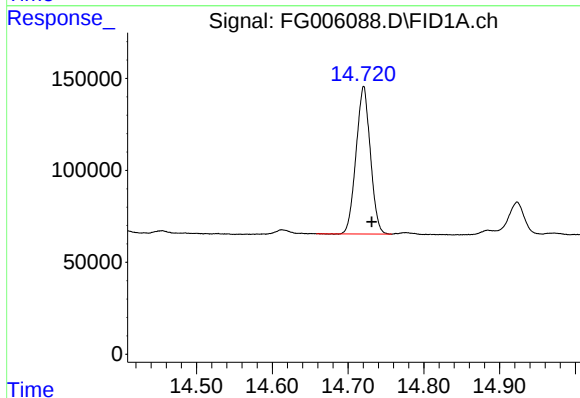


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.720 min
Delta R.T.: -0.011 min
Response: 1050816
Conc: 9.35 ug/ml

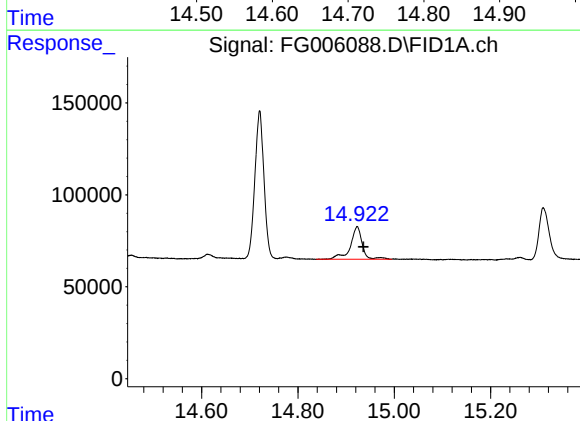


#10 N-TETRACOSANE

R.T.: 14.923 min
Delta R.T.: -0.013 min
Response: 301383
Conc: 2.36 ug/ml

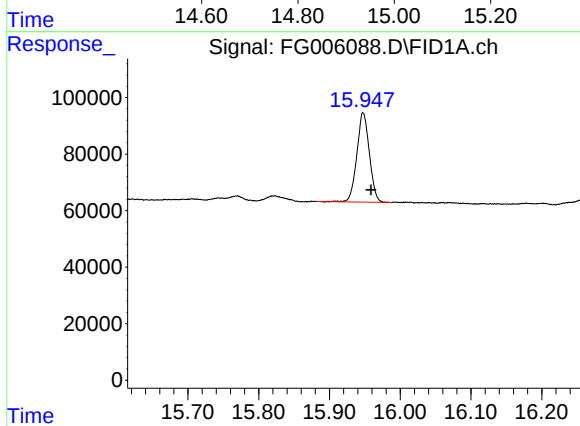

#11 N-HEXACOSANE


R.T.: 15.948 min
Delta R.T.: -0.011 min
Response: 390001
Conc: 3.18 ug/ml

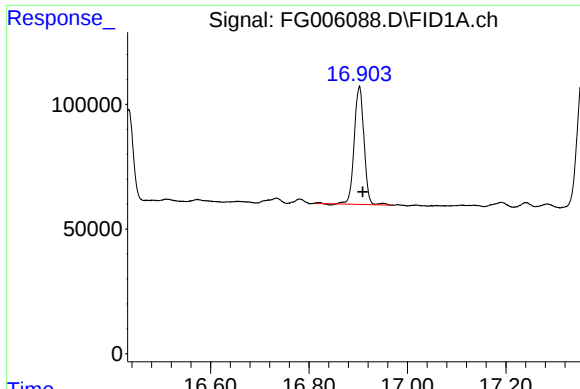

#12 N-OCTACOSANE


R.T.: 16.902 min
Delta R.T.: -0.007 min
Response: 651926
Conc: 5.53 ug/ml

Instrument :
FID_G
ClientSampleId :
SIMW-04-20190926

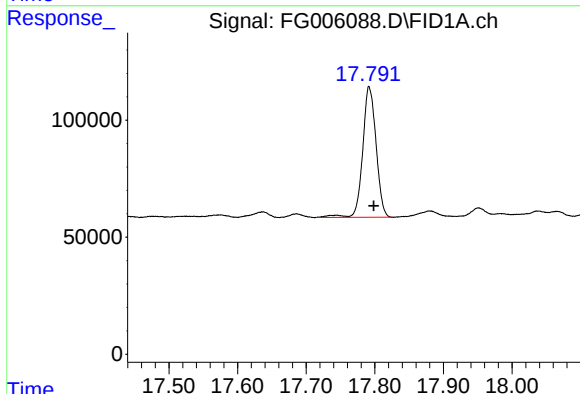

#13 N-TRIACONTANE

R.T.: 17.792 min
Delta R.T.: -0.007 min
Response: 758722
Conc: 6.70 ug/ml

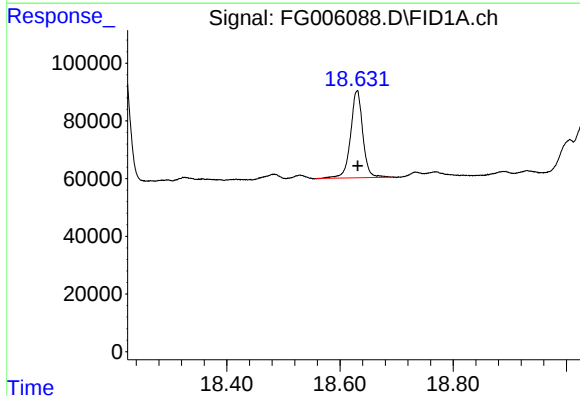

#14 N-DOTRIACONTANE

R.T.: 18.630 min
Delta R.T.: -0.002 min
Response: 449348
Conc: 4.20 ug/ml