

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG093019\
 Data File : FG006106.D
 Signal(s) : FID1A.ch
 Acq On : 30 Sep 2019 21:51
 Operator : DD\AJ
 Sample : K5093-06 2X
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Oct 01 02:20:10 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG090719.M
 Quant Title :
 QLast Update : Mon Sep 09 05:03:58 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.720	1085488	9.662 ug/ml
Target Compounds			
4) N-TETRADECANE	8.318f	188924	1.340 ug/ml
7) N-EICOSANE	12.697f	705689	5.197 ug/ml
10) N-TETRACOSANE	14.930	727735	5.706 ug/ml
12) N-OCTACOSANE	16.900	346706	2.940 ug/ml
13) N-TRIACONTANE	17.794	878350	7.752 ug/ml
14) N-DOTRIACONTANE	18.627	635161	5.935 ug/ml
15) N-TETRATRIACONTANE	19.454	210649	2.036 ug/ml
16) N-HEXATRIACONTANE	20.160	166774	1.674 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG093019\
Data File : FG006106.D
Signal(s) : FID1A.ch
Acq On : 30 Sep 2019 21:51
Operator : DD\AJ
Sample : K5093-06 2X
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
FID_G
ClientSampled :

Integration File: autoint1.e
Quant Time: Oct 01 02:20:10 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG090719.M
Quant Title :
QLast Update : Mon Sep 09 05:03:58 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

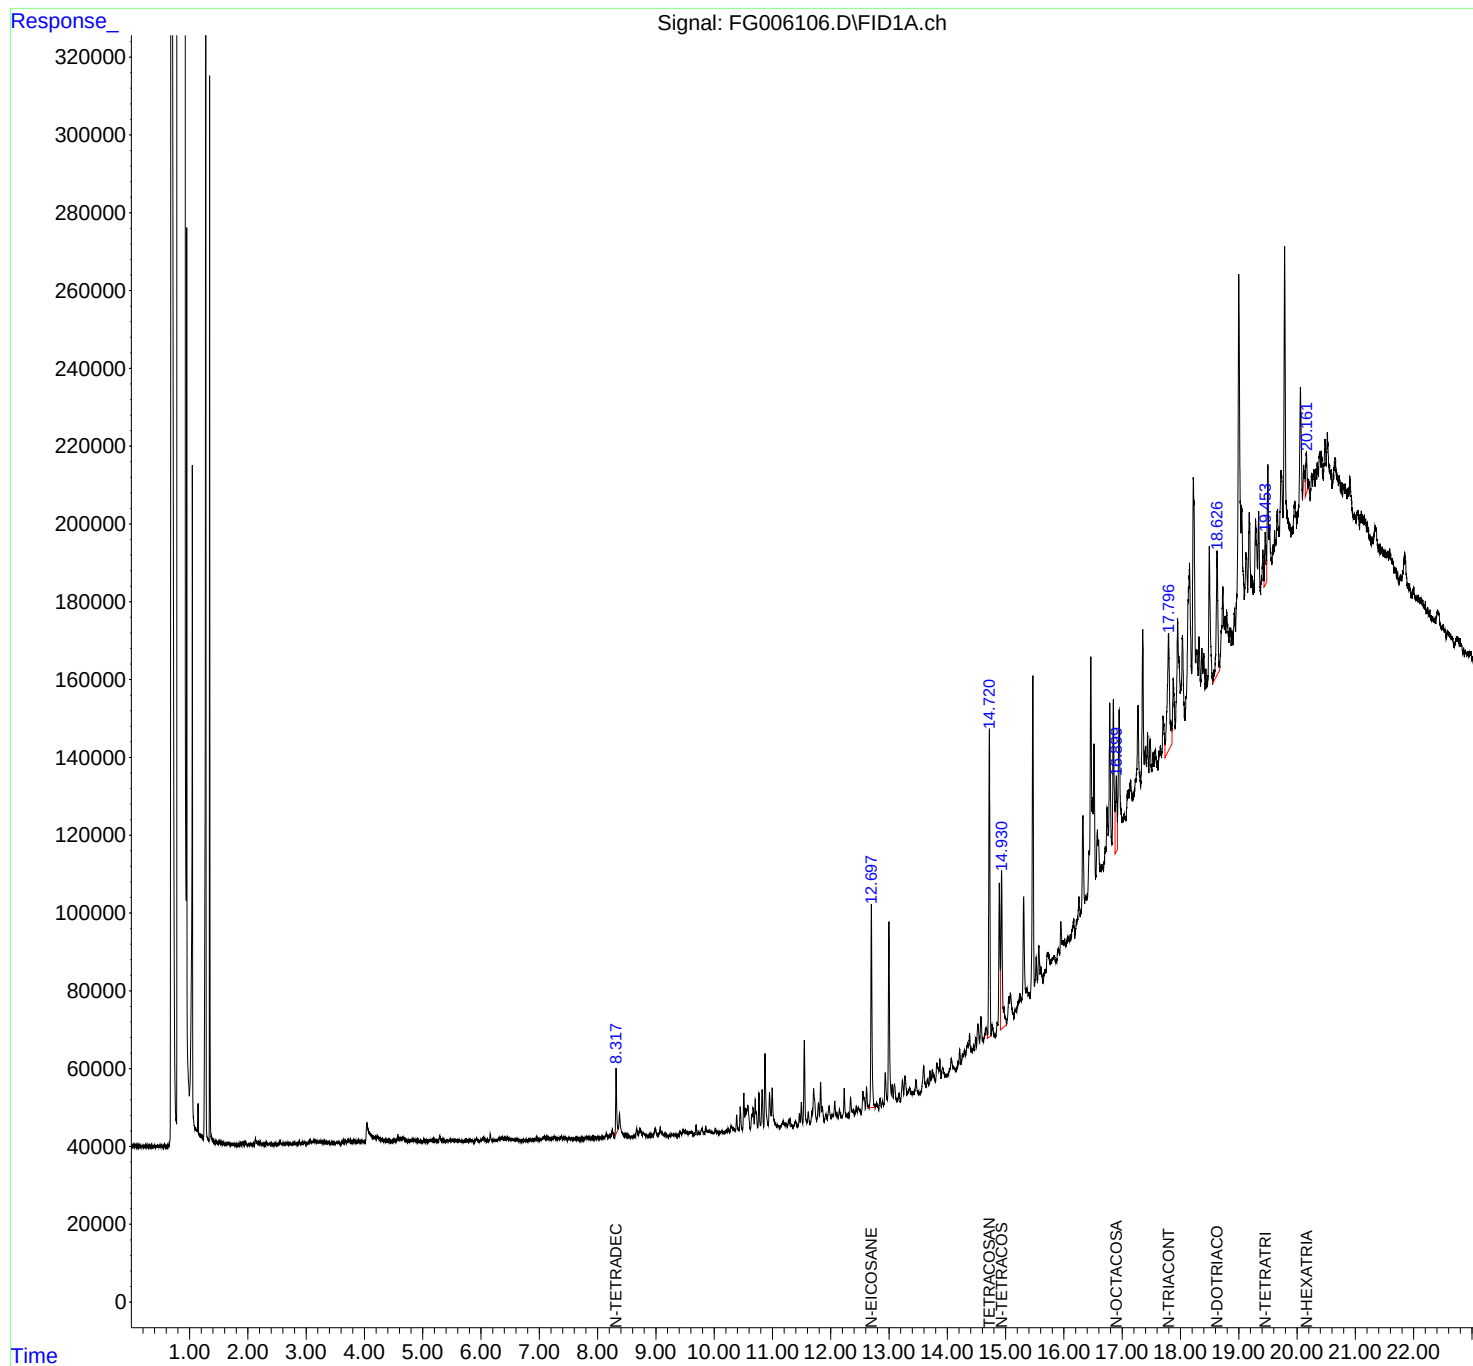


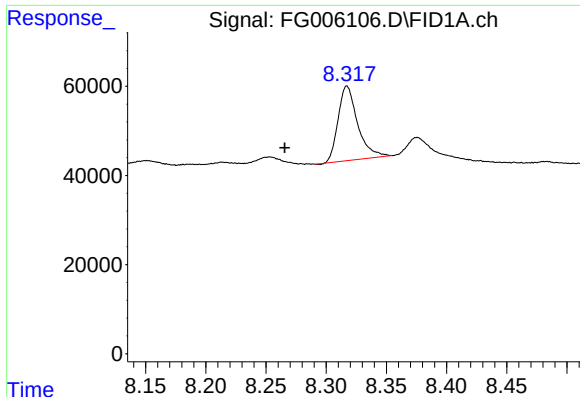

#4 N-TETRADECANE


R.T.: 8.318 min
Delta R.T.: 0.052 min
Response: 188924
Conc: 1.34 ug/ml

Instrument :
FID_G
ClientSampleId :

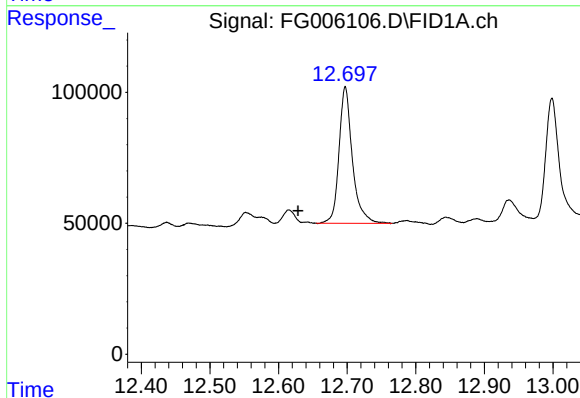


#7 N-EICOSANE

R.T.: 12.697 min
Delta R.T.: 0.069 min
Response: 705689
Conc: 5.20 ug/ml

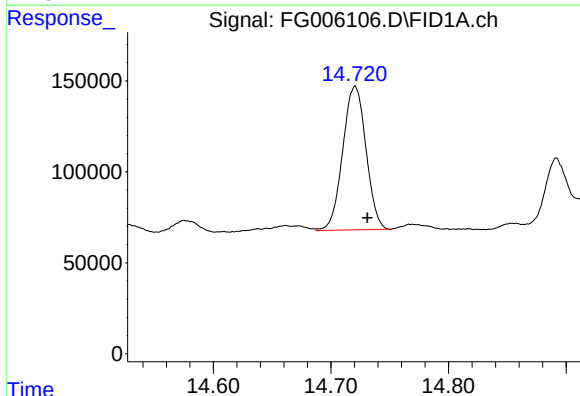


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.720 min
Delta R.T.: -0.011 min
Response: 1085488
Conc: 9.66 ug/ml

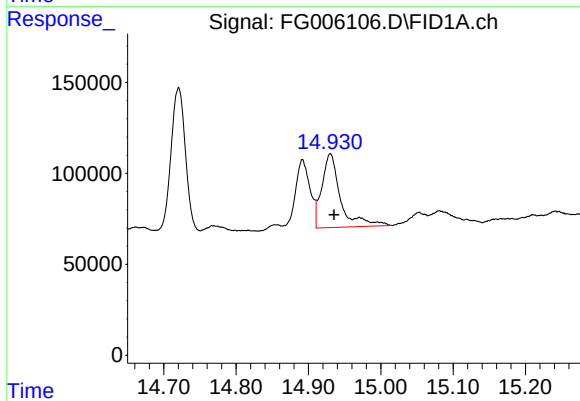

#10 N-TETRACOSANE


R.T.: 14.930 min
Delta R.T.: -0.005 min
Response: 727735
Conc: 5.71 ug/ml

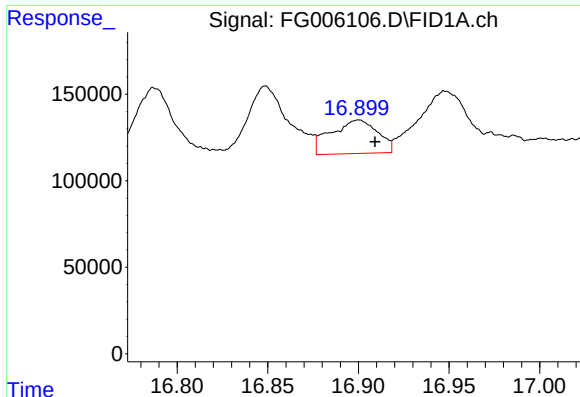

#12 N-OCTACOSANE


R.T.: 16.900 min
Delta R.T.: -0.009 min
Response: 346706
Conc: 2.94 ug/ml

Instrument :
FID_G
ClientSampleId :

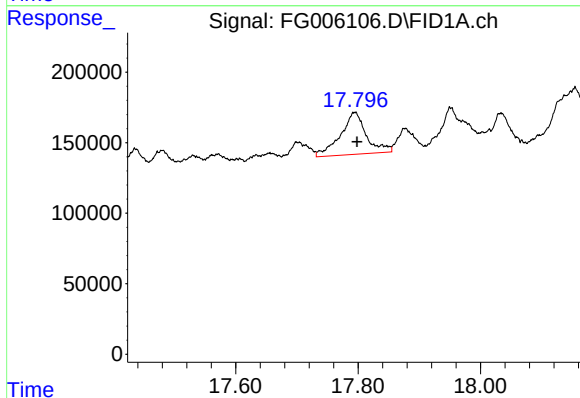


#13 N-TRIACONTANE

R.T.: 17.794 min
Delta R.T.: -0.004 min
Response: 878350
Conc: 7.75 ug/ml

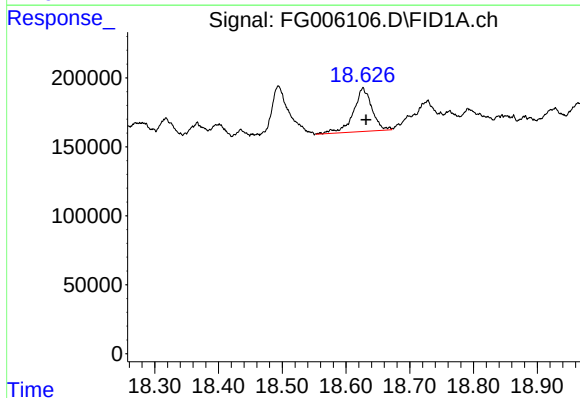


#14 N-DOTRIACONTANE

R.T.: 18.627 min
Delta R.T.: -0.005 min
Response: 635161
Conc: 5.93 ug/ml

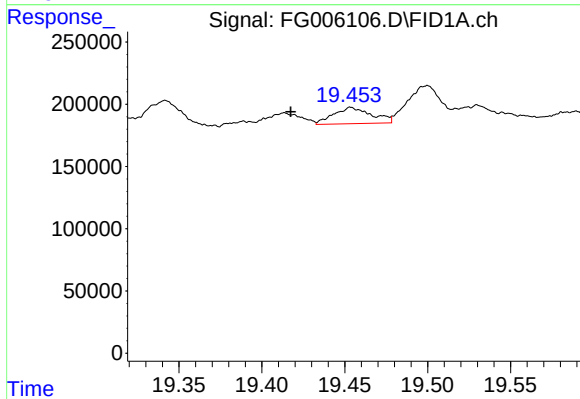

#15 N-TETRATRIACONTANE

R.T.: 19.454 min
Delta R.T.: 0.037 min
Response: 210649
Conc: 2.04 ug/ml

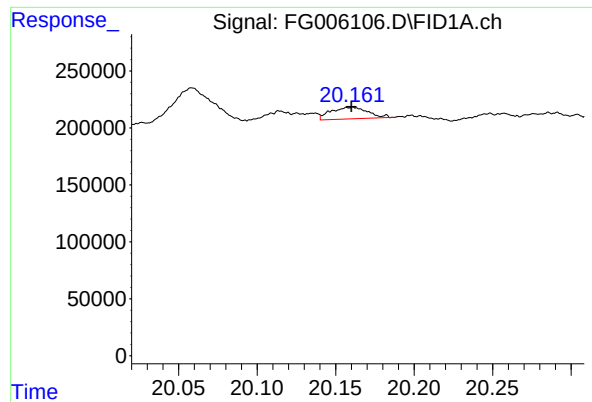

#16 N-HEXATRIACONTANE

R.T.: 20.160 min
Delta R.T.: 0.000 min
Response: 166774
Conc: 1.67 ug/ml

Instrument :
FID_G
ClientSampleId :