

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG093019\
 Data File : FG006107.D
 Signal(s) : FID1A.ch
 Acq On : 30 Sep 2019 22:21
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Oct 01 02:20:23 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG090719.M
 Quant Title :
 QLast Update : Mon Sep 09 05:03:58 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.720	1892457	16.845 ug/ml
Target Compounds			
14) N-DOTRIACONTANE	18.623	81144	0.758 ug/ml
15) N-TETRATRIACONTANE	19.413	123055	1.190 ug/ml
16) N-HEXATRIACONTANE	20.161	306288	3.074 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG093019\
Data File : FG006107.D
Signal(s) : FID1A.ch
Acq On : 30 Sep 2019 22:21
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Oct 01 02:20:23 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG090719.M
Quant Title :
QLast Update : Mon Sep 09 05:03:58 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

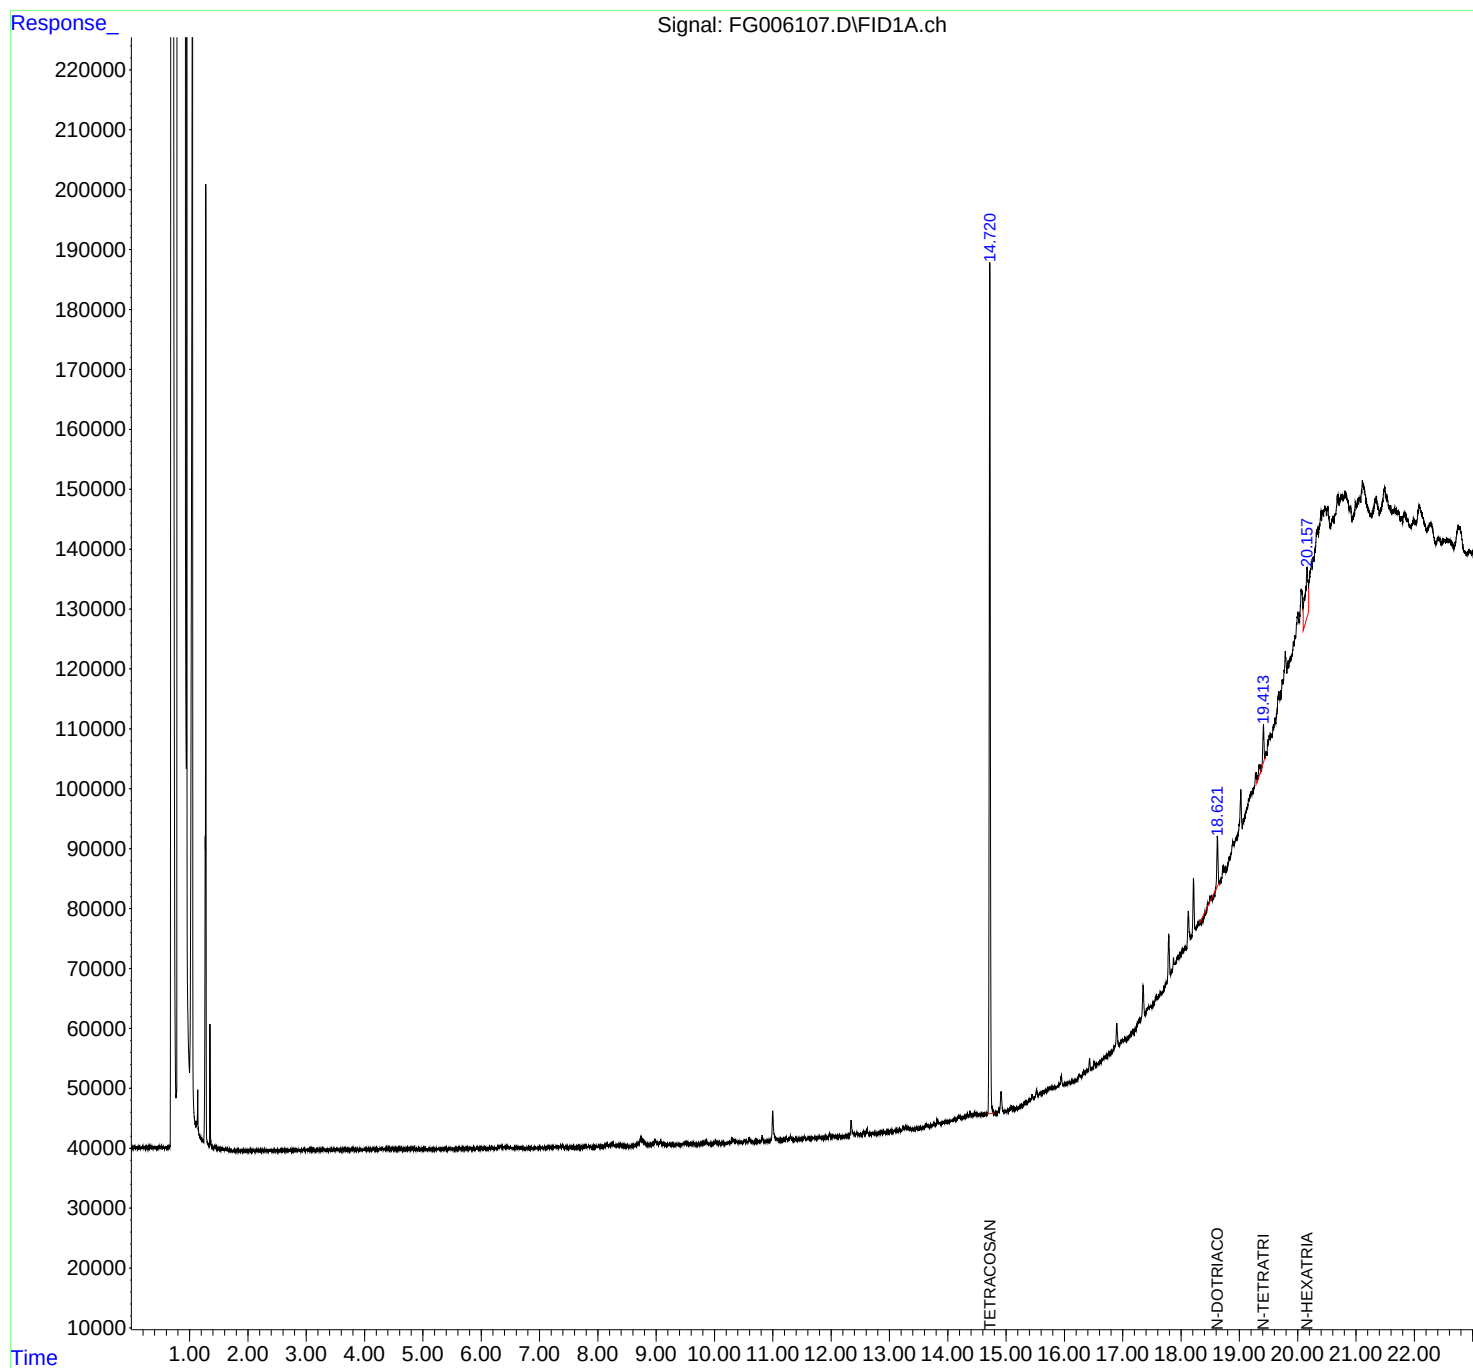


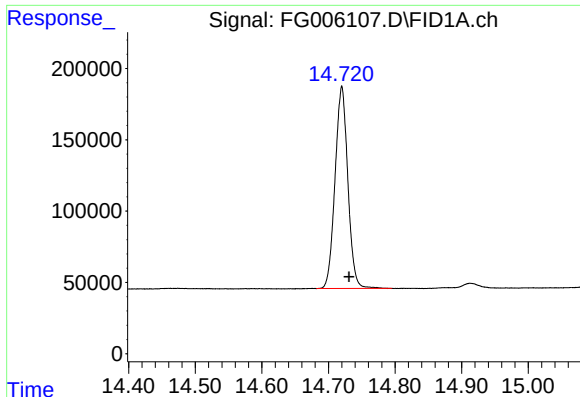

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.720 min
Delta R.T.: -0.011 min
Response: 1892457
Conc: 16.84 ug/ml

Instrument :
FID_G
ClientSampleId :

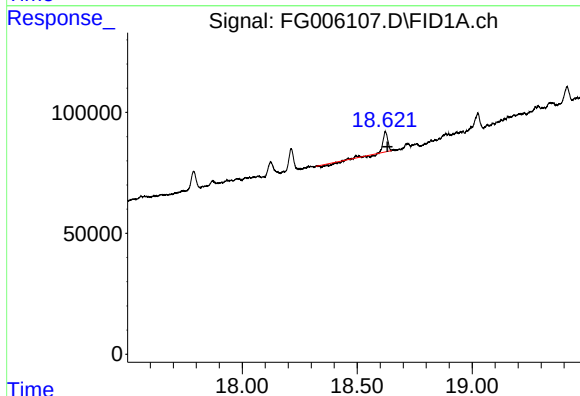


#14 N-DOTRIACONTANE

R.T.: 18.623 min
Delta R.T.: -0.009 min
Response: 81144
Conc: 0.76 ug/ml

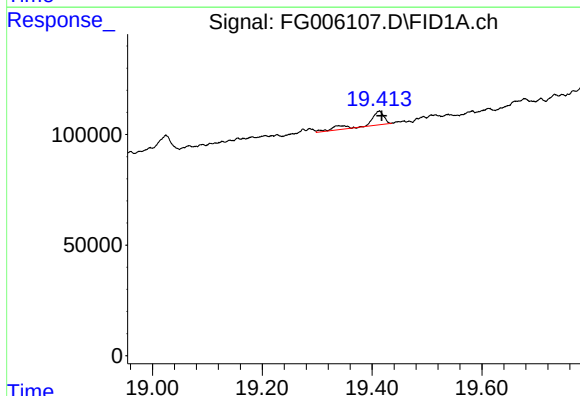

#15 N-TETRATRIACONTANE

R.T.: 19.413 min
Delta R.T.: -0.005 min
Response: 123055
Conc: 1.19 ug/ml

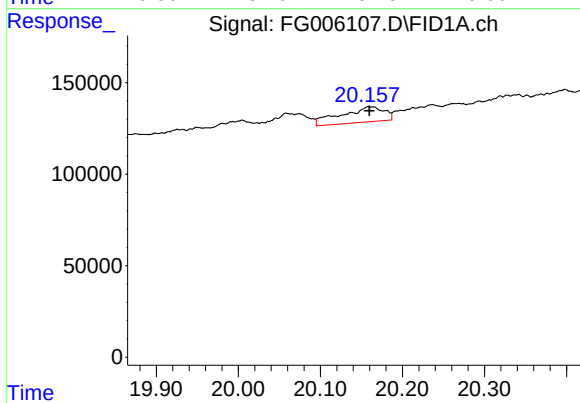

#16 N-HEXATRIACONTANE

R.T.: 20.161 min
Delta R.T.: 0.001 min
Response: 306288
Conc: 3.07 ug/ml