

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG093019\
 Data File : FG006102.D
 Signal(s) : FID1A.ch
 Acq On : 30 Sep 2019 19:52
 Operator : DD\AJ
 Sample : PB123462BS
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :
 PB123462BS

Integration File: autoint1.e
 Quant Time: Oct 01 02:19:15 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG090719.M
 Quant Title :
 QLast Update : Mon Sep 09 05:03:58 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.720	1776151	15.809 ug/ml
Target Compounds			
2) N-DECANE	4.422	2146915	15.297 ug/ml
3) N-DODECANE	6.449	2142751	15.134 ug/ml
4) N-TETRADECANE	8.250	2073784	14.708 ug/ml
5) N-HEXADECANE	9.857	2047044	14.566 ug/ml
6) N-OCTADECANE	11.303	2004962	14.619 ug/ml
7) N-EICOSANE	12.616	1964476	14.468 ug/ml
8) N-DOCOSANE	13.818	1934915	14.710 ug/ml
10) N-TETRACOSANE	14.924	1947849	15.274 ug/ml
11) N-HEXACOSANE	15.948	1923501	15.697 ug/ml
12) N-OCTACOSANE	16.901	1953812	16.568 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG093019\
Data File : FG006102.D
Signal(s) : FID1A.ch
Acq On : 30 Sep 2019 19:52
Operator : DD\AJ
Sample : PB123462BS
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
PB123462BS

Integration File: autoint1.e
Quant Time: Oct 01 02:19:15 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG090719.M
Quant Title :
QLast Update : Mon Sep 09 05:03:58 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

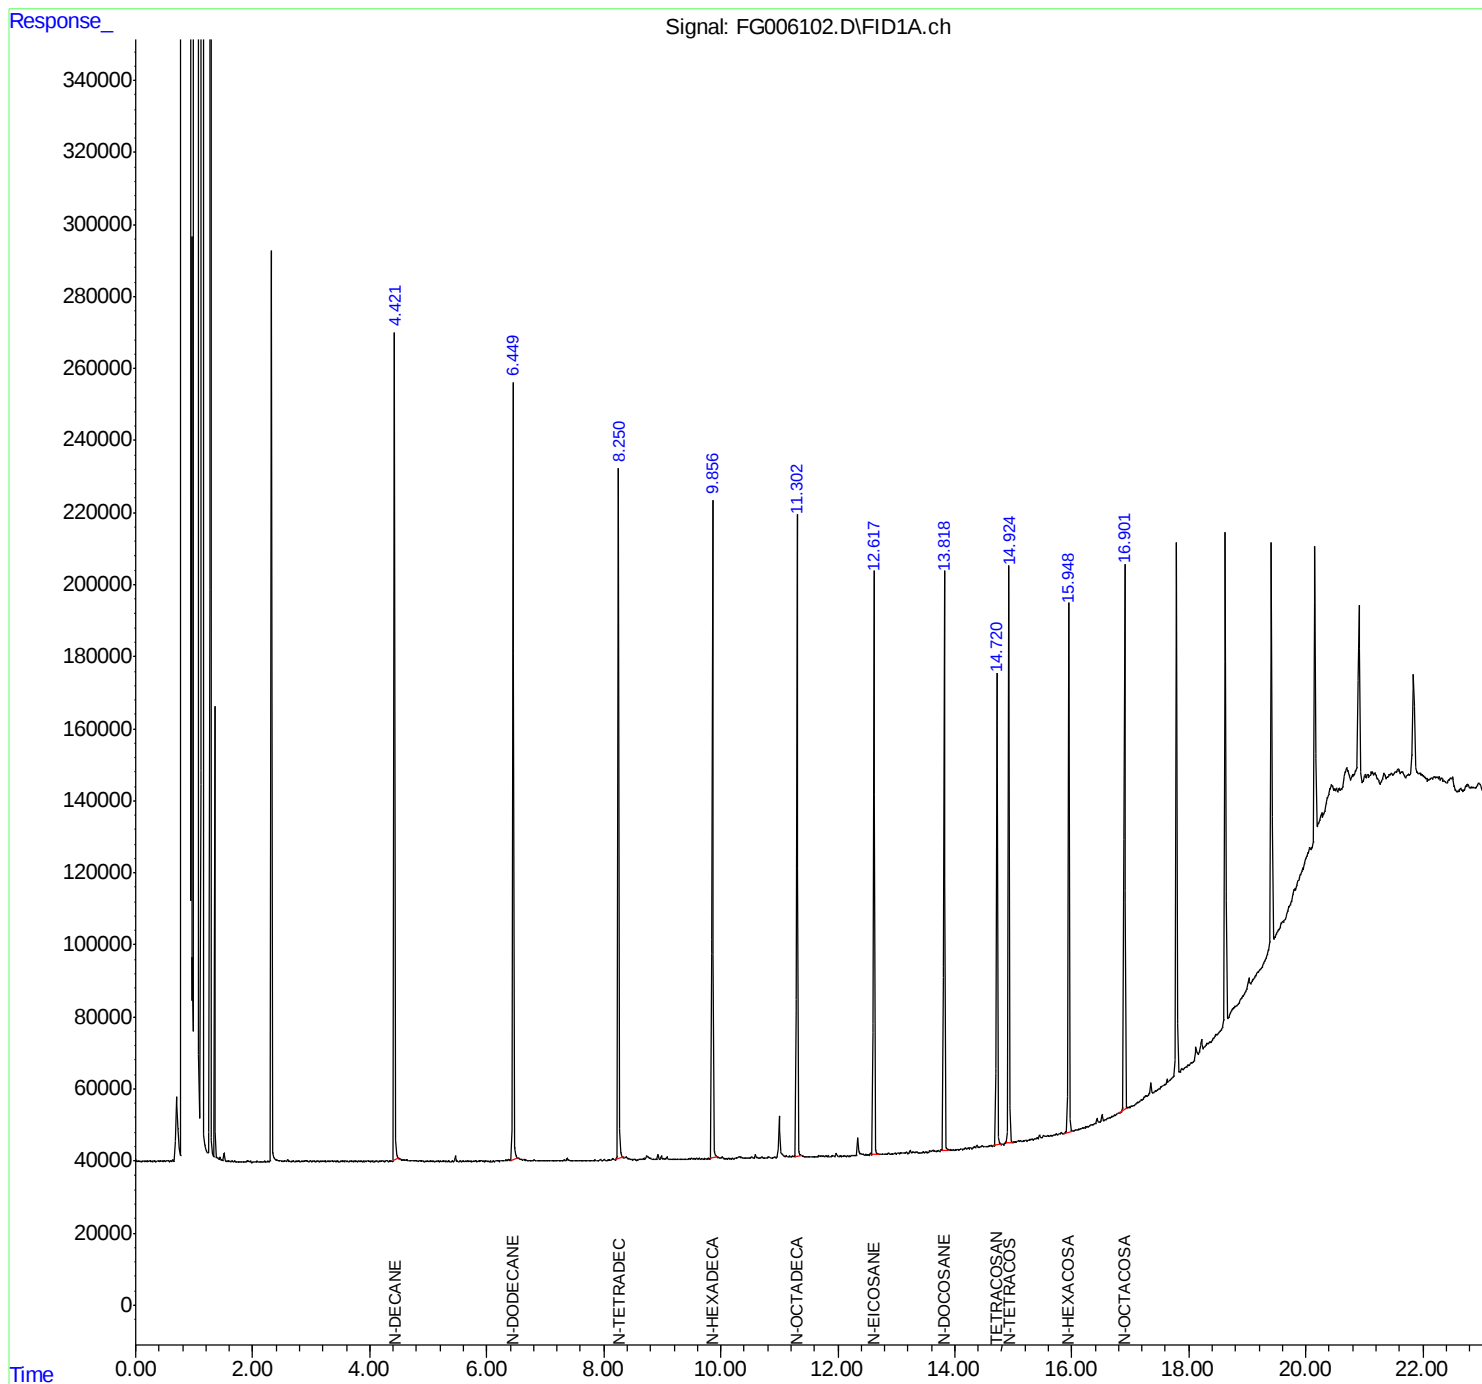


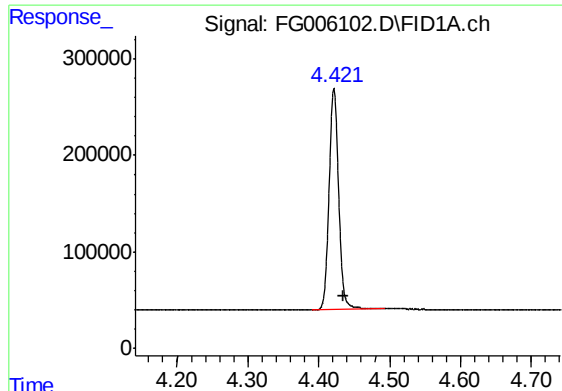

#2 N-DECANE


R.T.: 4.422 min
Delta R.T.: -0.013 min
Response: 2146915
Conc: 15.30 ug/ml

Instrument :
FID_G
ClientSampleId :
PB123462BS

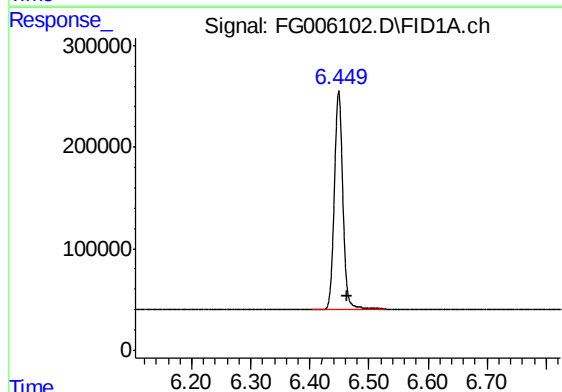


#3 N-DODECANE

R.T.: 6.449 min
Delta R.T.: -0.014 min
Response: 2142751
Conc: 15.13 ug/ml

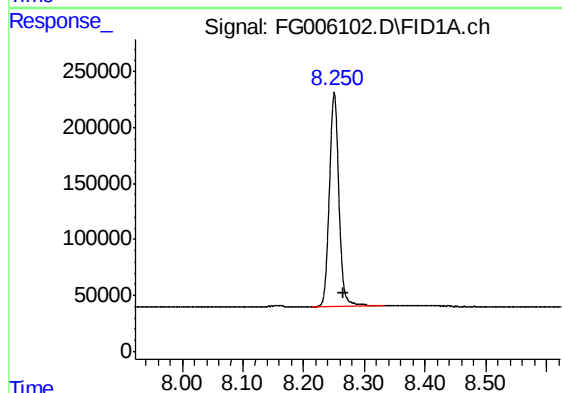


#4 N-TETRADECANE

R.T.: 8.250 min
Delta R.T.: -0.015 min
Response: 2073784
Conc: 14.71 ug/ml

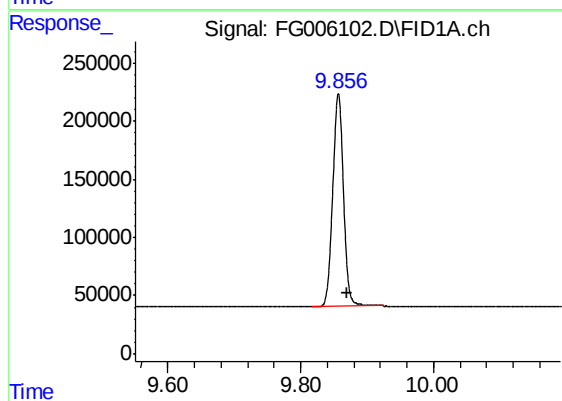

#5 N-HEXADECANE


R.T.: 9.857 min
Delta R.T.: -0.014 min
Response: 2047044
Conc: 14.57 ug/ml

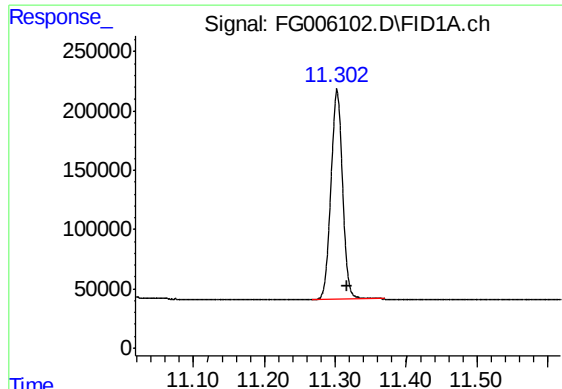

#6 N-OCTADECANE


R.T.: 11.303 min
Delta R.T.: -0.014 min
Response: 2004962
Conc: 14.62 ug/ml

Instrument :
FID_G
ClientSampleId :
PB123462BS

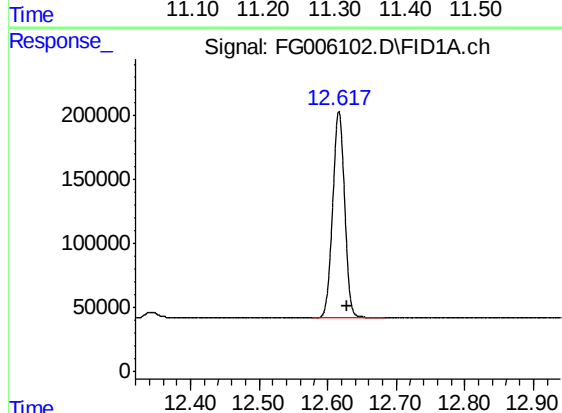


#7 N-EICOSANE

R.T.: 12.616 min
Delta R.T.: -0.012 min
Response: 1964476
Conc: 14.47 ug/ml

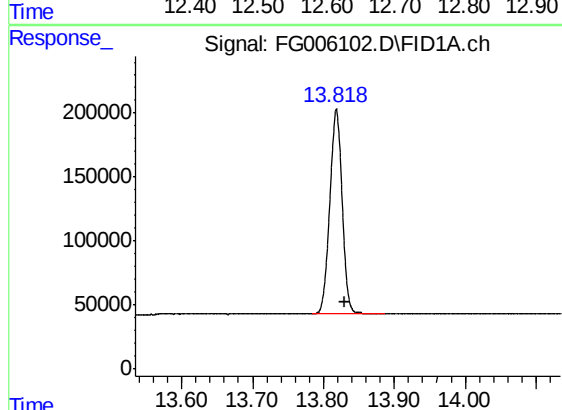


#8 N-DOCOSANE

R.T.: 13.818 min
Delta R.T.: -0.012 min
Response: 1934915
Conc: 14.71 ug/ml

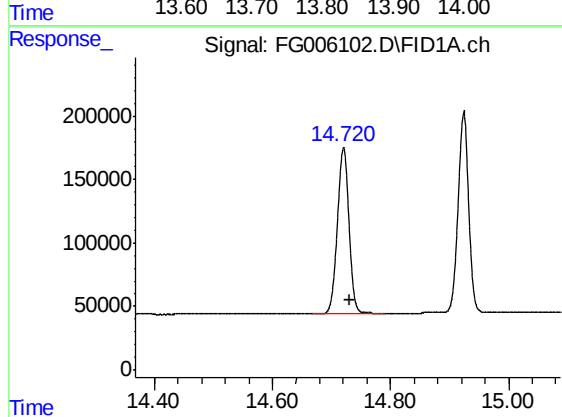

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.720 min
Delta R.T.: -0.011 min
Response: 1776151
Conc: 15.81 ug/ml

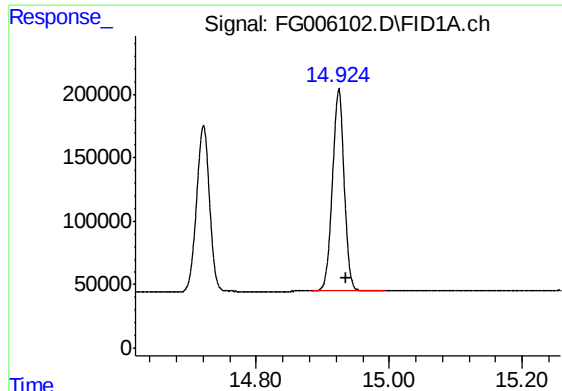

#10 N-TETRACOSANE


R.T.: 14.924 min
Delta R.T.: -0.012 min
Response: 1947849
Conc: 15.27 ug/ml

Instrument :
FID_G
ClientSampleId :
PB123462BS

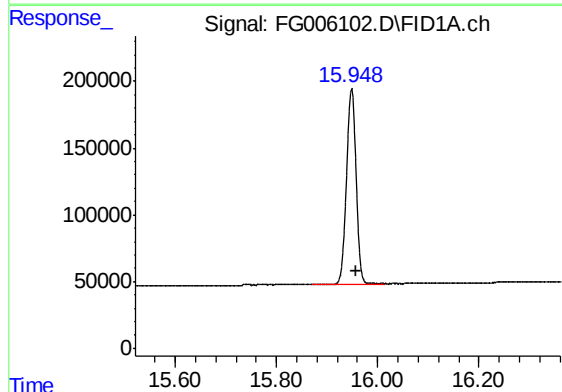

#11 N-HEXACOSANE

R.T.: 15.948 min
Delta R.T.: -0.010 min
Response: 1923501
Conc: 15.70 ug/ml

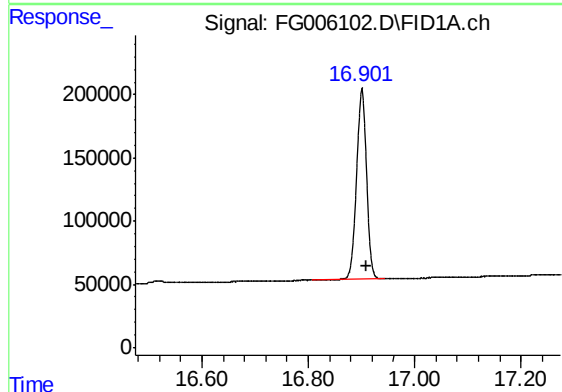

#12 N-OCTACOSANE

R.T.: 16.901 min
Delta R.T.: -0.008 min
Response: 1953812
Conc: 16.57 ug/ml