

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG100118\
 Data File : FG002454.D
 Signal(s) : FID1A.ch
 Acq On : 01 Oct 2018 19:19
 Operator : AJ\SJ
 Sample : J4776-09 10X
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Oct 02 04:22:44 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG100118.M
 Quant Title :
 QLast Update : Mon Oct 01 12:36:17 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
9) S	TETRACOSANE-d50 (SURR...	14.759	149182	1.300 ug/ml
Target Compounds				
7)	N-EICOSANE	12.715f	393234	2.948 ug/ml
10)	N-TETRACOSANE	14.938	195788	1.506 ug/ml
12)	N-OCTACOSANE	16.943	215344	1.698 ug/ml
13)	N-TRIACONTANE	17.837	223725	1.778 ug/ml
14)	N-DOTRIACONTANE	18.671	172751	1.407 ug/ml
15)	N-TETRATRIACONTANE	19.448	33457	0.280 ug/ml
16)	N-HEXATRIACONTANE	20.200	134788	1.215 ug/ml
17)	N-OCTATRIACONTANE	20.965	135745	1.385 ug/ml
18)	N-TETRACONTANE	21.908	280712	3.001 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG100118\
Data File : FG002454.D
Signal(s) : FID1A.ch
Acq On : 01 Oct 2018 19:19
Operator : AJ\SJ
Sample : J4776-09 10X
Misc :
ALS Vial : 14 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Oct 02 04:22:44 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG100118.M
Quant Title :
QLast Update : Mon Oct 01 12:36:17 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

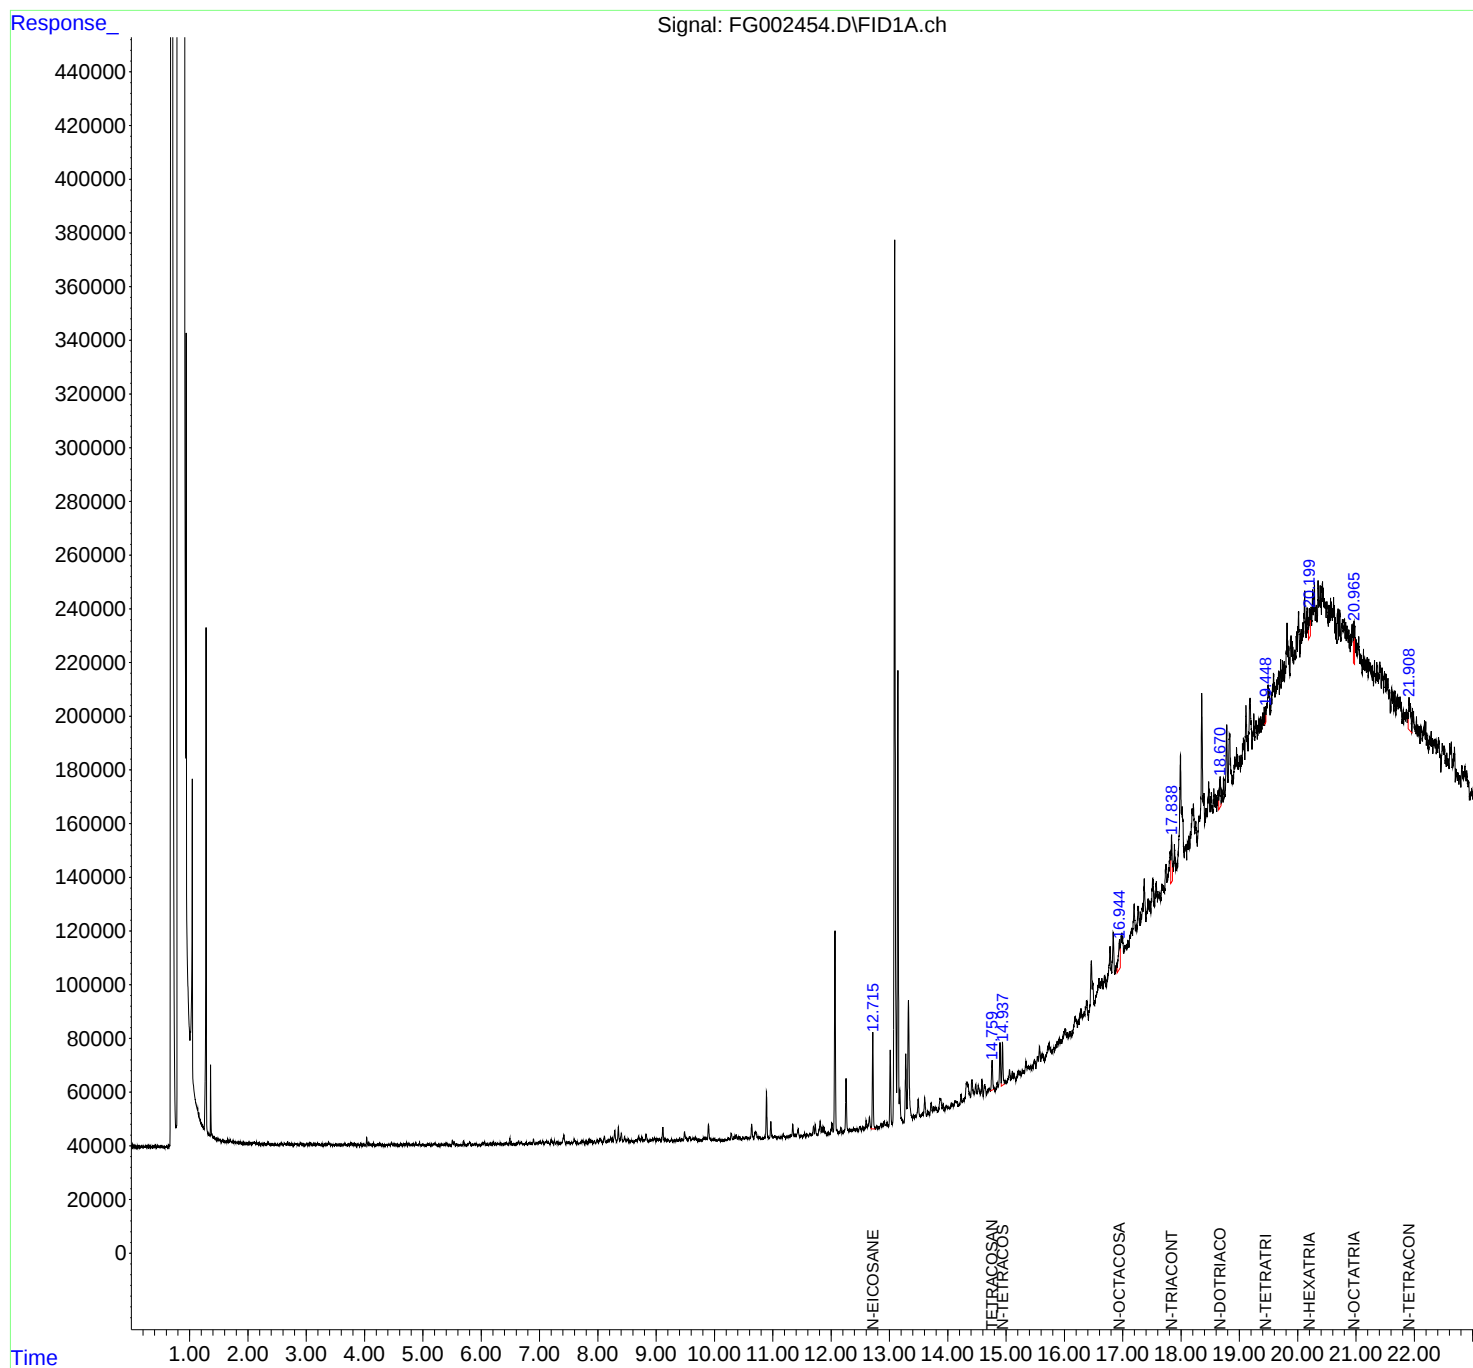

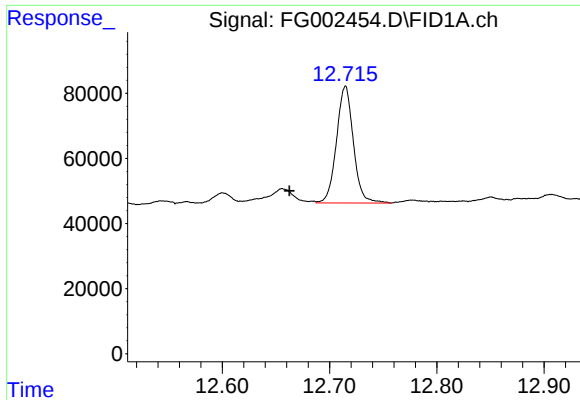


#7 N-EICOSANE

R.T.: 12.715 min
Delta R.T.: 0.052 min
Response: 393234
Conc: 2.95 ug/ml

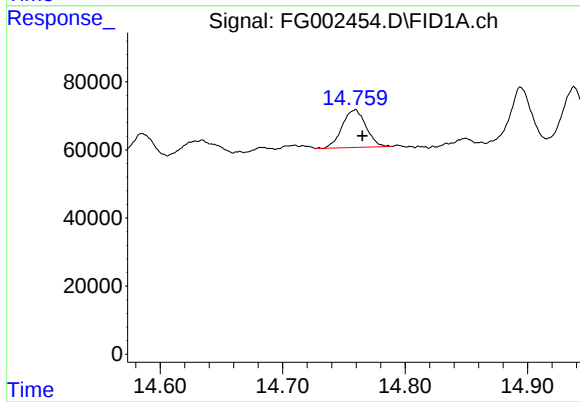


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.759 min
Delta R.T.: -0.006 min
Response: 149182
Conc: 1.30 ug/ml

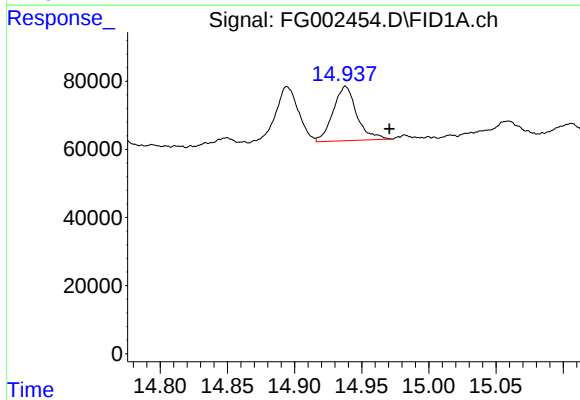


#10 N-TETRACOSANE

R.T.: 14.938 min
Delta R.T.: -0.033 min
Response: 195788
Conc: 1.51 ug/ml

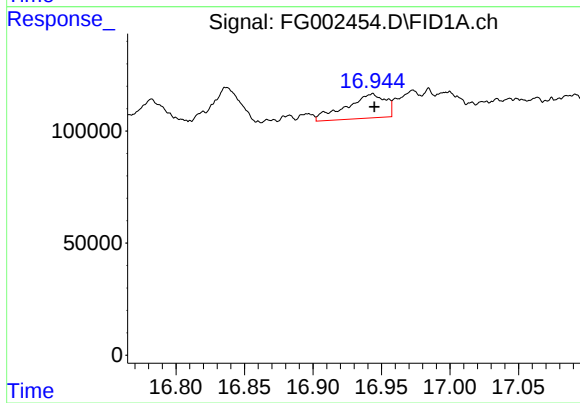


#12 N-OCTACOSANE

R.T.: 16.943 min
Delta R.T.: -0.002 min
Response: 215344
Conc: 1.70 ug/ml

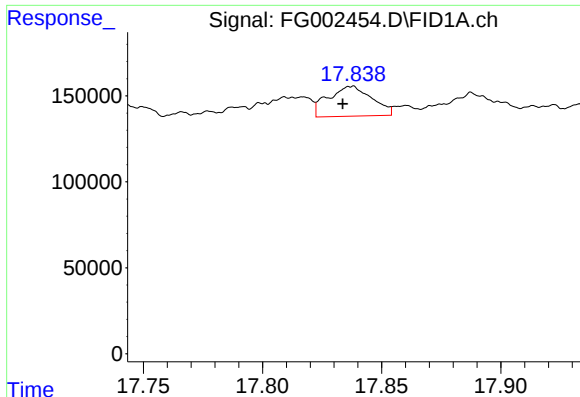


#13 N-TRIACONTANE

R.T.: 17.837 min
Delta R.T.: 0.004 min
Response: 223725
Conc: 1.78 ug/ml

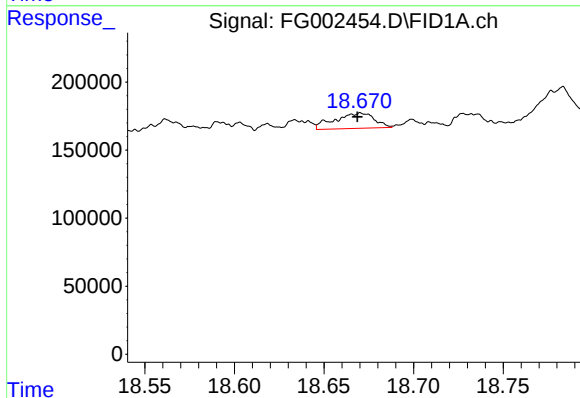


#14 N-DOTRIACONTANE

R.T.: 18.671 min
Delta R.T.: 0.002 min
Response: 172751
Conc: 1.41 ug/ml

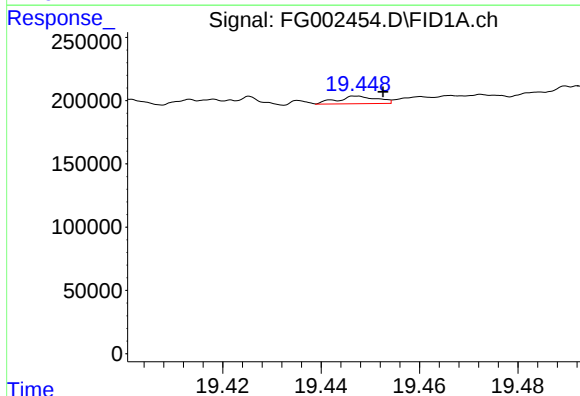


#15 N-TETRATRIACONTANE

R.T.: 19.448 min
Delta R.T.: -0.005 min
Response: 33457
Conc: 0.28 ug/ml

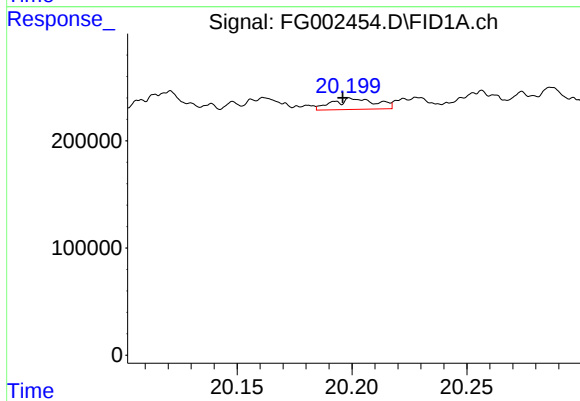


#16 N-HEXATRIACONTANE

R.T.: 20.200 min
Delta R.T.: 0.004 min
Response: 134788
Conc: 1.21 ug/ml

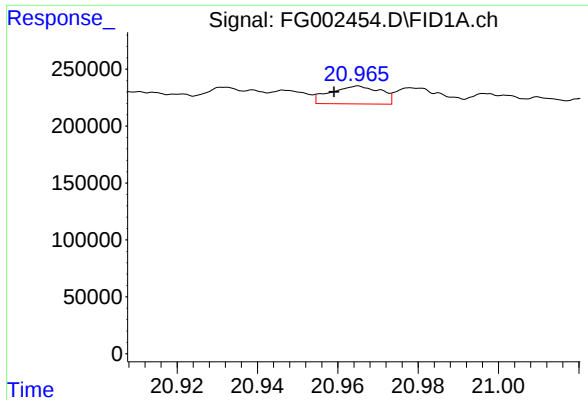

#17 N-OCTATRIACONTANE

R.T.: 20.965 min
Delta R.T.: 0.006 min
Response: 135745
Conc: 1.38 ug/ml

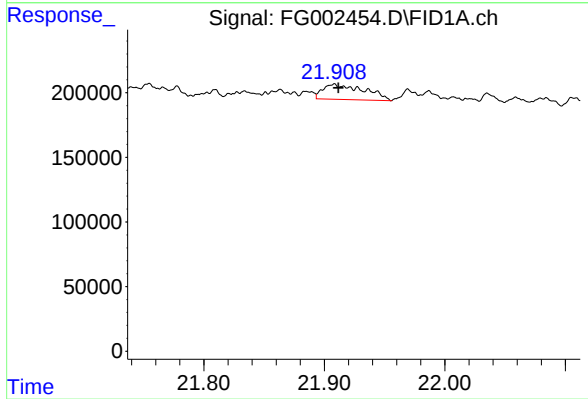

#18 N-TETRACONTANE

R.T.: 21.908 min
Delta R.T.: -0.004 min
Response: 280712
Conc: 3.00 ug/ml