

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG100118\
Data File : FG002456.D
Signal(s) : FID1A.ch
Acq On : 01 Oct 2018 20:20
Operator : AJ\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Oct 02 04:23:08 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG100118.M
Quant Title :
QLast Update : Mon Oct 01 12:36:17 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.761	2209377	19.249 ug/ml
Target Compounds			
13) N-TRIACONTANE	17.830	79690	0.633 ug/ml
14) N-DOTRIACONTANE	18.661	134166	1.093 ug/ml
15) N-TETRATRIACONTANE	19.456	83618	0.701 ug/ml
16) N-HEXATRIACONTANE	20.199	492083	4.435 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG100118\
Data File : FG002456.D
Signal(s) : FID1A.ch
Acq On : 01 Oct 2018 20:20
Operator : AJ\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Oct 02 04:23:08 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG100118.M
Quant Title :
QLast Update : Mon Oct 01 12:36:17 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

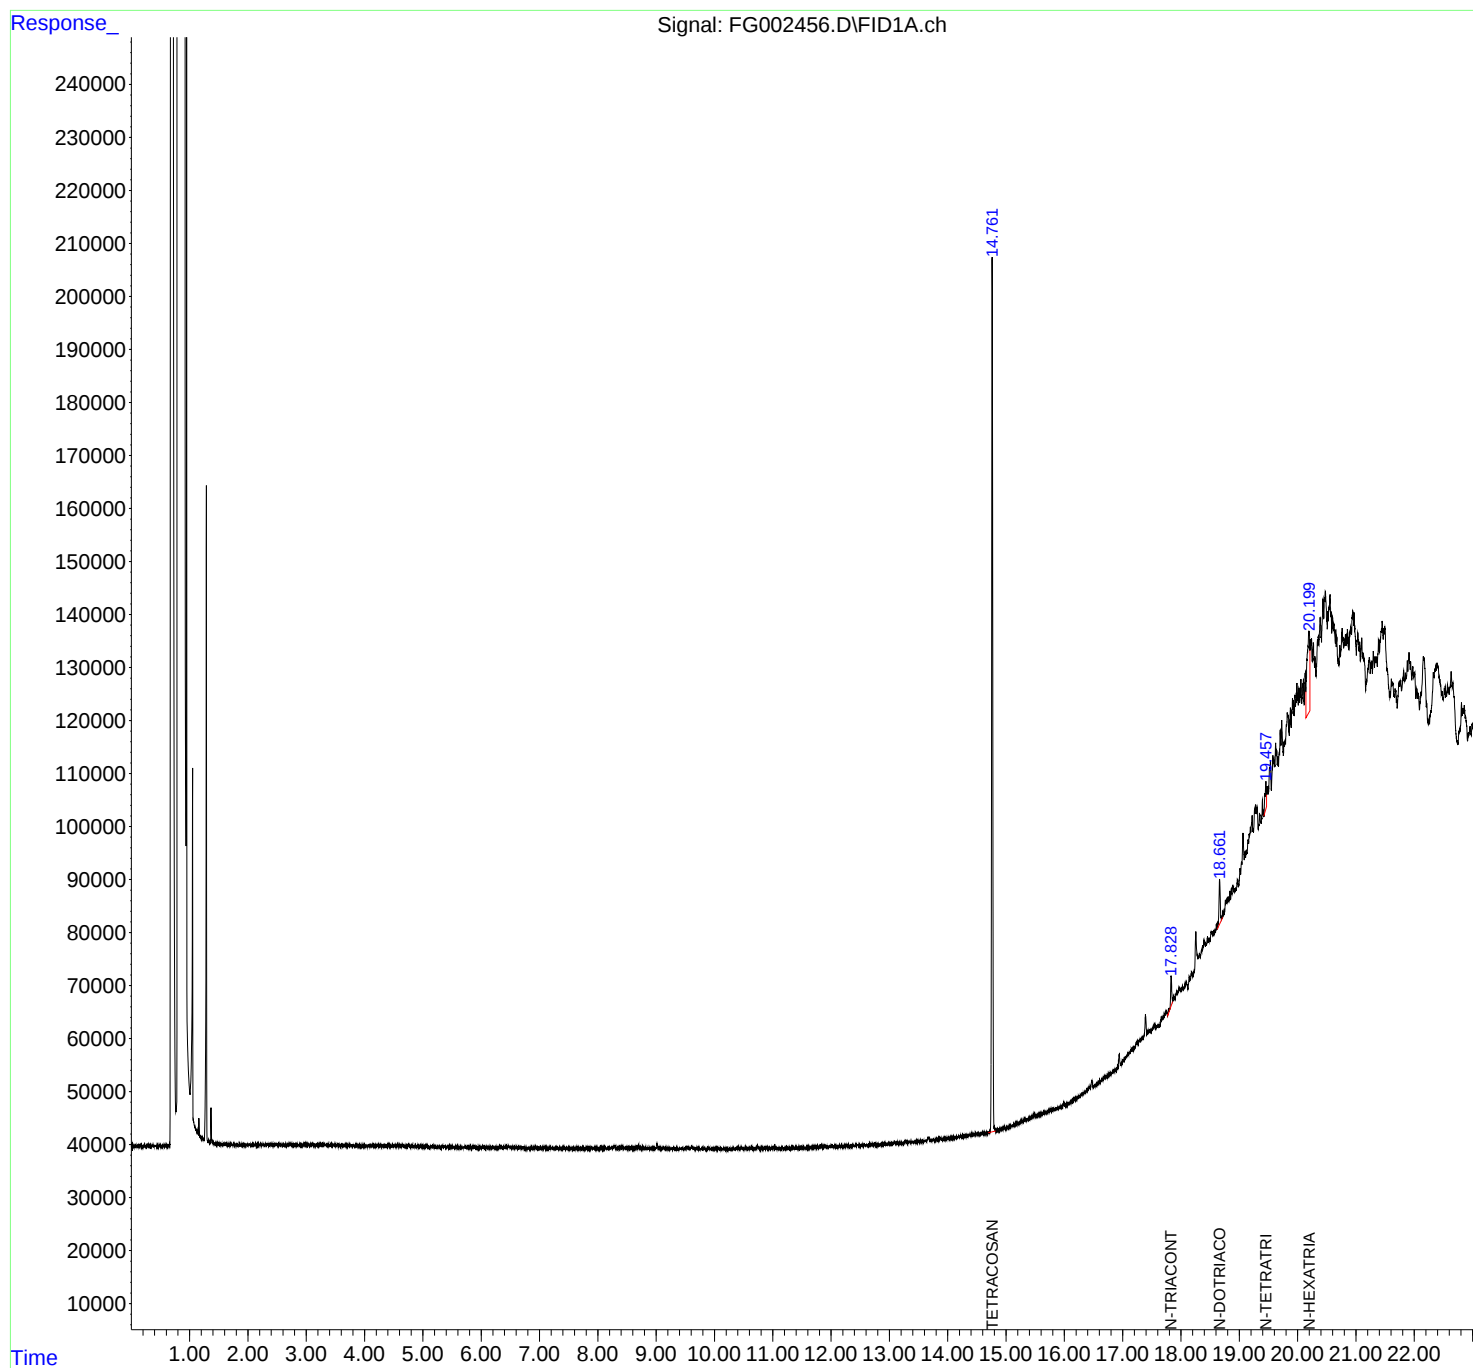

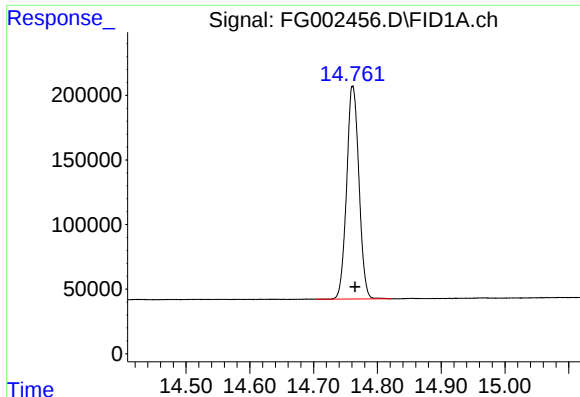


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.761 min
Delta R.T.: -0.004 min
Response: 2209377
Conc: 19.25 ug/ml

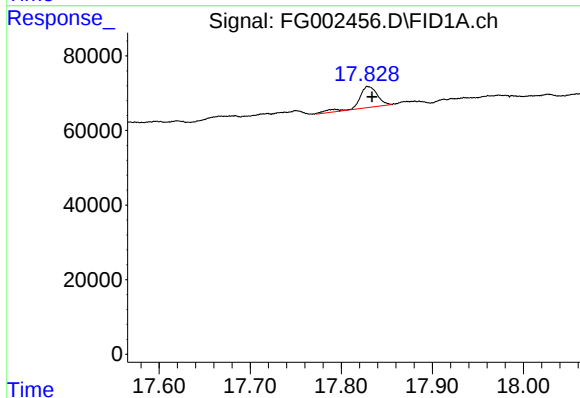


#13 N-TRIACONTANE

R.T.: 17.830 min
Delta R.T.: -0.004 min
Response: 79690
Conc: 0.63 ug/ml

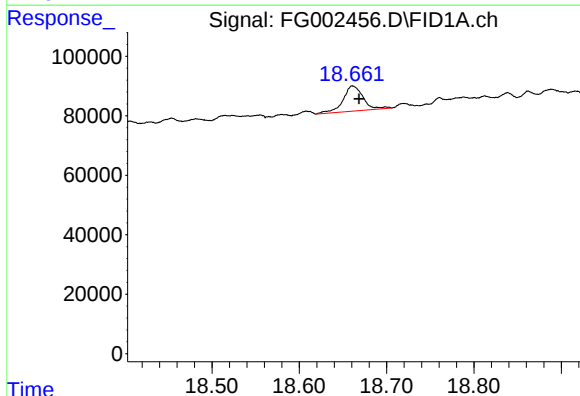


#14 N-DOTRIACONTANE

R.T.: 18.661 min
Delta R.T.: -0.007 min
Response: 134166
Conc: 1.09 ug/ml

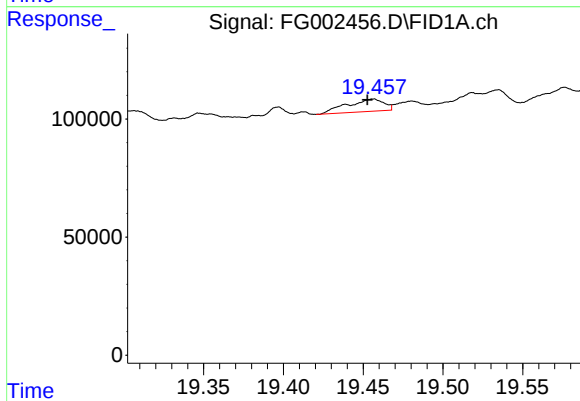

#15 N-TETRATRIACONTANE

R.T.: 19.456 min
Delta R.T.: 0.004 min
Response: 83618
Conc: 0.70 ug/ml

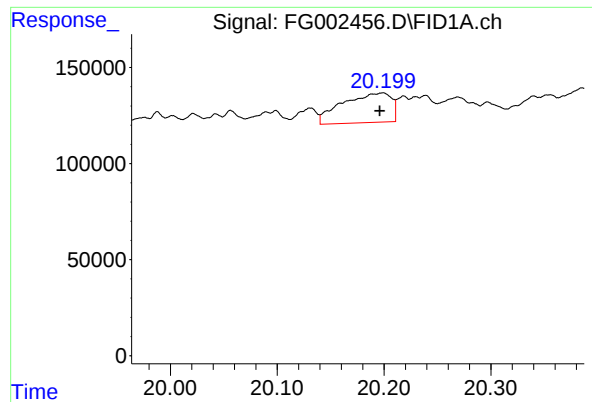

#16 N-HEXATRIACONTANE

R.T.: 20.199 min
Delta R.T.: 0.003 min
Response: 492083
Conc: 4.44 ug/ml