

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG100224\
Data File : FG014364.D
Signal(s) : FID1A.ch
Acq On : 02 Oct 2024 15:34
Operator : YP\AJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Oct 03 04:45:55 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG100224.M
Quant Title :
QLast Update : Thu Oct 03 04:45:13 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
13) N-TRIACONTANE	18.009	27865	0.201 ug/ml
14) N-DOTRIACONTANE	18.846	62799	0.461 ug/ml
15) N-TETRATRIACONTANE	19.628	54716	0.416 ug/ml
16) N-HEXATRIACONTANE	20.402f	71765	0.561 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG100224\
Data File : FG014364.D
Signal(s) : FID1A.ch
Acq On : 02 Oct 2024 15:34
Operator : YP\AJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Oct 03 04:45:55 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG100224.M
Quant Title :
QLast Update : Thu Oct 03 04:45:13 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

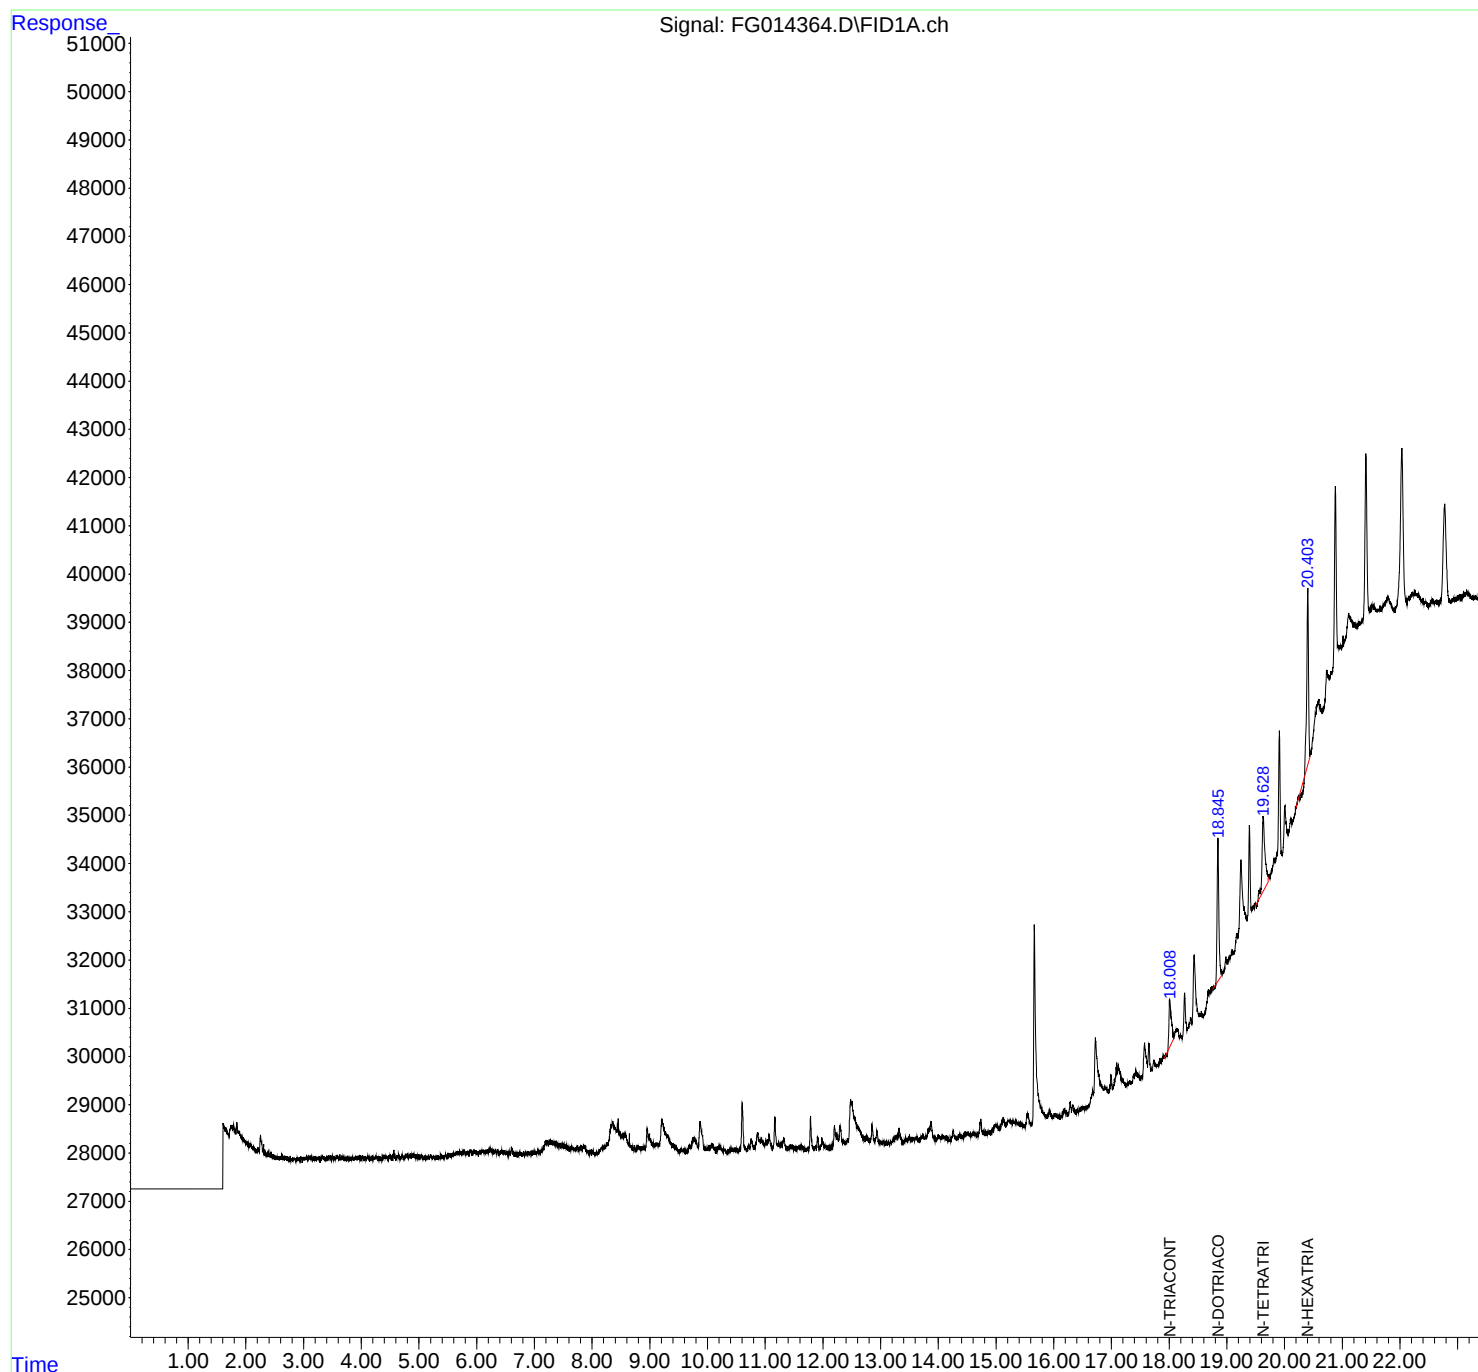


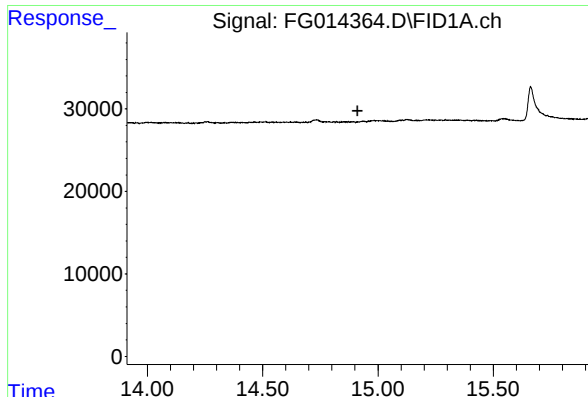

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 0.000 min
Exp R.T.: 14.911 min
Response: 0
Conc: N.D.

Instrument :
FID_G
ClientSampleId :

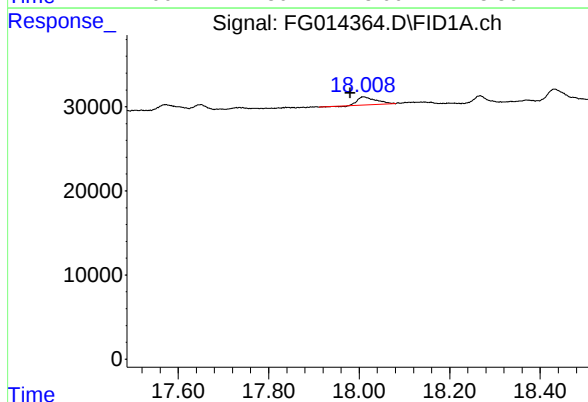


#13 N-TRIACONTANE

R.T.: 18.009 min
Delta R.T.: 0.028 min
Response: 27865
Conc: 0.20 ug/ml

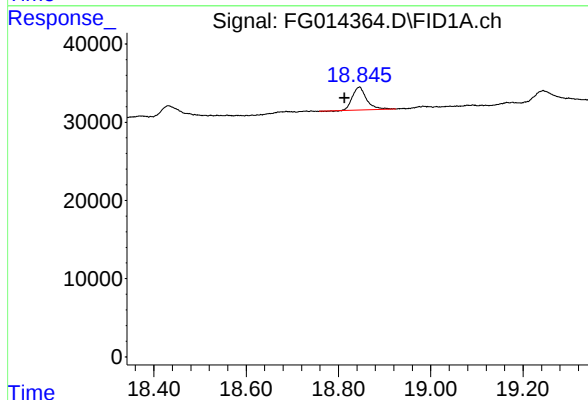


#14 N-DOTRIACONTANE

R.T.: 18.846 min
Delta R.T.: 0.032 min
Response: 62799
Conc: 0.46 ug/ml

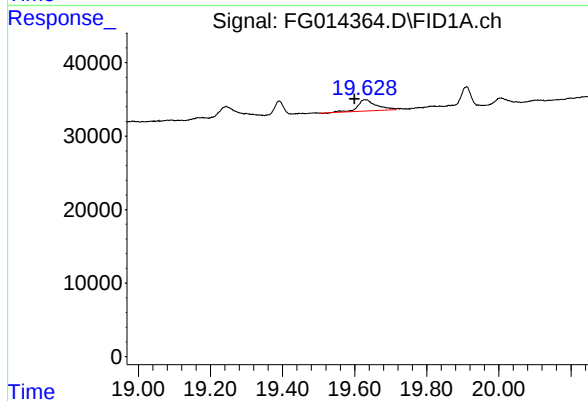

#15 N-TETRATRIACONTANE

R.T.: 19.628 min
Delta R.T.: 0.028 min
Response: 54716
Conc: 0.42 ug/ml

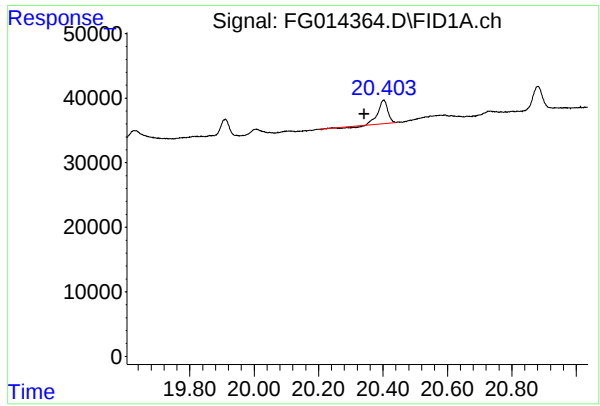

#16 N-HEXATRIACONTANE

R.T.: 20.402 min
Delta R.T.: 0.060 min
Response: 71765
Conc: 0.56 ug/ml

Instrument :

FID_G

ClientSampleId :