

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG100318\
 Data File : FG002494.D
 Signal(s) : FID1A.ch
 Acq On : 03 Oct 2018 19:09
 Operator : AJ\SJ
 Sample : PB113469BS
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Oct 04 05:32:01 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG100118.M
 Quant Title :
 QLast Update : Mon Oct 01 12:36:17 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.758	1838501	16.017 ug/ml
Target Compounds			
2) N-DECANE	4.462	2290960	17.583 ug/ml
3) N-DODECANE	6.491	2357551	17.864 ug/ml
4) N-TETRADECANE	8.291	2357104	17.678 ug/ml
5) N-HEXADECANE	9.897	2353624	17.545 ug/ml
6) N-OCTADECANE	11.342	2357954	17.509 ug/ml
7) N-EICOSANE	12.655	2332021	17.483 ug/ml
8) N-DOCOSANE	13.857	2307153	17.485 ug/ml
10) N-TETRACOSANE	14.962	2268641	17.451 ug/ml
11) N-HEXACOSANE	15.986	2217772	17.265 ug/ml
12) N-OCTACOSANE	16.937	2175870	17.162 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG100318\
Data File : FG002494.D
Signal(s) : FID1A.ch
Acq On : 03 Oct 2018 19:09
Operator : AJ\SJ
Sample : PB113469BS
Misc :
ALS Vial : 13 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Oct 04 05:32:01 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG100118.M
Quant Title :
QLast Update : Mon Oct 01 12:36:17 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

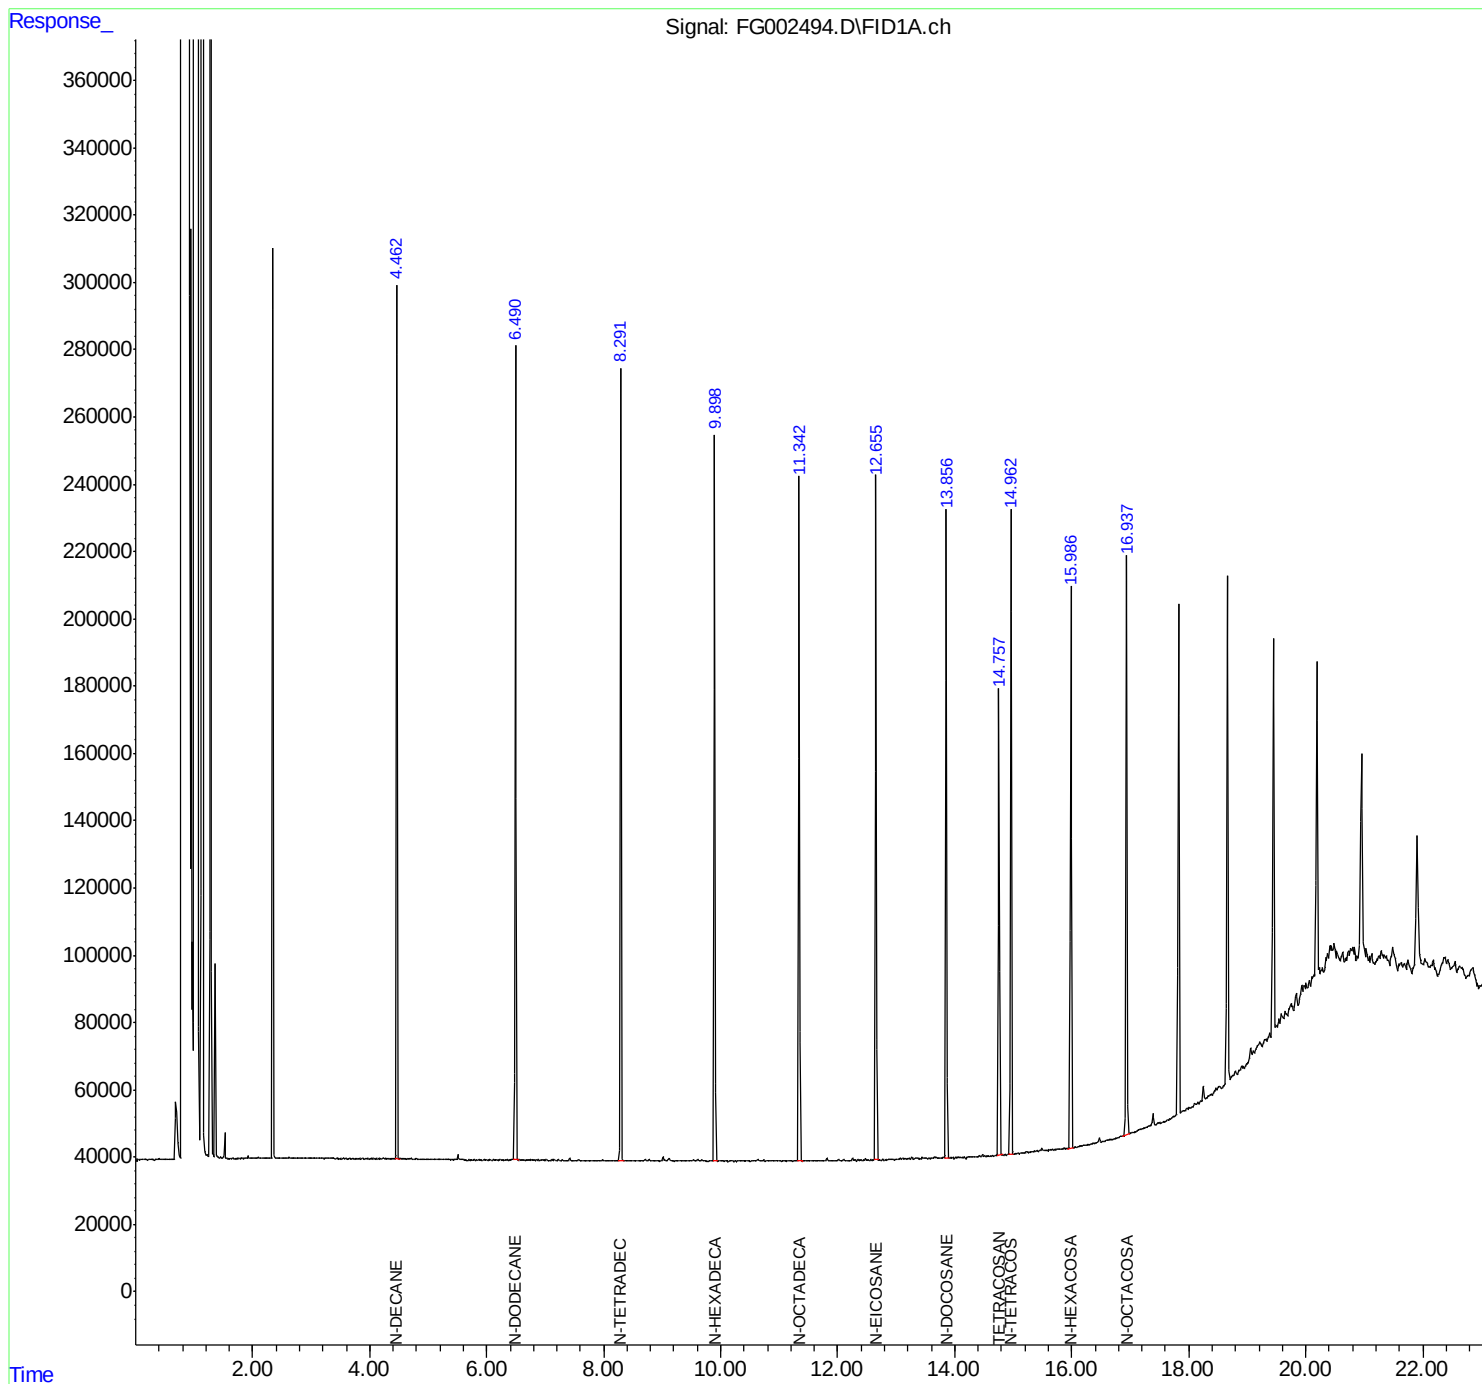

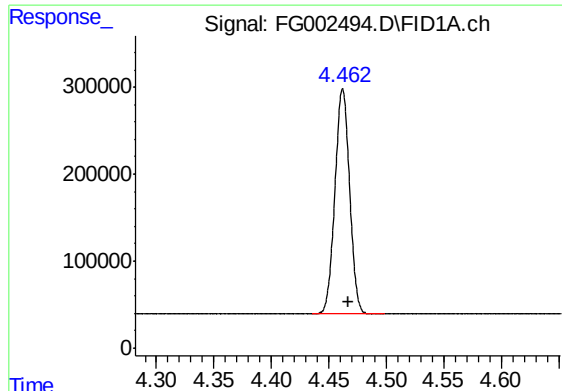


#2 N-DECANE

R.T.: 4.462 min
Delta R.T.: -0.005 min
Response: 2290960
Conc: 17.58 ug/ml

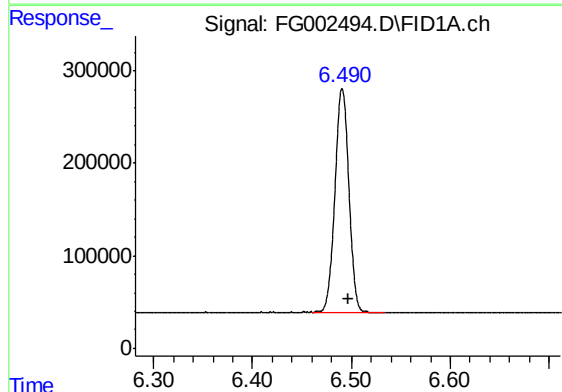


#3 N-DODECANE

R.T.: 6.491 min
Delta R.T.: -0.007 min
Response: 2357551
Conc: 17.86 ug/ml

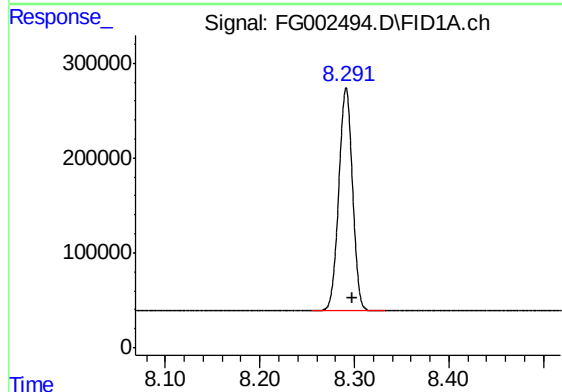


#4 N-TETRADECANE

R.T.: 8.291 min
Delta R.T.: -0.006 min
Response: 2357104
Conc: 17.68 ug/ml

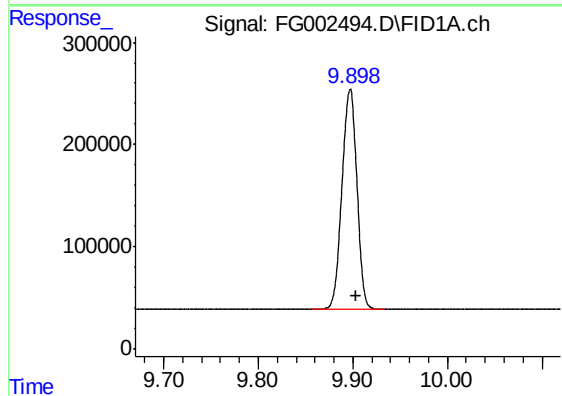


#5 N-HEXADECANE

R.T.: 9.897 min
Delta R.T.: -0.006 min
Response: 2353624
Conc: 17.55 ug/ml

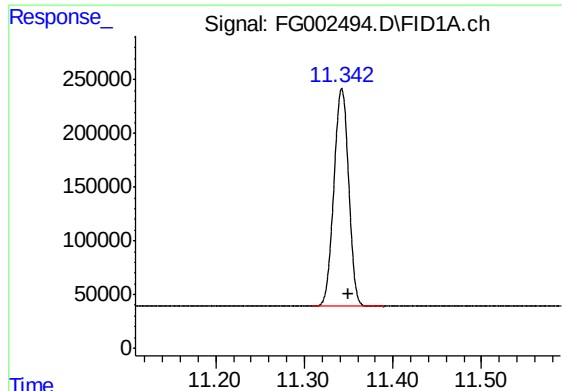


#6 N-OCTADECANE

R.T.: 11.342 min
Delta R.T.: -0.007 min
Response: 2357954
Conc: 17.51 ug/ml

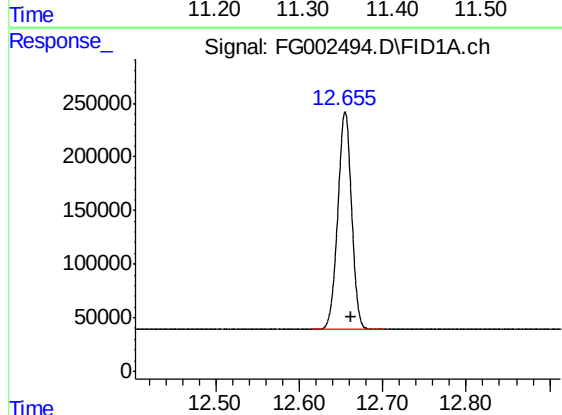


#7 N-EICOSANE

R.T.: 12.655 min
Delta R.T.: -0.008 min
Response: 2332021
Conc: 17.48 ug/ml

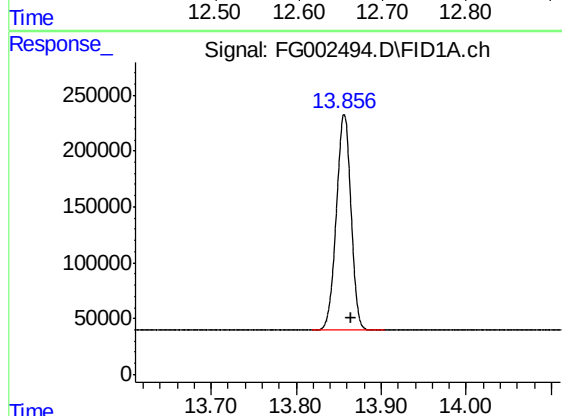


#8 N-DOCOSANE

R.T.: 13.857 min
Delta R.T.: -0.008 min
Response: 2307153
Conc: 17.48 ug/ml

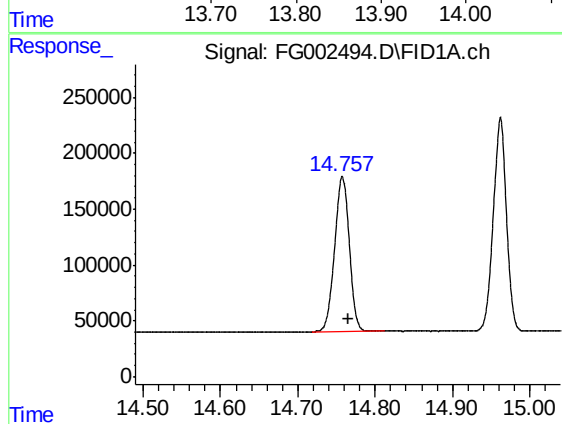


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.758 min
Delta R.T.: -0.008 min
Response: 1838501
Conc: 16.02 ug/ml

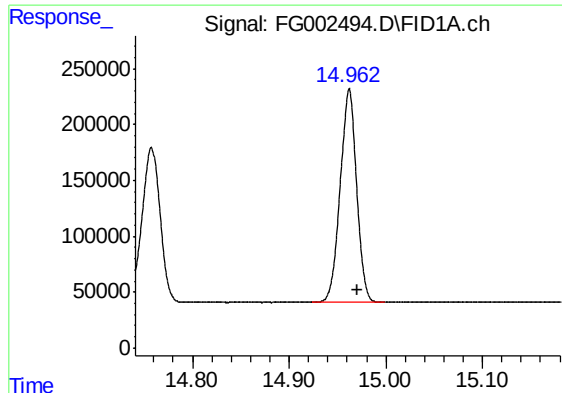


#10 N-TETRACOSANE

R.T.: 14.962 min
Delta R.T.: -0.008 min
Response: 2268641
Conc: 17.45 ug/ml

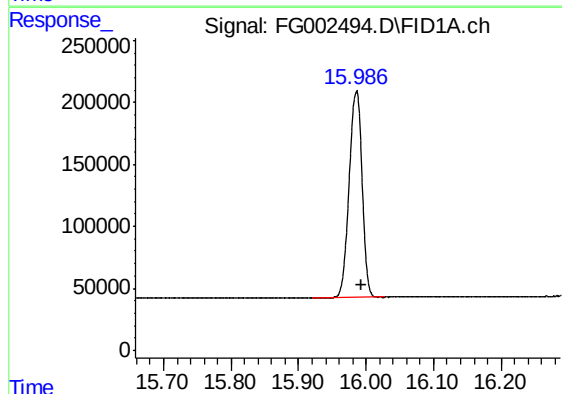

#11 N-HEXACOSANE

R.T.: 15.986 min
Delta R.T.: -0.008 min
Response: 2217772
Conc: 17.26 ug/ml

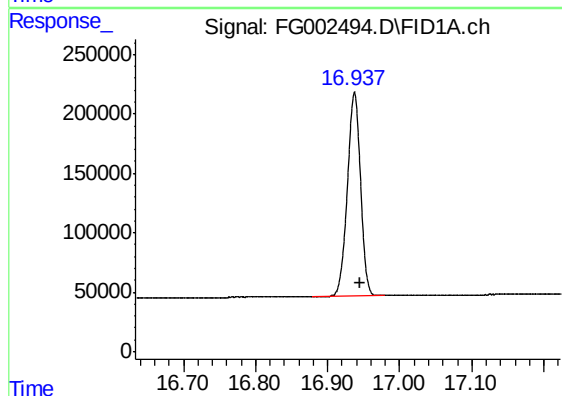

#12 N-OCTACOSANE

R.T.: 16.937 min
Delta R.T.: -0.008 min
Response: 2175870
Conc: 17.16 ug/ml