

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG100318\
 Data File : FG002495.D
 Signal(s) : FID1A.ch
 Acq On : 03 Oct 2018 19:39
 Operator : AJ\SJ
 Sample : PB113469BSD
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Oct 04 05:32:16 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG100118.M
 Quant Title :
 QLast Update : Mon Oct 01 12:36:17 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.757	2296763	20.010 ug/ml
Target Compounds			
2) N-DECANE	4.462	2520066	19.342 ug/ml
3) N-DODECANE	6.491	2600370	19.704 ug/ml
4) N-TETRADECANE	8.291	2619780	19.648 ug/ml
5) N-HEXADECANE	9.897	2632500	19.624 ug/ml
6) N-OCTADECANE	11.343	2641612	19.615 ug/ml
7) N-EICOSANE	12.656	2624907	19.679 ug/ml
8) N-DOCOSANE	13.856	2600518	19.708 ug/ml
10) N-TETRACOSANE	14.962	2563315	19.718 ug/ml
11) N-HEXACOSANE	15.985	2513814	19.569 ug/ml
12) N-OCTACOSANE	16.936	2465879	19.449 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG100318\
Data File : FG002495.D
Signal(s) : FID1A.ch
Acq On : 03 Oct 2018 19:39
Operator : AJ\SJ
Sample : PB113469BSD
Misc :
ALS Vial : 14 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Oct 04 05:32:16 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG100118.M
Quant Title :
QLast Update : Mon Oct 01 12:36:17 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

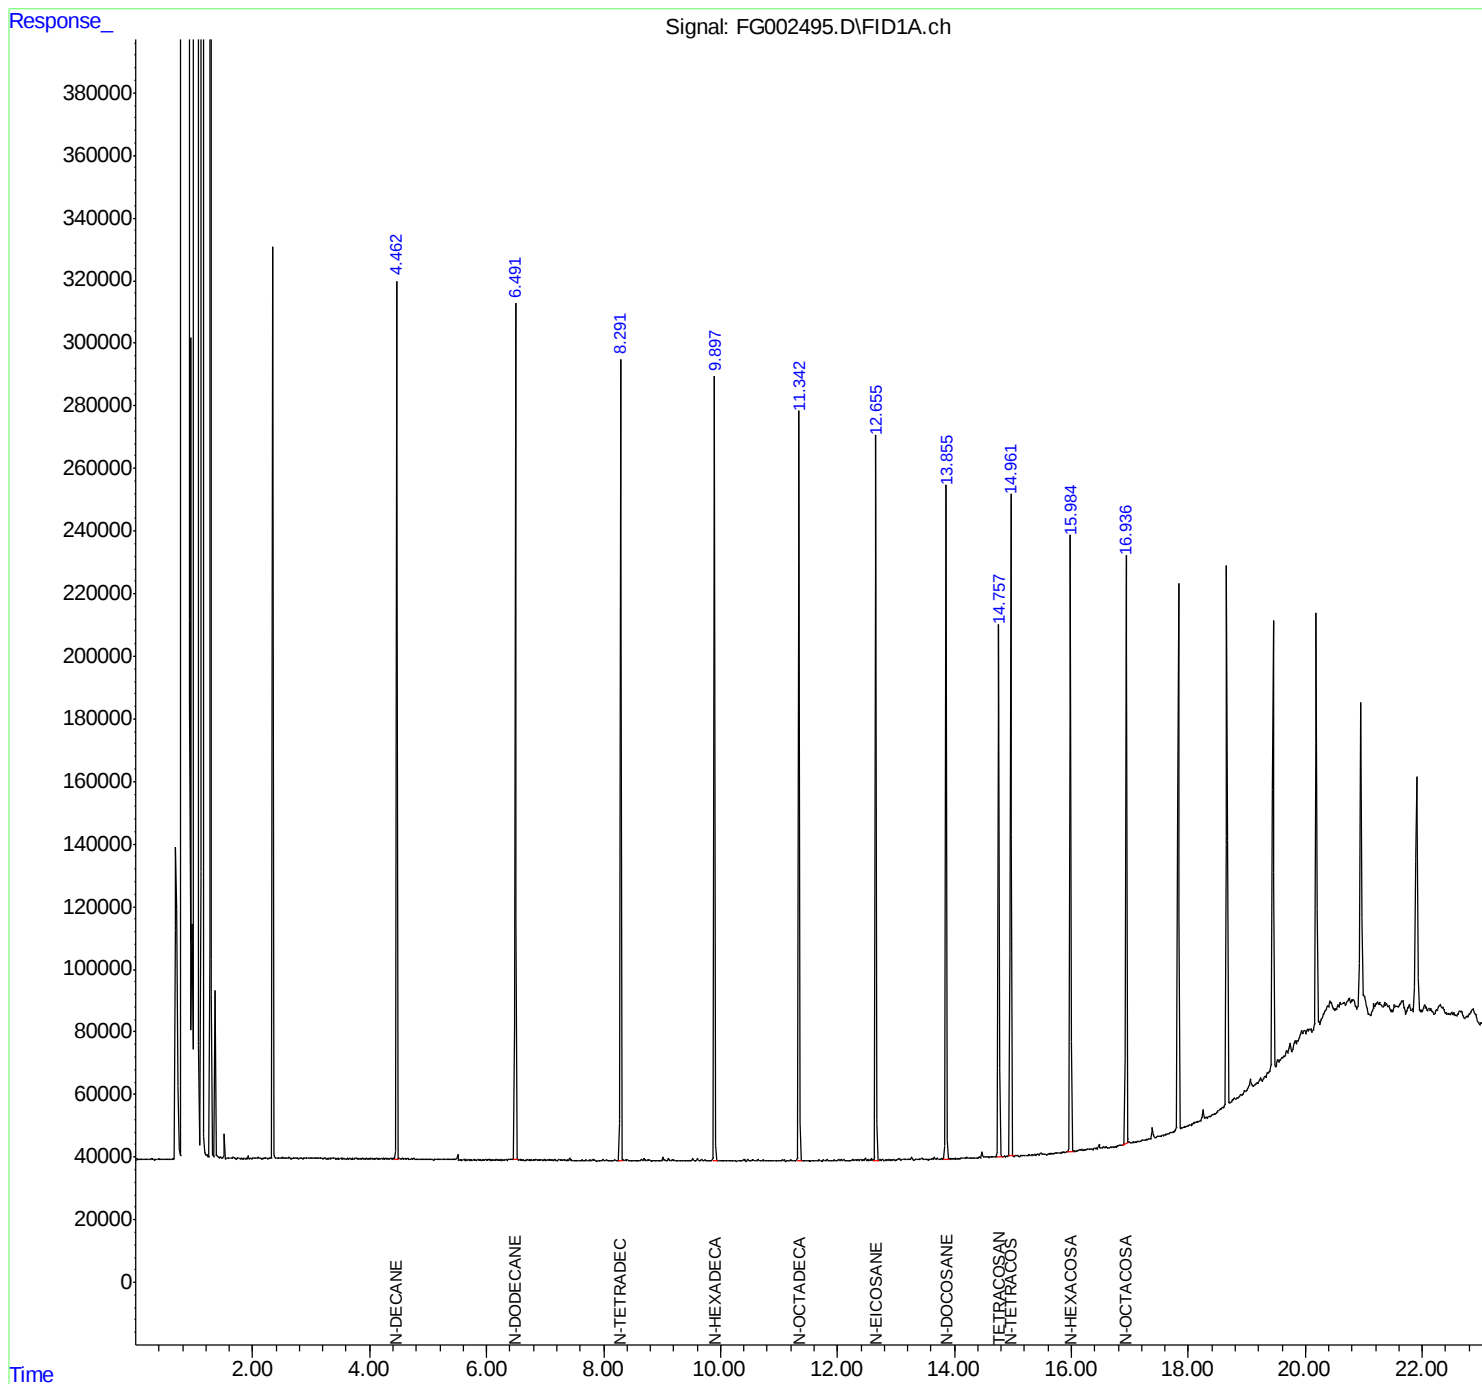

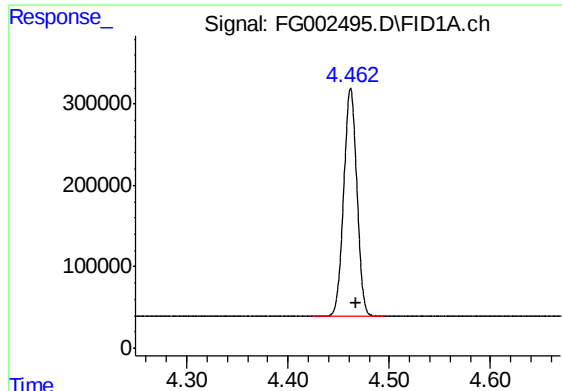


#2 N-DECANE

R.T.: 4.462 min
Delta R.T.: -0.005 min
Response: 2520066
Conc: 19.34 ug/ml

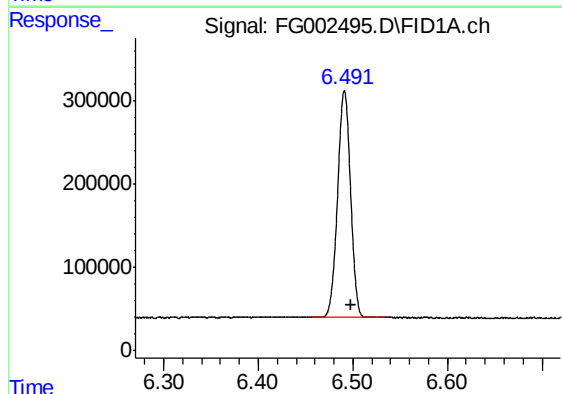


#3 N-DODECANE

R.T.: 6.491 min
Delta R.T.: -0.006 min
Response: 2600370
Conc: 19.70 ug/ml

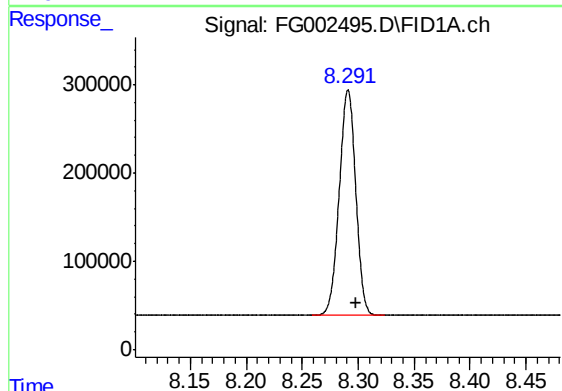


#4 N-TETRADECANE

R.T.: 8.291 min
Delta R.T.: -0.007 min
Response: 2619780
Conc: 19.65 ug/ml

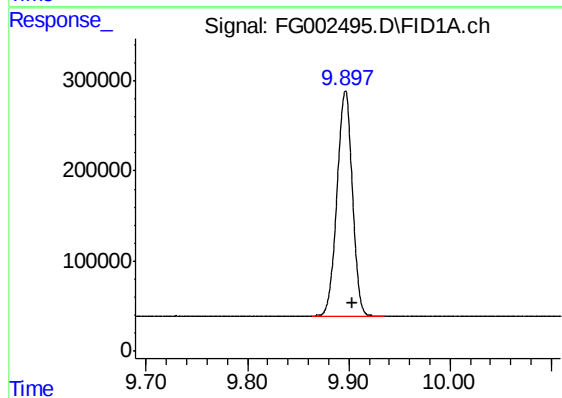


#5 N-HEXADECANE

R.T.: 9.897 min
Delta R.T.: -0.007 min
Response: 2632500
Conc: 19.62 ug/ml

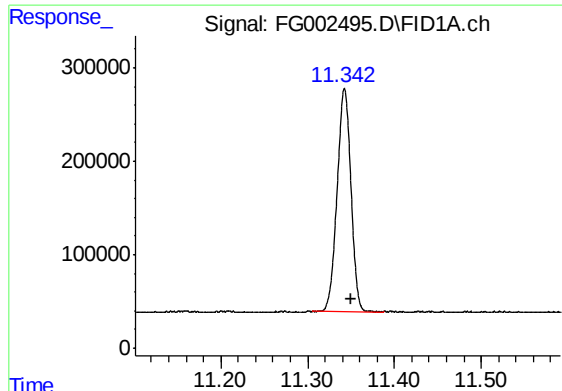


#6 N-OCTADECANE

R.T.: 11.343 min
Delta R.T.: -0.007 min
Response: 2641612
Conc: 19.61 ug/ml

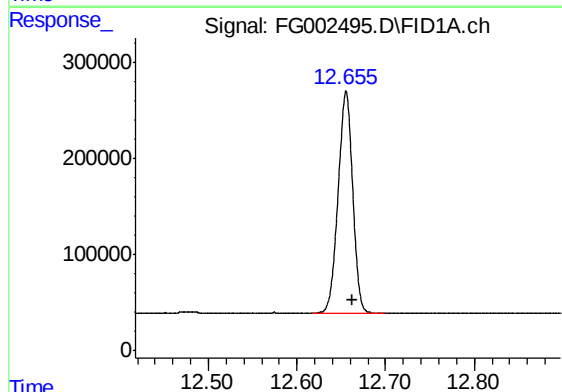


#7 N-EICOSANE

R.T.: 12.656 min
Delta R.T.: -0.007 min
Response: 2624907
Conc: 19.68 ug/ml

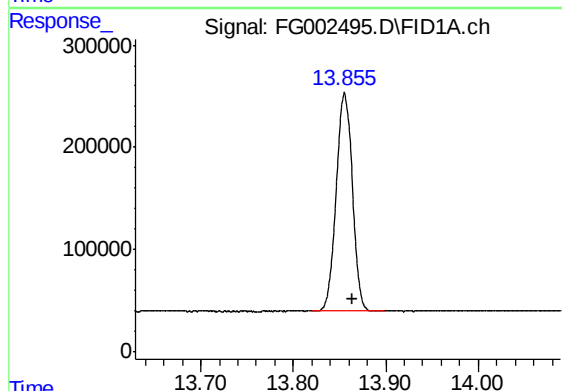


#8 N-DOCOSANE

R.T.: 13.856 min
Delta R.T.: -0.009 min
Response: 2600518
Conc: 19.71 ug/ml

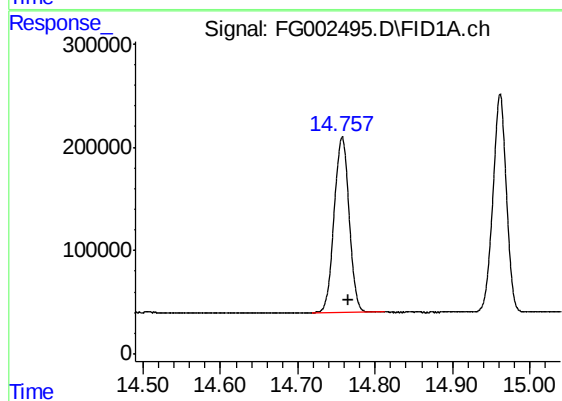


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.757 min
Delta R.T.: -0.008 min
Response: 2296763
Conc: 20.01 ug/ml

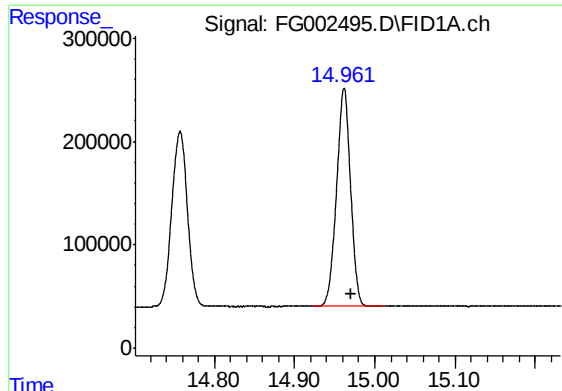


#10 N-TETRACOSANE

R.T.: 14.962 min
Delta R.T.: -0.009 min
Response: 2563315
Conc: 19.72 ug/ml

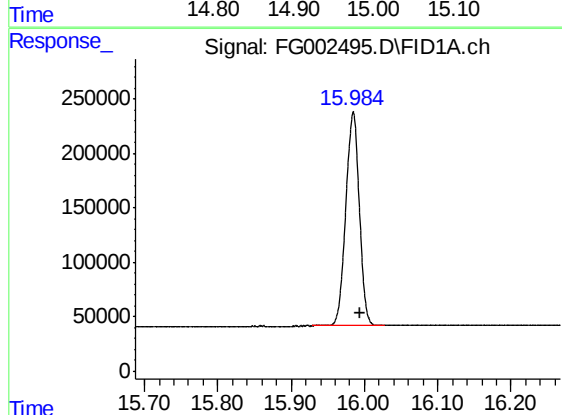

#11 N-HEXACOSANE

R.T.: 15.985 min
Delta R.T.: -0.009 min
Response: 2513814
Conc: 19.57 ug/ml

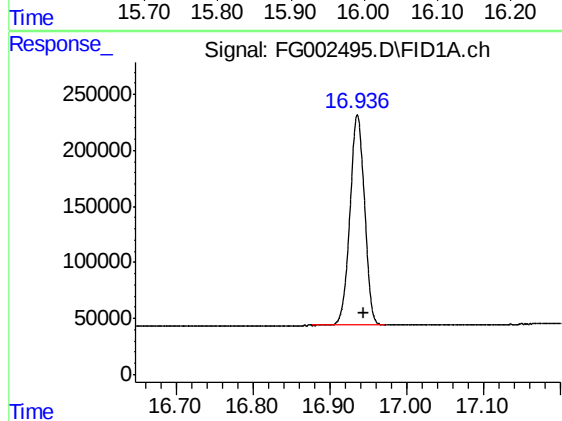

#12 N-OCTACOSANE

R.T.: 16.936 min
Delta R.T.: -0.009 min
Response: 2465879
Conc: 19.45 ug/ml