

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG100324\
 Data File : FG014380.D
 Signal(s) : FID1A.ch
 Acq On : 03 Oct 2024 14:04
 Operator : YP\AJ
 Sample : P4277-01
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Oct 04 01:53:27 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG100224.M
 Quant Title :
 QLast Update : Thu Oct 03 05:57:06 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.911	1102889	8.907 ug/ml
Target Compounds			
5) N-HEXADECANE	10.051	7229	0.057 ug/ml
7) N-EICOSANE	12.807	27309	0.196 ug/ml
8) N-DOCOSANE	14.019	69157	0.504 ug/ml
10) N-TETRACOSANE	15.083	177163	1.285 ug/ml
11) N-HEXACOSANE	16.142	25773	0.186 ug/ml
12) N-OCTACOSANE	17.096	71319	0.520 ug/ml
13) N-TRIACONTANE	17.976	104197	0.751 ug/ml
14) N-DOTRIACONTANE	18.811	127586	0.936 ug/ml
15) N-TETRATRIACONTANE	19.604	88681	0.674 ug/ml
16) N-HEXATRIACONTANE	20.343	111678	0.873 ug/ml
17) N-OCTATRIACONTANE	21.077	12763	0.112 ug/ml
18) N-TETRACONTANE	21.959	225192	2.098 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG100324\
Data File : FG014380.D
Signal(s) : FID1A.ch
Acq On : 03 Oct 2024 14:04
Operator : YP\AJ
Sample : P4277-01
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Oct 04 01:53:27 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG100224.M
Quant Title :
QLast Update : Thu Oct 03 05:57:06 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

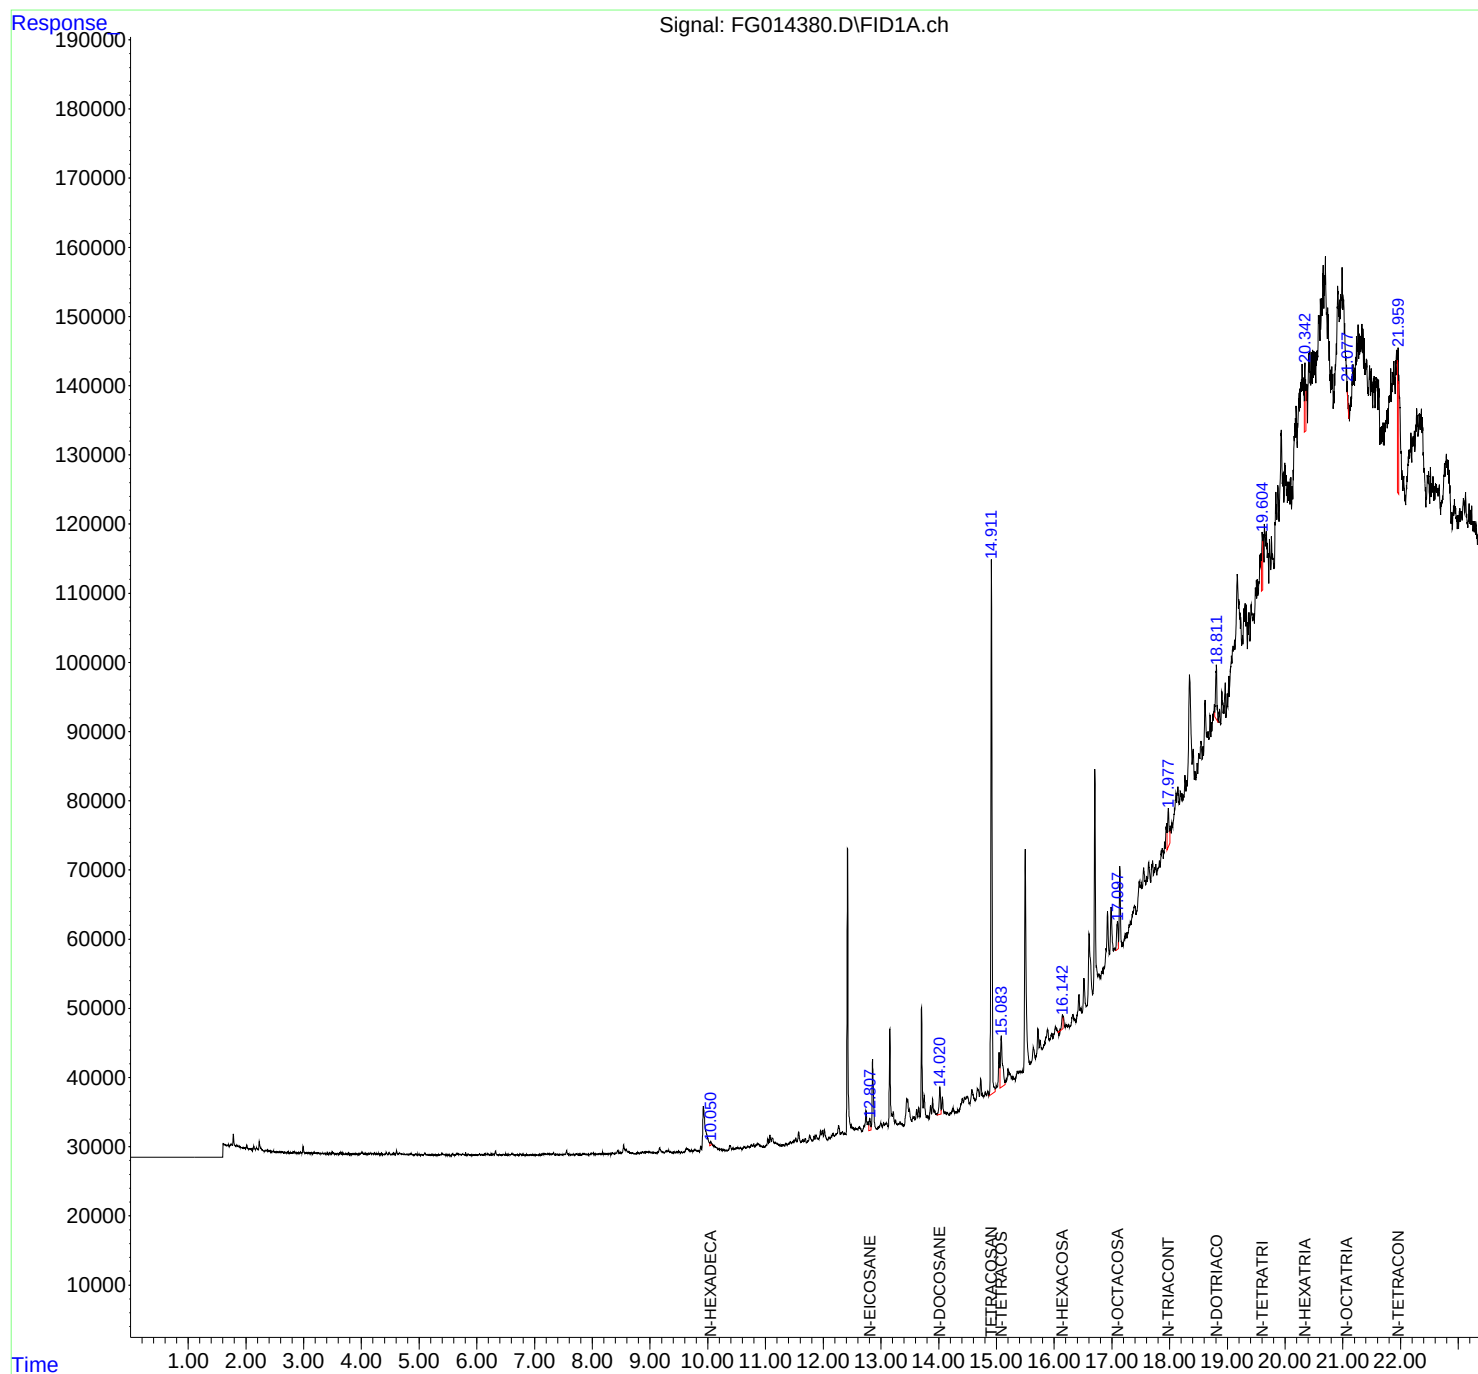


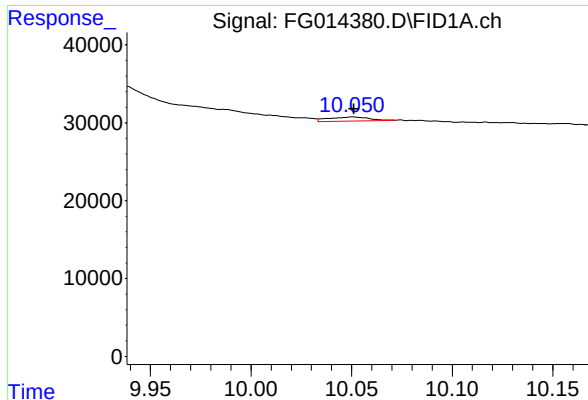

#5 N-HEXADECANE


R.T.: 10.051 min
Delta R.T.: 0.000 min
Response: 7229
Conc: 0.06 ug/ml

Instrument :
FID_G
ClientSampleId :

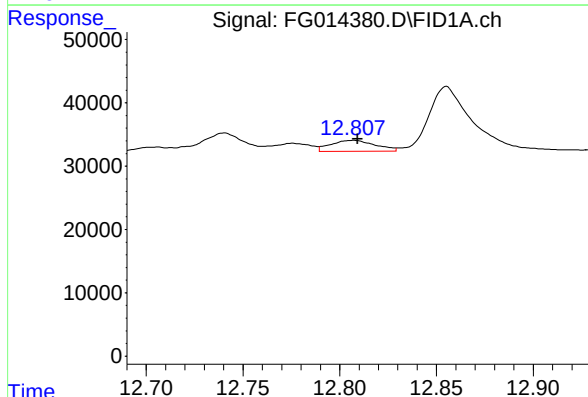


#7 N-EICOSANE

R.T.: 12.807 min
Delta R.T.: -0.002 min
Response: 27309
Conc: 0.20 ug/ml

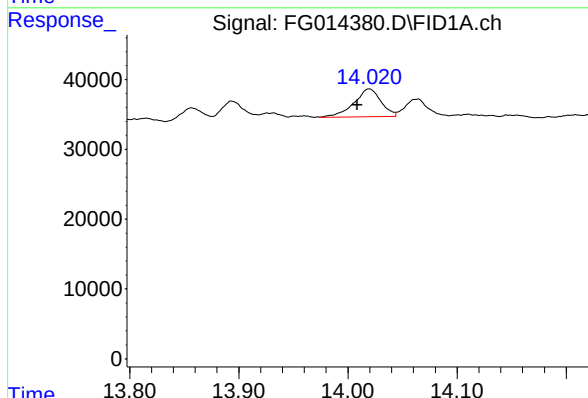


#8 N-DOCOSANE

R.T.: 14.019 min
Delta R.T.: 0.011 min
Response: 69157
Conc: 0.50 ug/ml

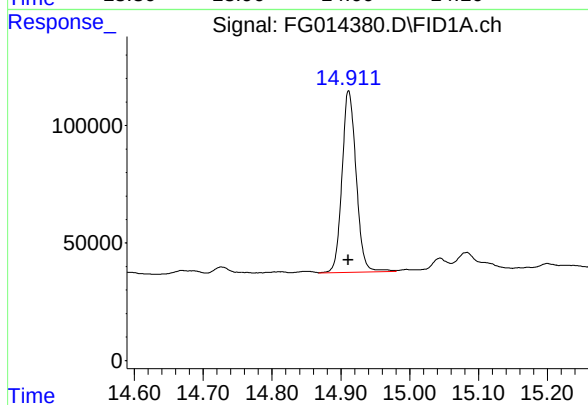

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.911 min
Delta R.T.: 0.000 min
Response: 1102889
Conc: 8.91 ug/ml

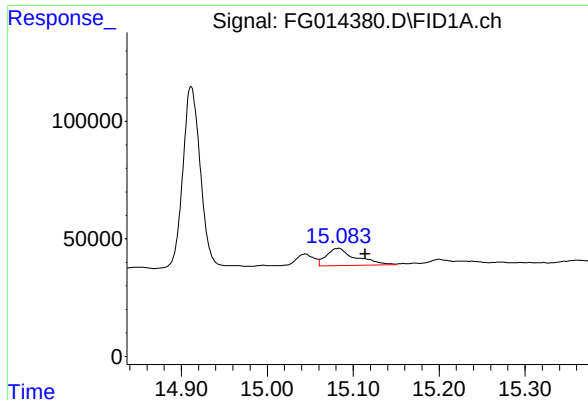


#10 N-TETRACOSANE

R.T.: 15.083 min
Delta R.T.: -0.031 min
Response: 177163
Conc: 1.29 ug/ml

Instrument :


FID_G

ClientSampleId :

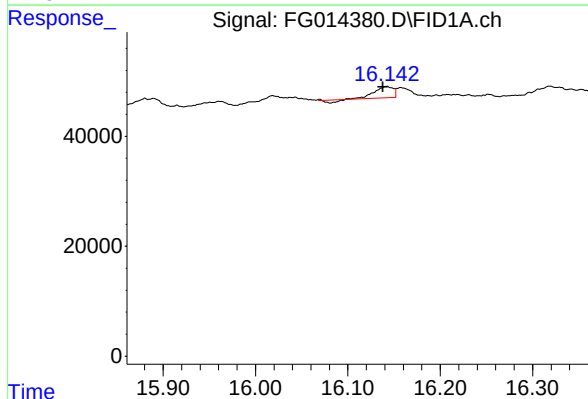


#11 N-HEXACOSANE

R.T.: 16.142 min
Delta R.T.: 0.004 min
Response: 25773
Conc: 0.19 ug/ml

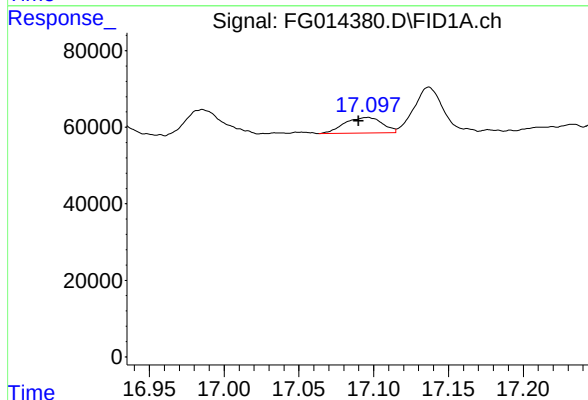


#12 N-OCTACOSANE

R.T.: 17.096 min
Delta R.T.: 0.006 min
Response: 71319
Conc: 0.52 ug/ml

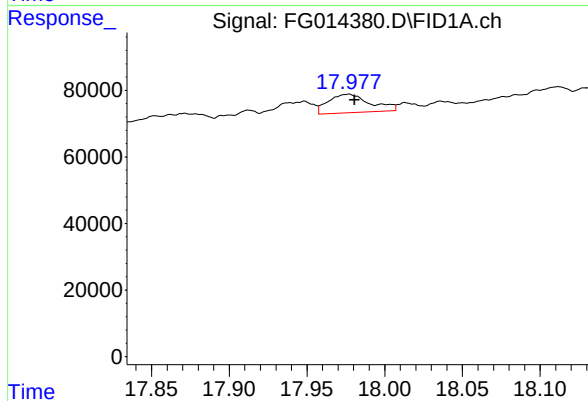

#13 N-TRIACONTANE


R.T.: 17.976 min
Delta R.T.: -0.004 min
Response: 104197
Conc: 0.75 ug/ml

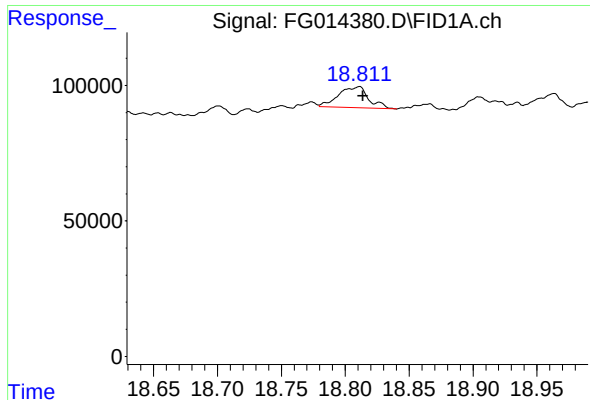

#14 N-DOTRIACONTANE


R.T.: 18.811 min
Delta R.T.: -0.003 min
Response: 127586
Conc: 0.94 ug/ml

Instrument :
FID_G
ClientSampleId :

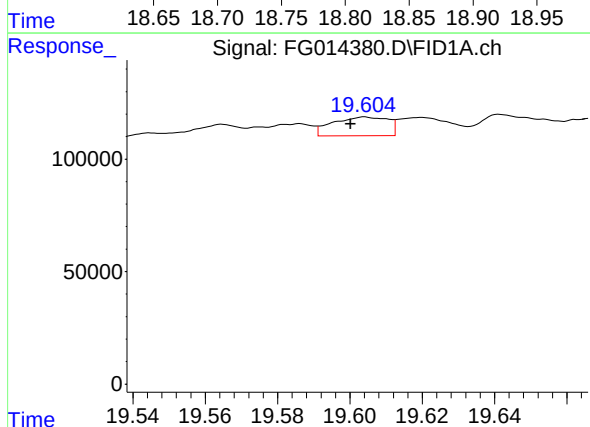


#15 N-TETRATRIACONTANE

R.T.: 19.604 min
Delta R.T.: 0.004 min
Response: 88681
Conc: 0.67 ug/ml

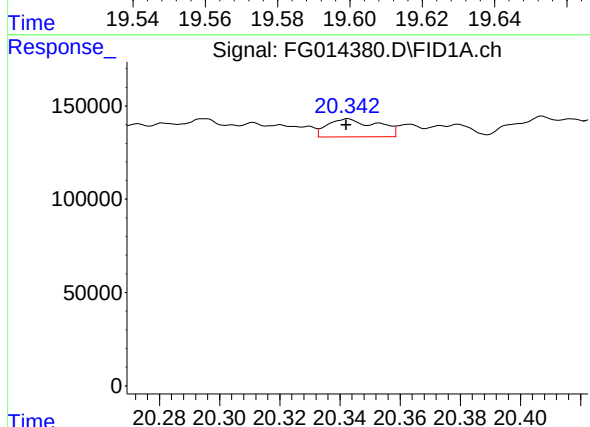


#16 N-HEXATRIACONTANE

R.T.: 20.343 min
Delta R.T.: 0.000 min
Response: 111678
Conc: 0.87 ug/ml

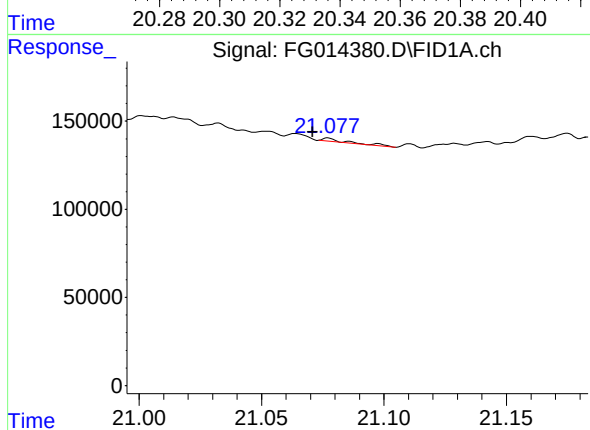

#17 N-OCTATRIACONTANE

R.T.: 21.077 min
Delta R.T.: 0.006 min
Response: 12763
Conc: 0.11 ug/ml

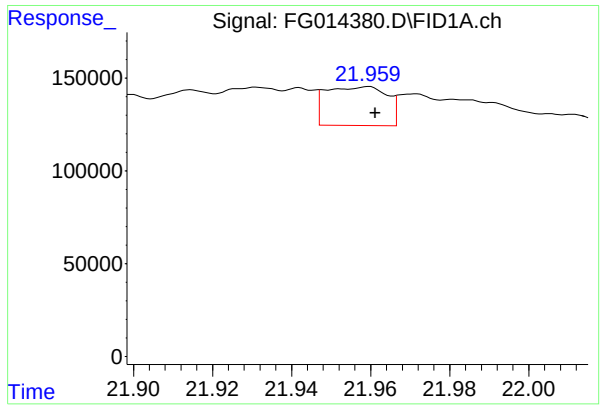

#18 N-TETRACONTANE

R.T.: 21.959 min
Delta R.T.: -0.002 min
Response: 225192
Conc: 2.10 ug/ml

Instrument :

FID_G

ClientSampleId :