

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG100324\
Data File : FG014379.D
Signal(s) : FID1A.ch
Acq On : 03 Oct 2024 13:35
Operator : YP\AJ
Sample : P4273-01
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
AU-05-100224

Integration File: autoint1.e
Quant Time: Oct 04 01:53:18 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG100224.M
Quant Title :
QLast Update : Thu Oct 03 05:57:06 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.909	1310958	10.587 ug/ml

Target Compounds

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG100324\
Data File : FG014379.D
Signal(s) : FID1A.ch
Acq On : 03 Oct 2024 13:35
Operator : YP\AJ
Sample : P4273-01
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
AU-05-100224

Integration File: autoint1.e
Quant Time: Oct 04 01:53:18 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG100224.M
Quant Title :
QLast Update : Thu Oct 03 05:57:06 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

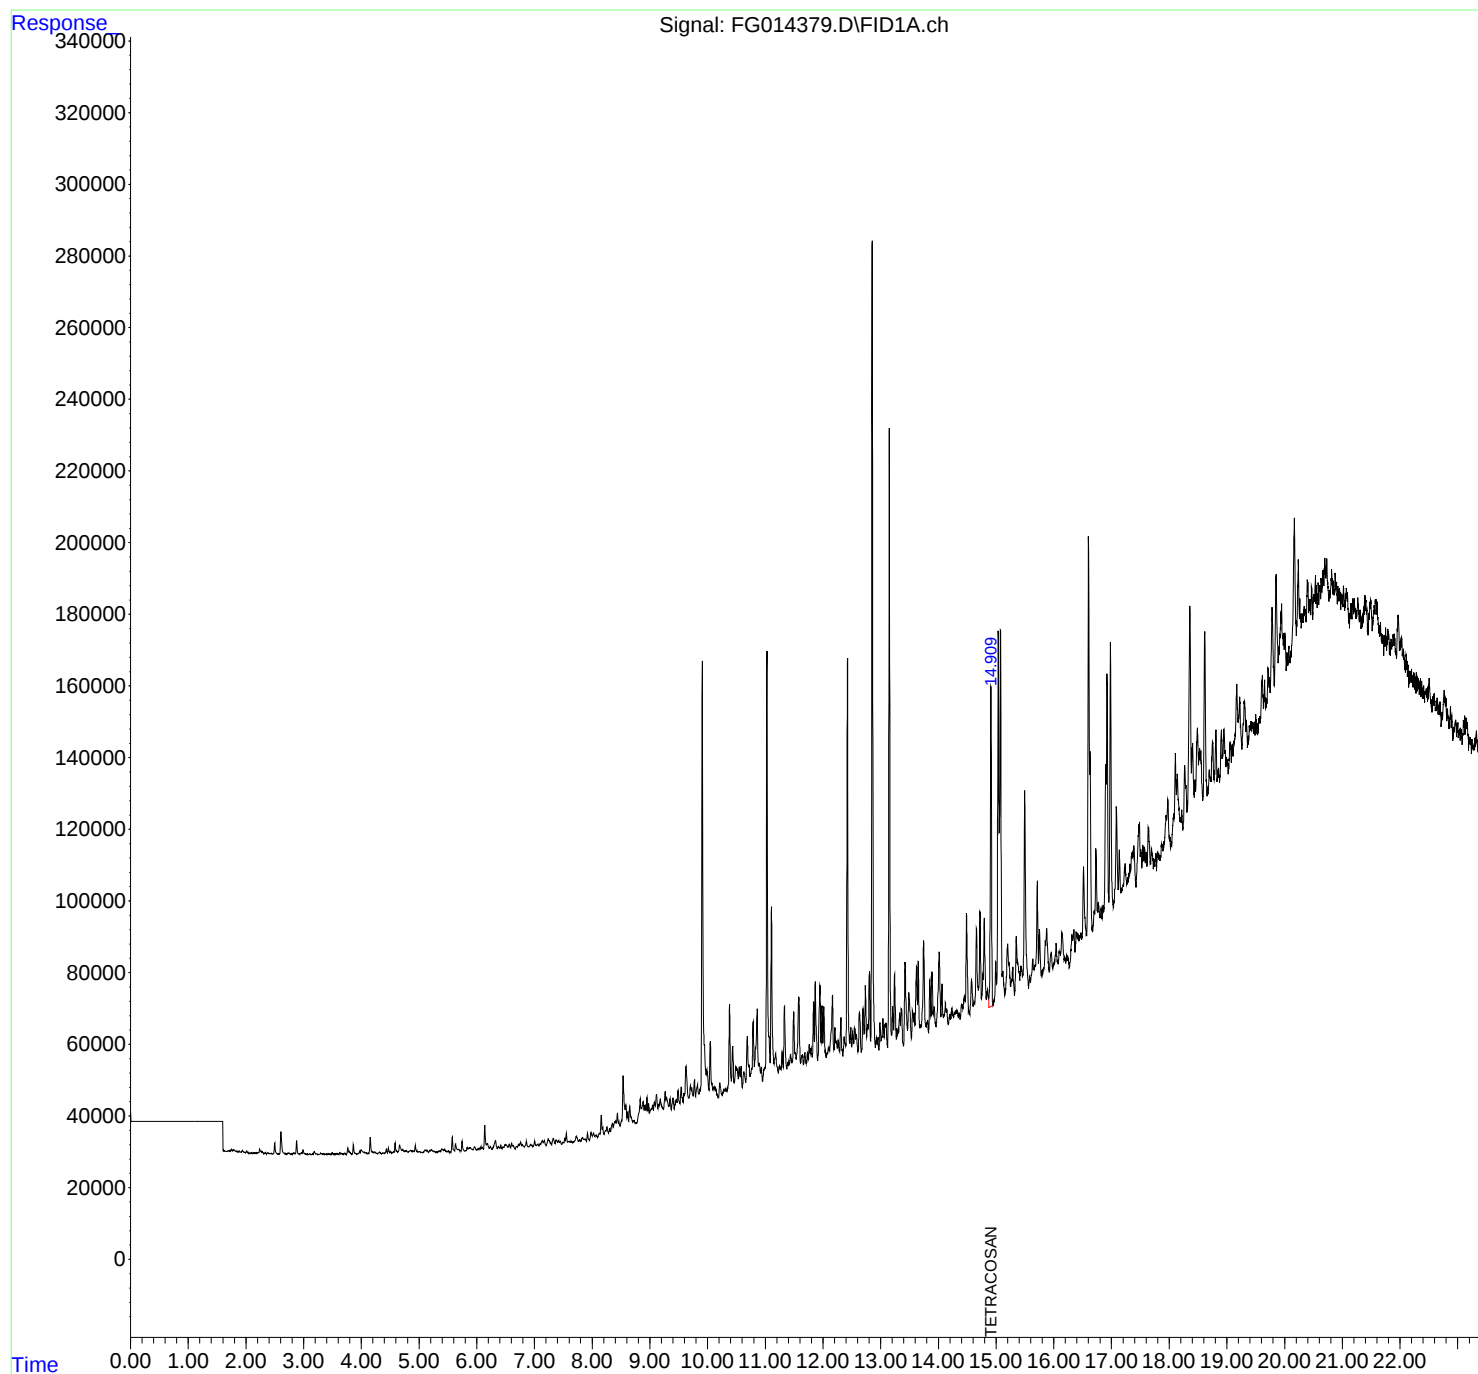

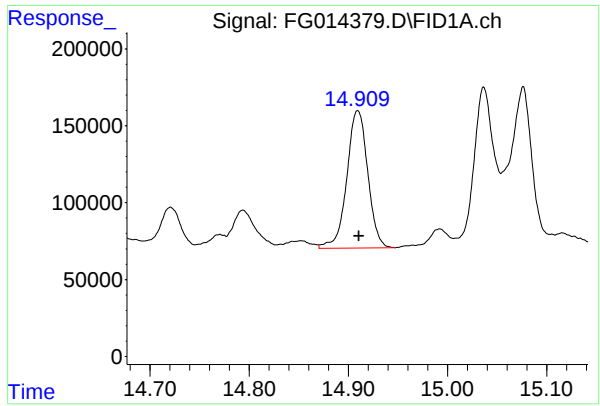

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.909 min
Delta R.T.: -0.001 min
Response: 1310958
Conc: 10.59 ug/ml

Instrument :
FID_G
ClientSampleId :
AU-05-100224