

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG100324\
Data File : FG014380.D
Signal(s) : FID1A.ch
Acq On : 03 Oct 2024 14:04
Operator : YP\AJ
Sample : P4277-01
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
BU-03-10022024

Integration File: autoint1.e
Quant Time: Oct 04 01:53:27 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG100224.M
Quant Title :
QLast Update : Thu Oct 03 05:57:06 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.911	1102889	8.907 ug/ml
Target Compounds			

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG100324\
Data File : FG014380.D
Signal(s) : FID1A.ch
Acq On : 03 Oct 2024 14:04
Operator : YP\AJ
Sample : P4277-01
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
BU-03-10022024

Integration File: autoint1.e
Quant Time: Oct 04 01:53:27 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG100224.M
Quant Title :
QLast Update : Thu Oct 03 05:57:06 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

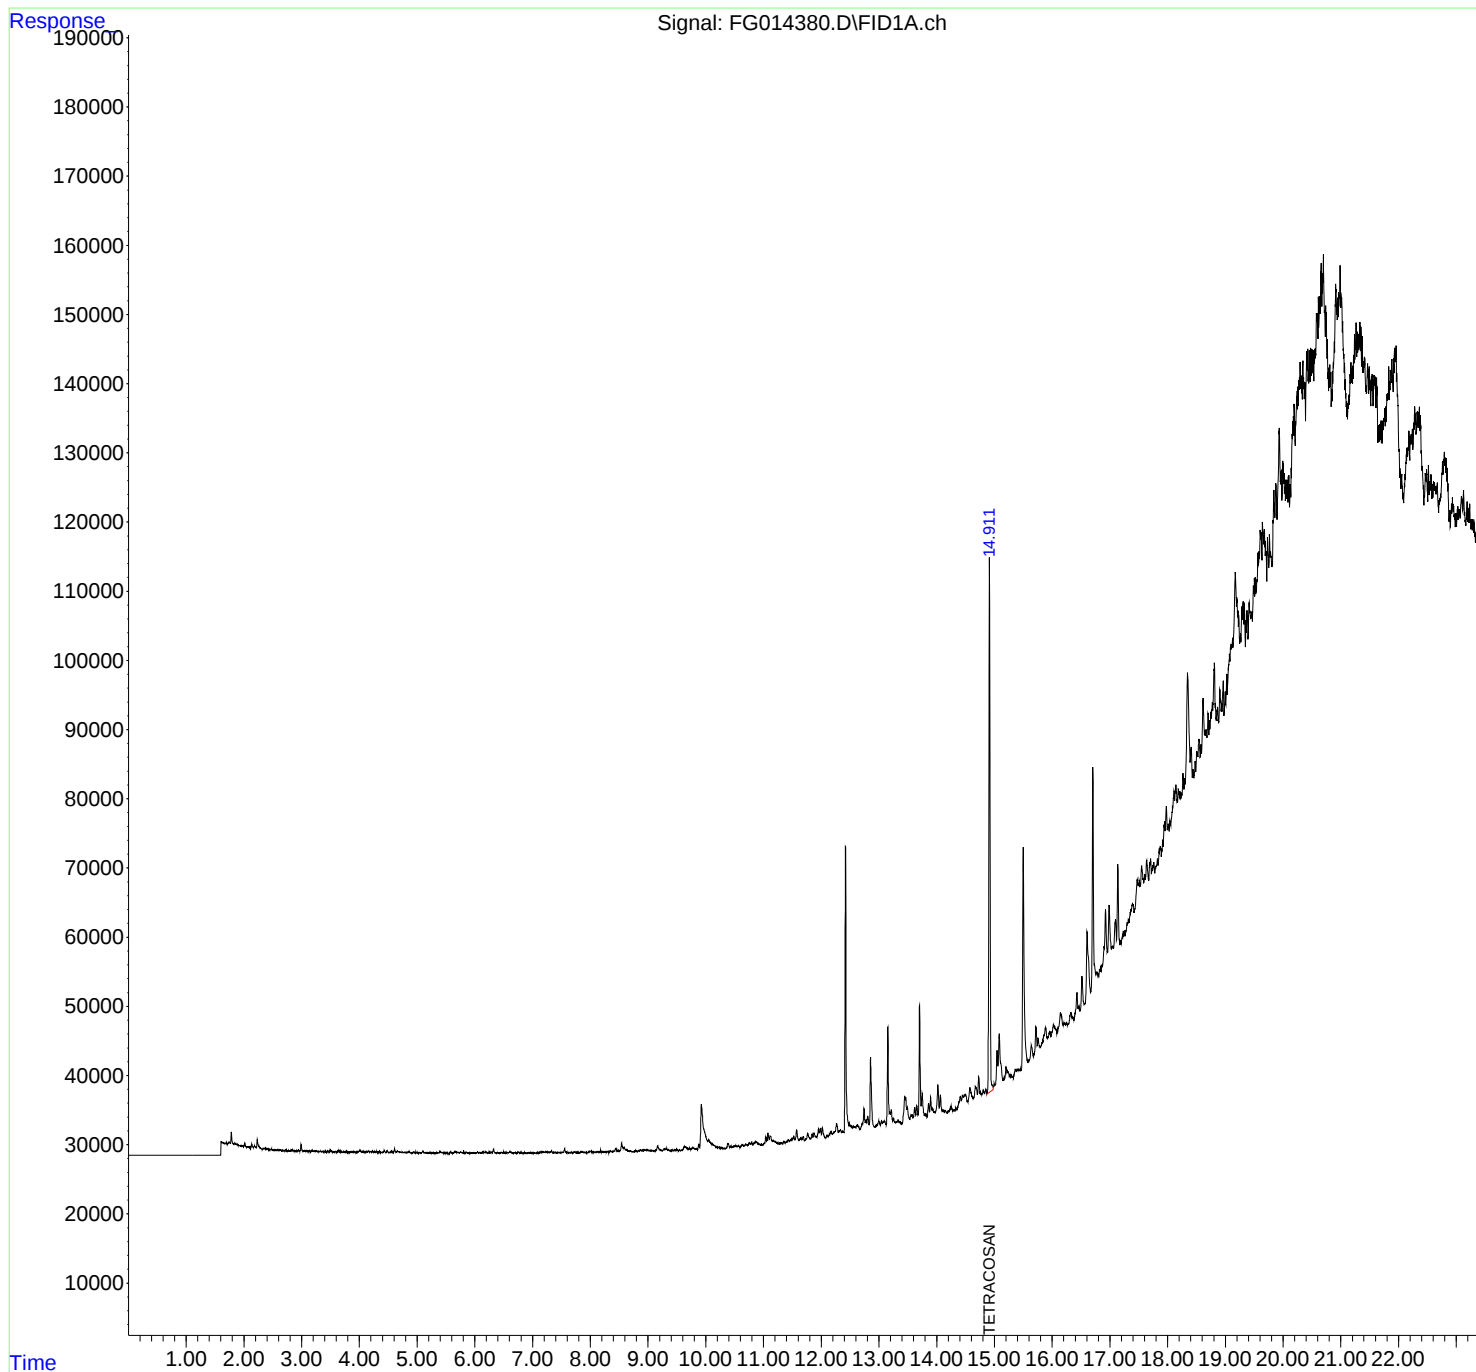

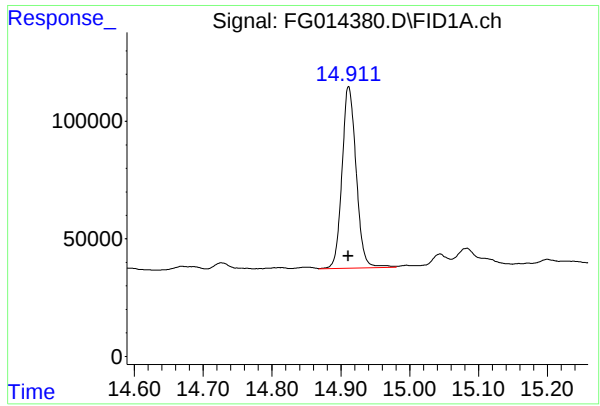

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.911 min
Delta R.T.: 0.000 min
Response: 1102889
Conc: 8.91 ug/ml

Instrument :
FID_G
ClientSampleId :
BU-03-10022024