

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG100421\
Data File : FG008771.D
Signal(s) : FID1A.ch
Acq On : 04 Oct 2021 16:34
Operator : DD\AJ
Sample : PB139592BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Oct 05 01:16:02 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG090721.M
Quant Title :
QLast Update : Wed Sep 08 09:33:21 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.740	2042771	18.393 ug/ml
Target Compounds			
14) N-DOTRIACONTANE	18.649	43261	0.405 ug/ml
16) N-HEXATRIACONTANE	20.176	23794	0.257 ug/ml
17) N-OCTATRIACONTANE	20.924	48824	0.554 ug/ml
18) N-TETRACONTANE	21.890	99283	1.067 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG100421\
Data File : FG008771.D
Signal(s) : FID1A.ch
Acq On : 04 Oct 2021 16:34
Operator : DD\AJ
Sample : PB139592BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Oct 05 01:16:02 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG090721.M
Quant Title :
QLast Update : Wed Sep 08 09:33:21 2021
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

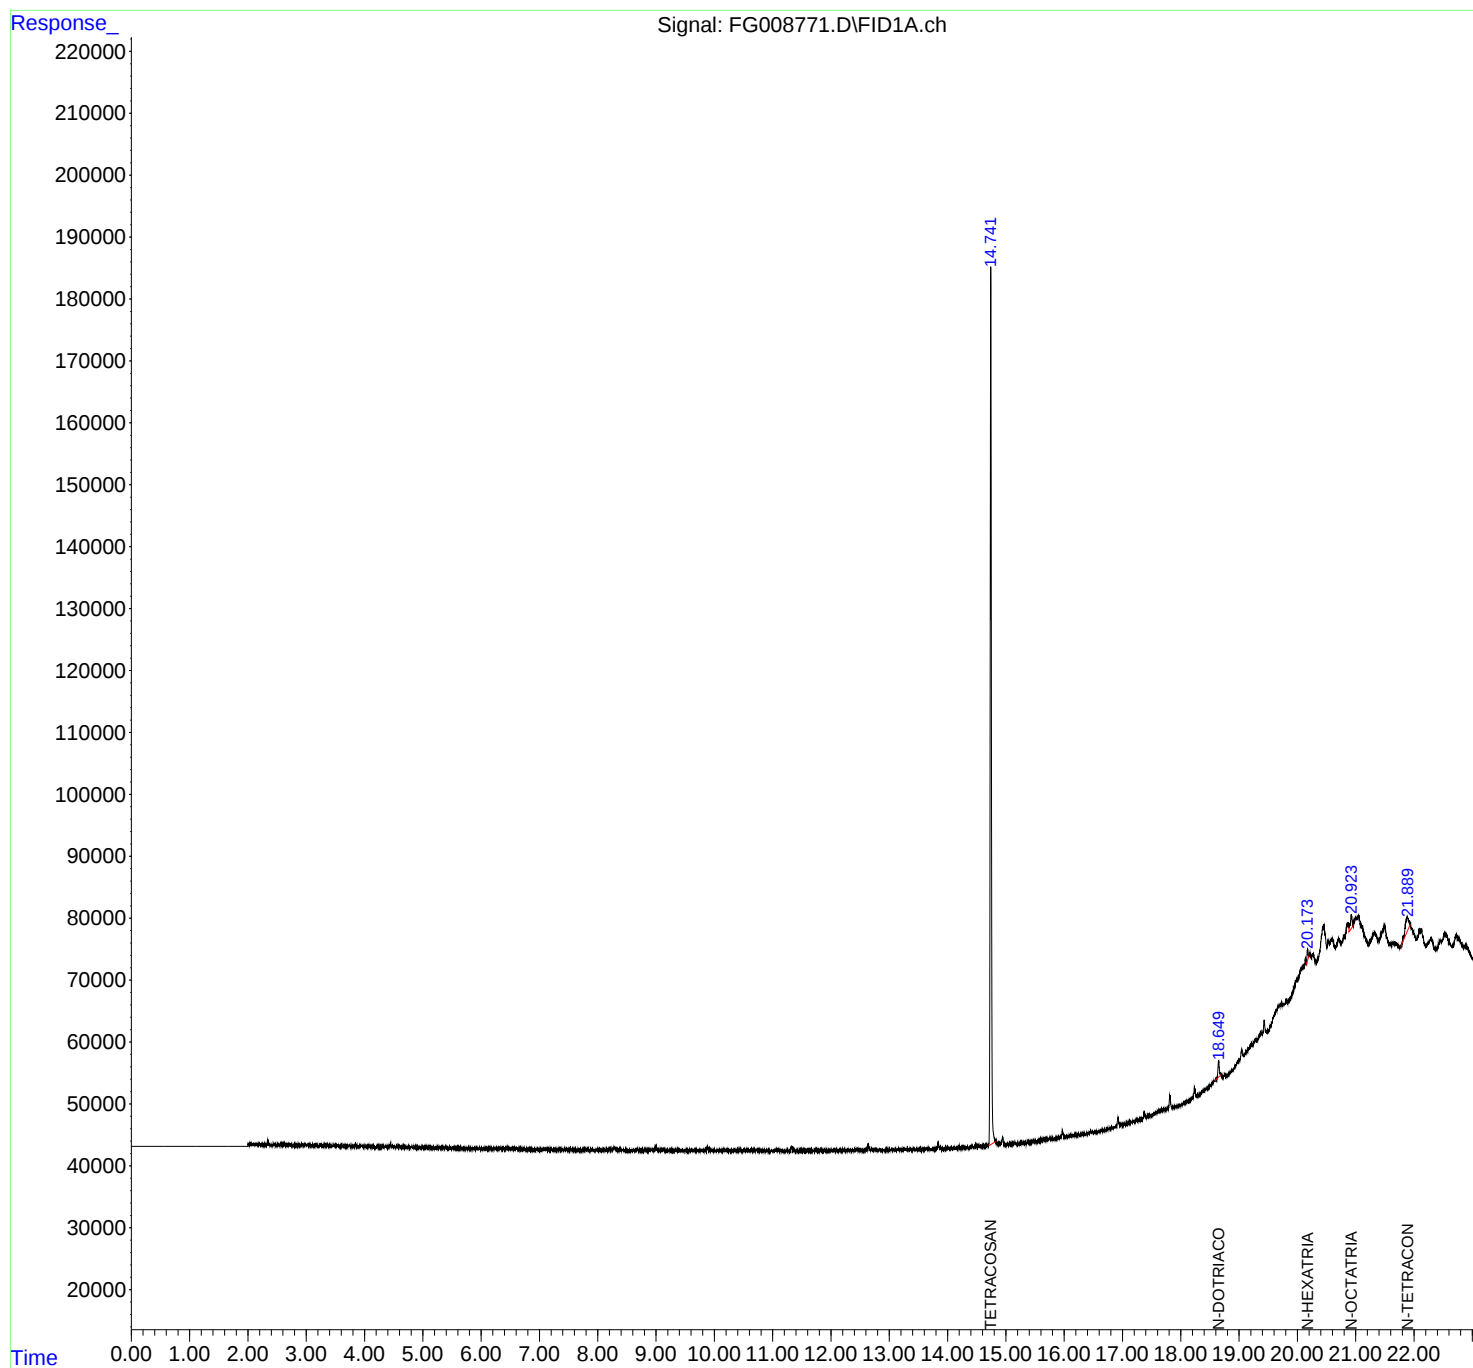

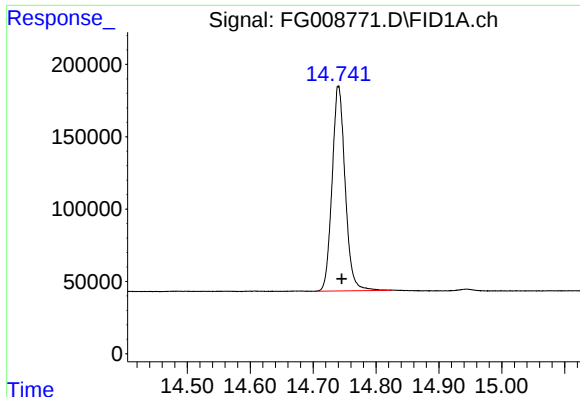


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.740 min
Delta R.T.: -0.005 min
Response: 2042771
Conc: 18.39 ug/ml

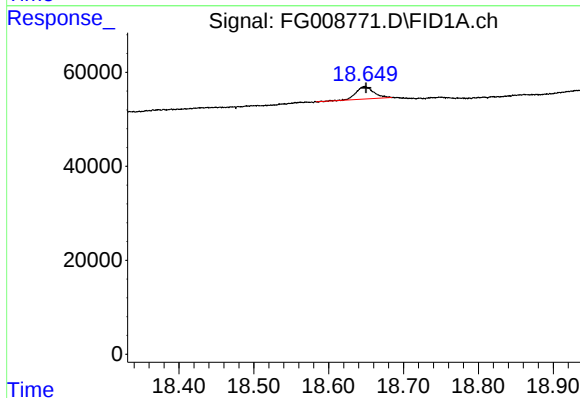


#14 N-DOTRIACONTANE

R.T.: 18.649 min
Delta R.T.: -0.001 min
Response: 43261
Conc: 0.41 ug/ml

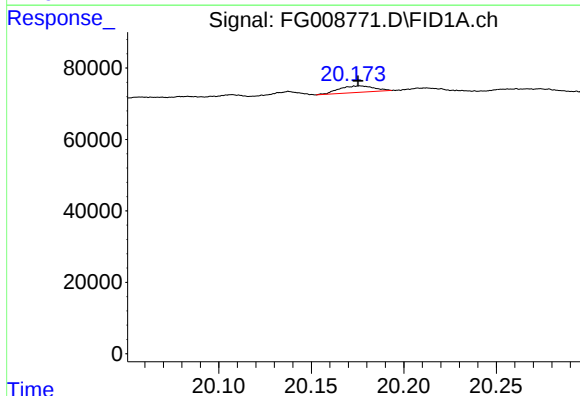


#16 N-HEXATRIACONTANE

R.T.: 20.176 min
Delta R.T.: 0.000 min
Response: 23794
Conc: 0.26 ug/ml

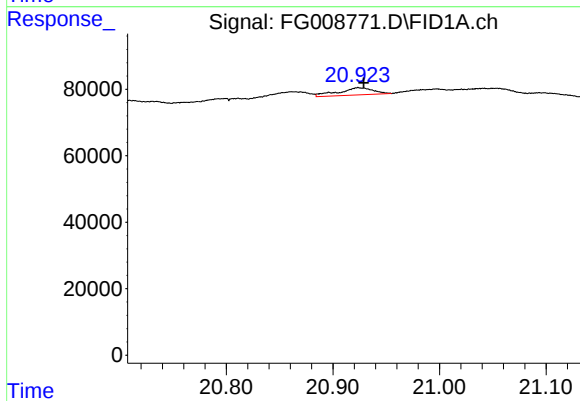

#17 N-OCTATRIACONTANE

R.T.: 20.924 min
Delta R.T.: -0.005 min
Response: 48824
Conc: 0.55 ug/ml

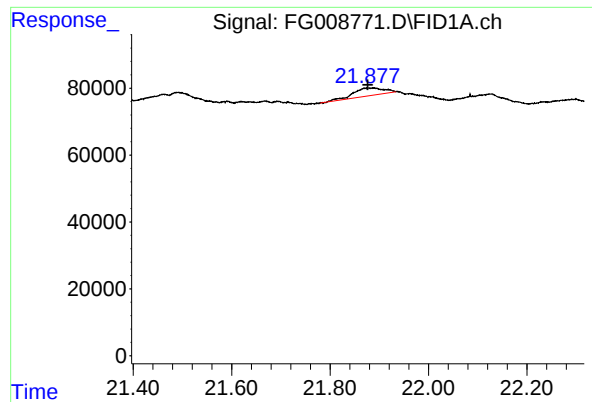

#18 N-TETRACONTANE

R.T.: 21.890 min
Delta R.T.: 0.013 min
Response: 99283
Conc: 1.07 ug/ml