

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG100421\
 Data File : FG008789.D
 Signal(s) : FID1A.ch
 Acq On : 05 Oct 2021 02:52
 Operator : DD\AJ
 Sample : 50 PPM TRPH STD
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Oct 05 04:02:58 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG090721.M
 Quant Title :
 QLast Update : Wed Sep 08 09:33:21 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.740	5595206	50.378 ug/ml
Target Compounds			
2) N-DECANE	4.444	6963775	52.095 ug/ml
3) N-DODECANE	6.471	6954754	51.345 ug/ml
4) N-TETRADECANE	8.272	6875996	50.688 ug/ml
5) N-HEXADECANE	9.877	6750339	50.403 ug/ml
6) N-OCTADECANE	11.324	6762413	50.254 ug/ml
7) N-EICOSANE	12.637	6686278	50.246 ug/ml
8) N-DOCOSANE	13.840	6494123	50.372 ug/ml
10) N-TETRACOSANE	14.947	6337574	50.113 ug/ml
11) N-HEXACOSANE	15.970	6074400	49.425 ug/ml
12) N-OCTACOSANE	16.921	5825852	48.512 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG100421\
Data File : FG008789.D
Signal(s) : FID1A.ch
Acq On : 05 Oct 2021 02:52
Operator : DD\AJ
Sample : 50 PPM TRPH STD
Misc :
ALS Vial : 3 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Oct 05 04:02:58 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG090721.M
Quant Title :
QLast Update : Wed Sep 08 09:33:21 2021
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

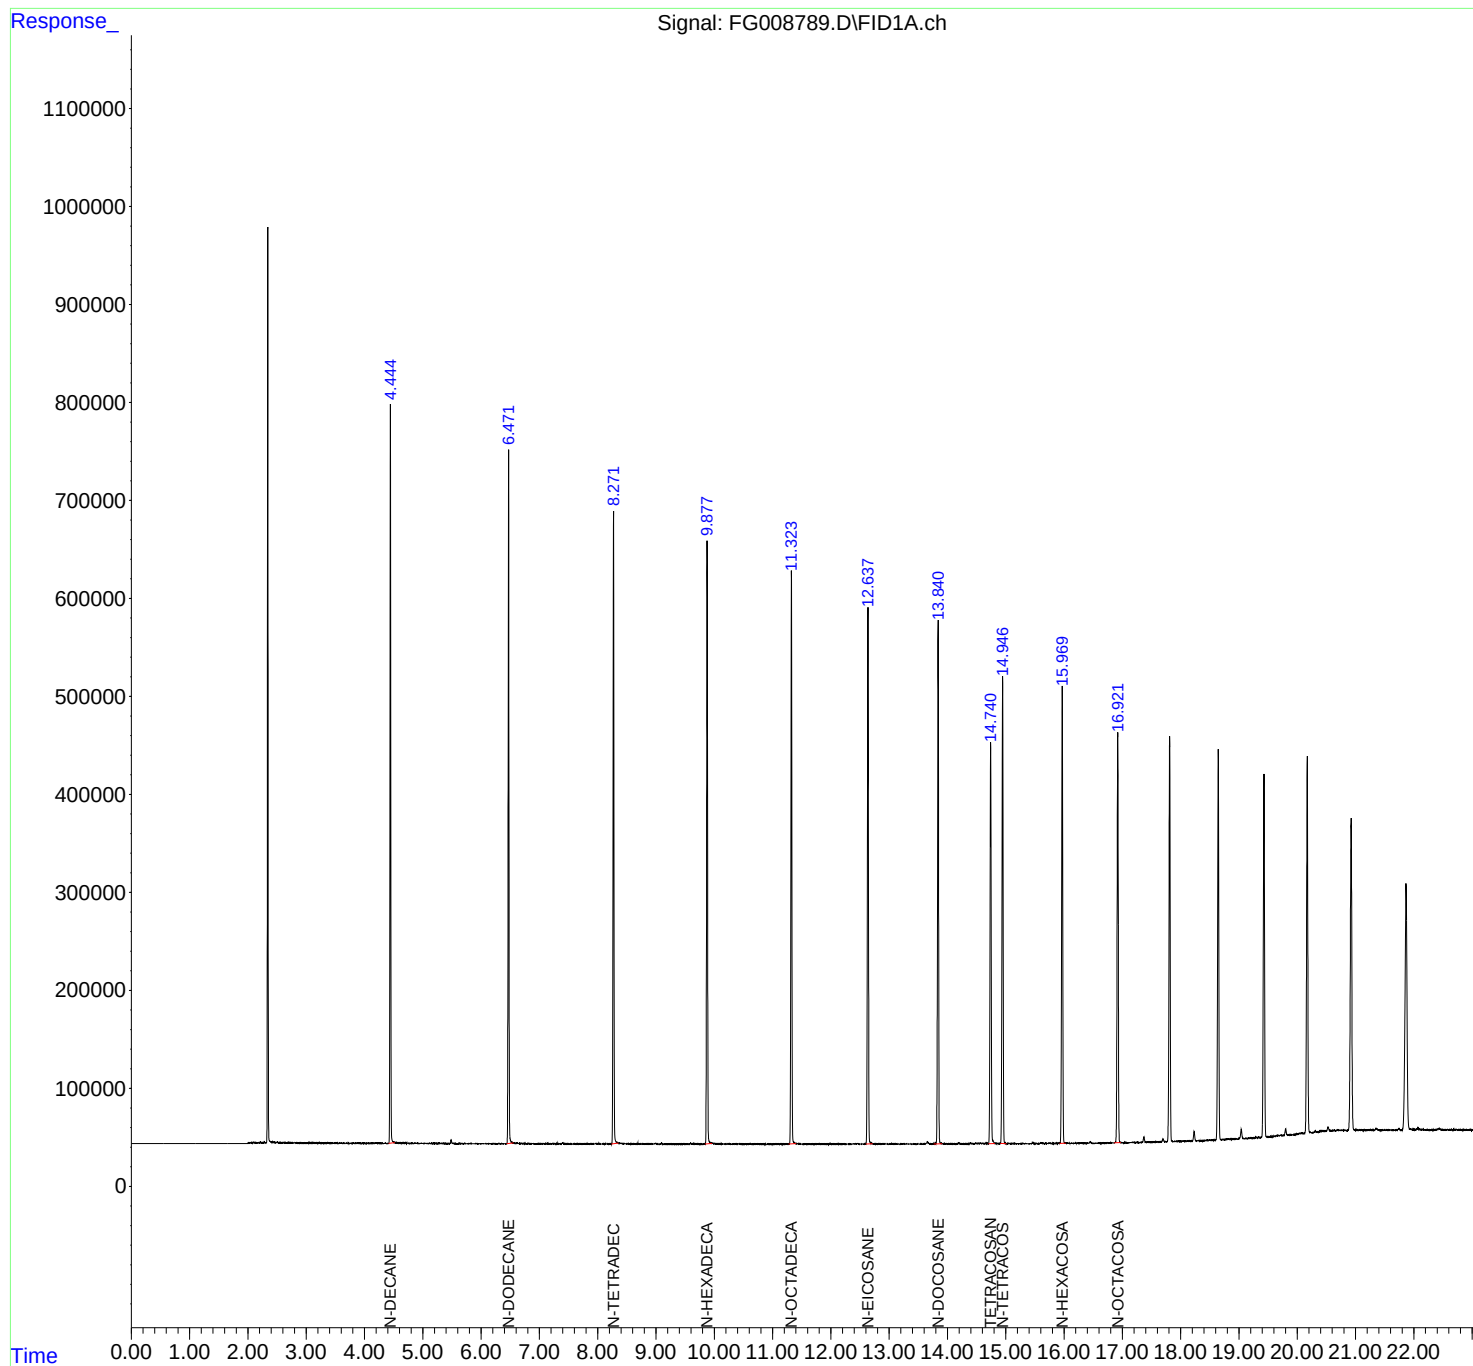

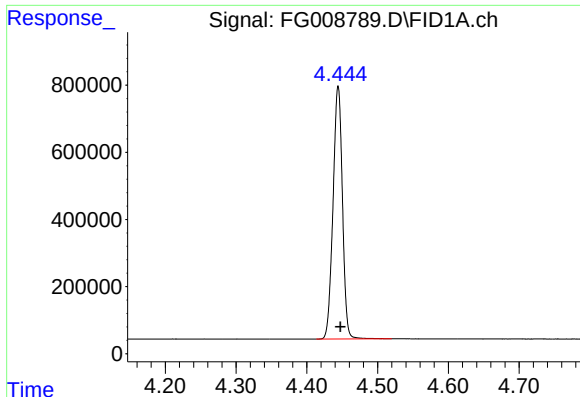


#2 N-DECANE

R.T.: 4.444 min
Delta R.T.: -0.003 min
Response: 6963775
Conc: 52.09 ug/ml

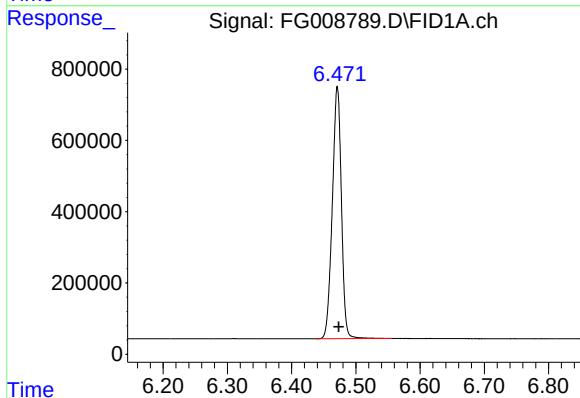


#3 N-DODECANE

R.T.: 6.471 min
Delta R.T.: -0.002 min
Response: 6954754
Conc: 51.35 ug/ml

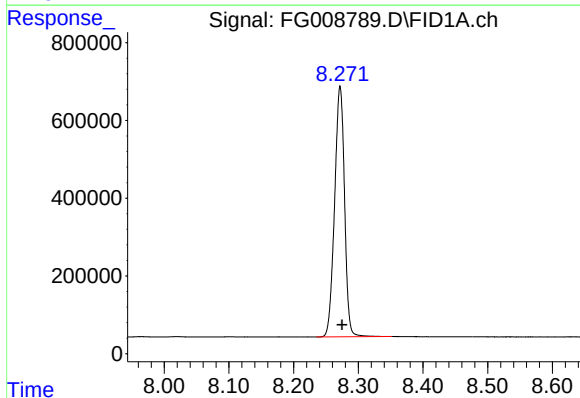


#4 N-TETRADECANE

R.T.: 8.272 min
Delta R.T.: -0.003 min
Response: 6875996
Conc: 50.69 ug/ml

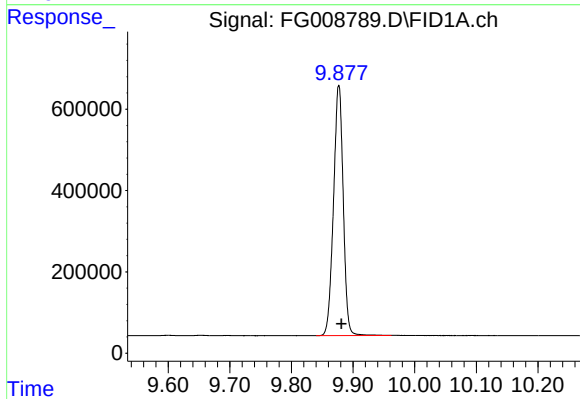


#5 N-HEXADECANE

R.T.: 9.877 min
Delta R.T.: -0.004 min
Response: 6750339
Conc: 50.40 ug/ml

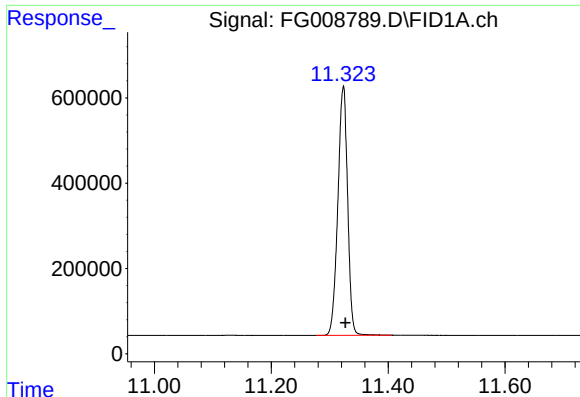


#6 N-OCTADECANE

R.T.: 11.324 min
Delta R.T.: -0.003 min
Response: 6762413
Conc: 50.25 ug/ml

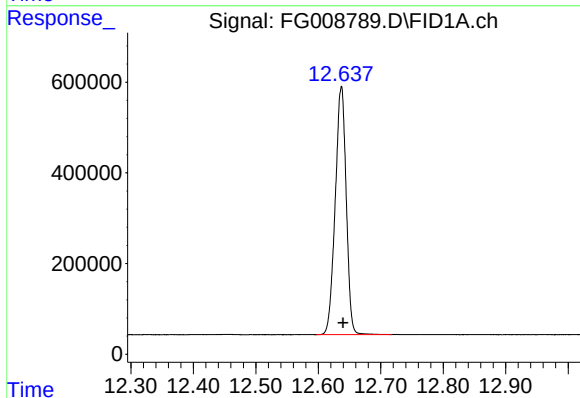


#7 N-EICOSANE

R.T.: 12.637 min
Delta R.T.: -0.002 min
Response: 6686278
Conc: 50.25 ug/ml

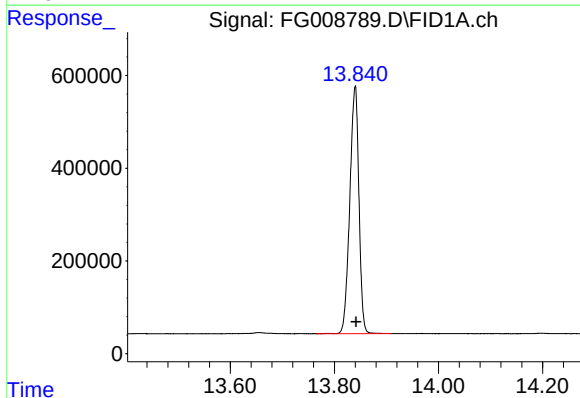


#8 N-DOCOSANE

R.T.: 13.840 min
Delta R.T.: -0.001 min
Response: 6494123
Conc: 50.37 ug/ml

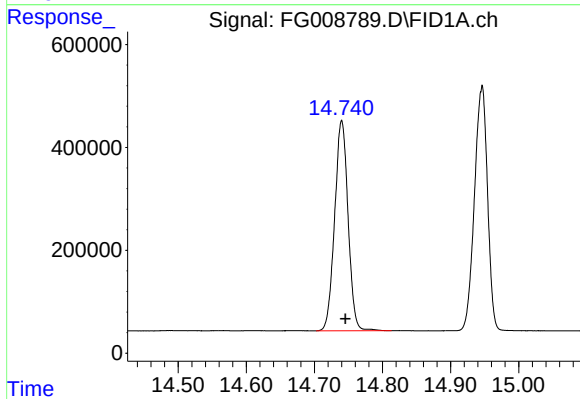


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.740 min
Delta R.T.: -0.006 min
Response: 5595206
Conc: 50.38 ug/ml

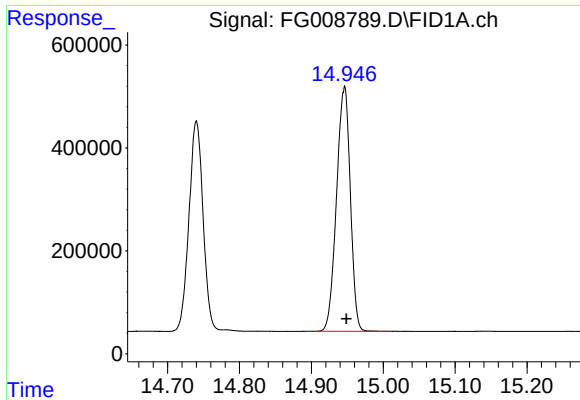


#10 N-TETRACOSANE

R.T.: 14.947 min
Delta R.T.: -0.002 min
Response: 6337574
Conc: 50.11 ug/ml

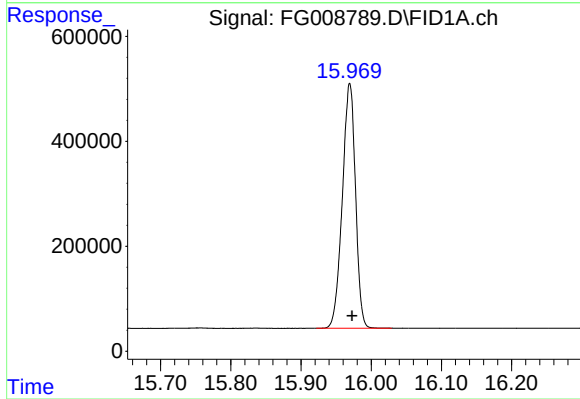

#11 N-HEXACOSANE

R.T.: 15.970 min
Delta R.T.: -0.003 min
Response: 6074400
Conc: 49.42 ug/ml

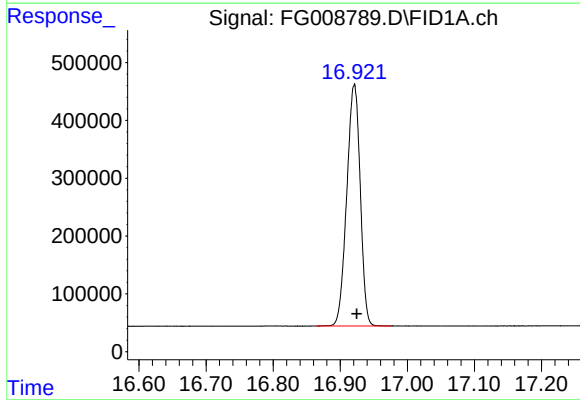

#12 N-OCTACOSANE

R.T.: 16.921 min
Delta R.T.: -0.004 min
Response: 5825852
Conc: 48.51 ug/ml