

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG100518\
 Data File : FG002519.D
 Signal(s) : FID1A.ch
 Acq On : 05 Oct 2018 15:29
 Operator : AJ\SJ
 Sample : J5195-01 5X
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Oct 06 00:43:06 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG100118.M
 Quant Title :
 QLast Update : Mon Oct 01 12:36:17 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.756	285293	2.486 ug/ml
Target Compounds			
3) N-DODECANE	6.490	252074	1.910 ug/ml
4) N-TETRADECANE	8.289	404366	3.033 ug/ml
5) N-HEXADECANE	9.896	226819	1.691 ug/ml
6) N-OCTADECANE	11.341	99520	0.739 ug/ml
7) N-EICOSANE	12.655	149116	1.118 ug/ml
11) N-HEXACOSANE	15.986	78783	0.613 ug/ml
12) N-OCTACOSANE	16.936	132659	1.046 ug/ml
13) N-TRIACONTANE	17.829	233228	1.854 ug/ml
14) N-DOTRIACONTANE	18.662	258035	2.102 ug/ml
15) N-TETRATRIACONTANE	19.448	237337	1.989 ug/ml
16) N-HEXATRIACONTANE	20.195	248456	2.239 ug/ml
17) N-OCTATRIACONTANE	20.956	114716	1.170 ug/ml
18) N-TETRACONTANE	21.921	102460	1.095 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG100518\
Data File : FG002519.D
Signal(s) : FID1A.ch
Acq On : 05 Oct 2018 15:29
Operator : AJ\SJ
Sample : J5195-01 5X
Misc :
ALS Vial : 9 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Oct 06 00:43:06 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG100118.M
Quant Title :
QLast Update : Mon Oct 01 12:36:17 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

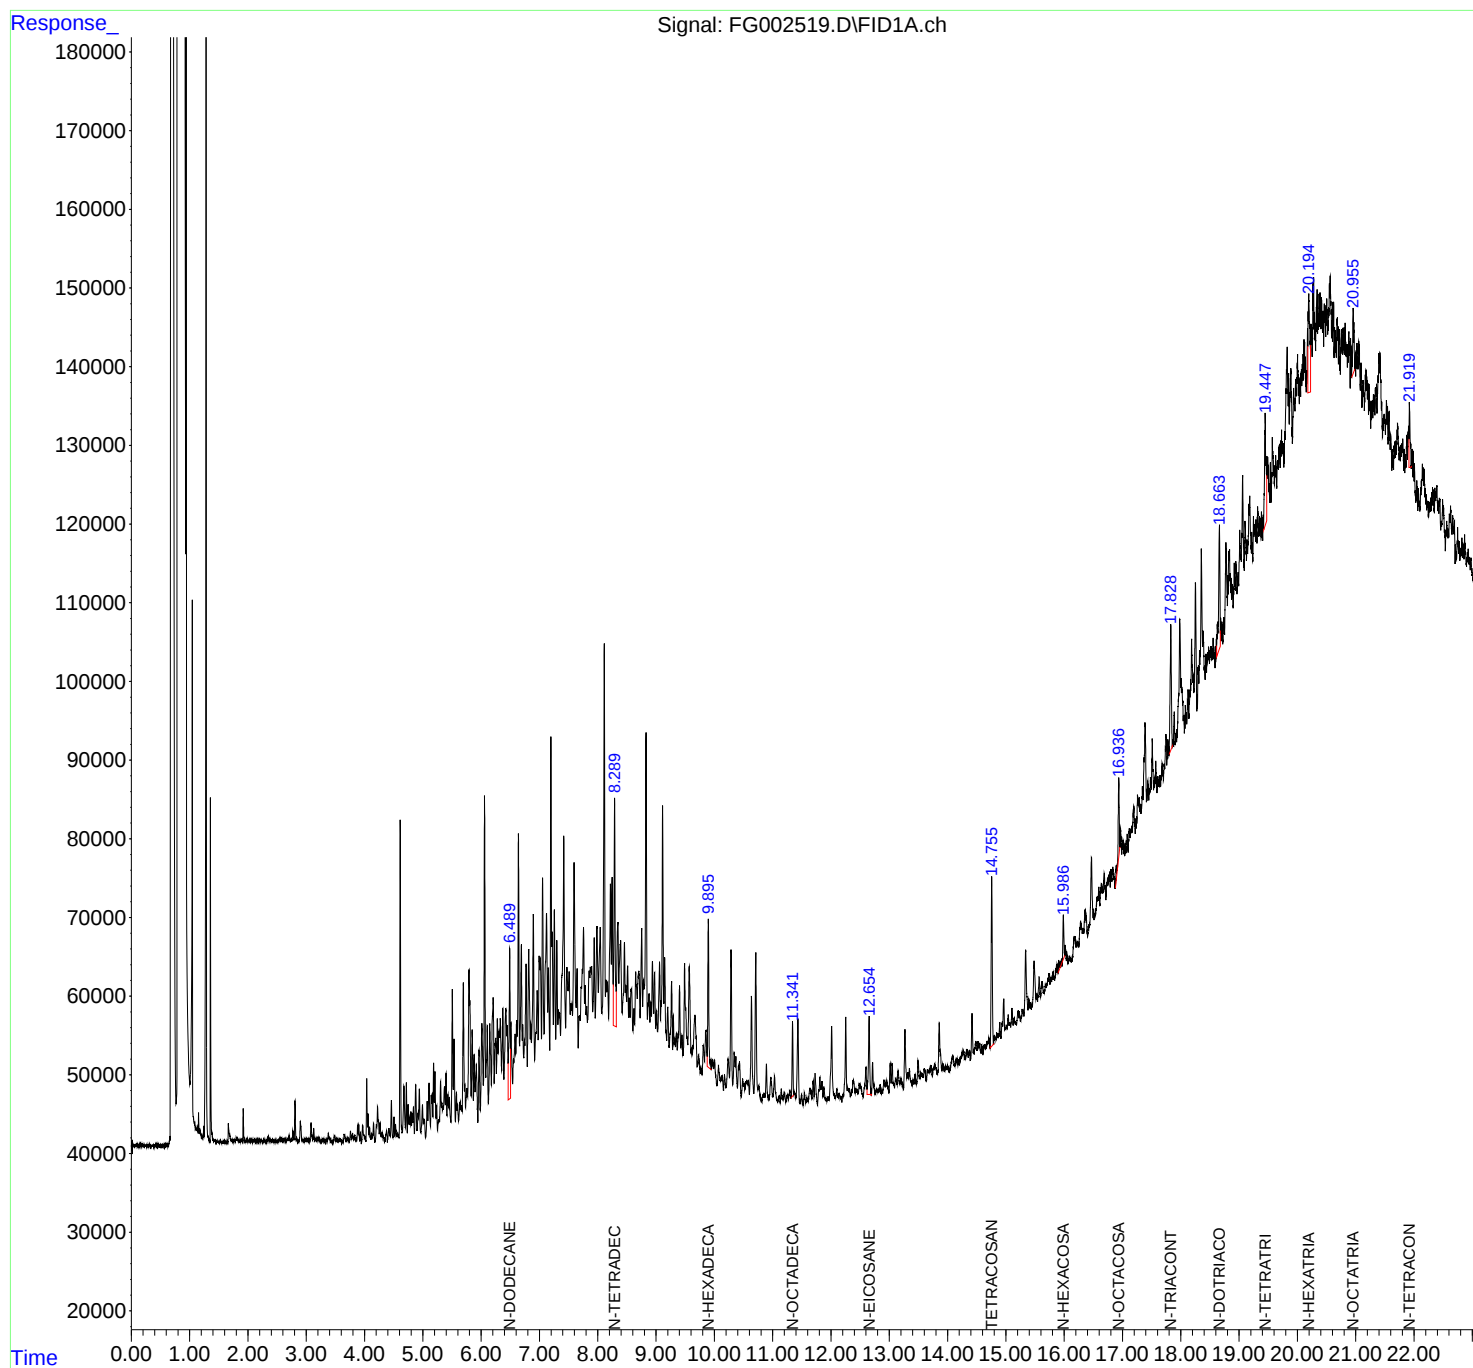

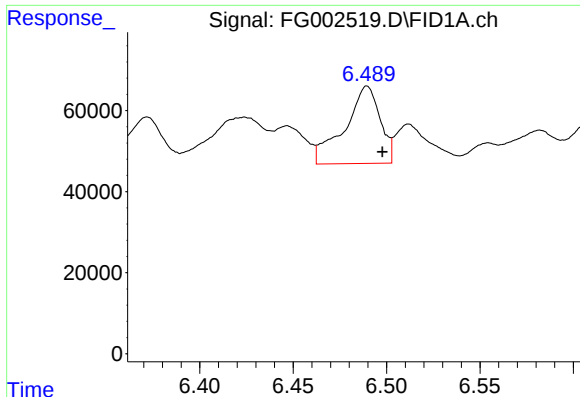


#3 N-DODECANE

R.T.: 6.490 min
Delta R.T.: -0.008 min
Response: 252074
Conc: 1.91 ug/ml

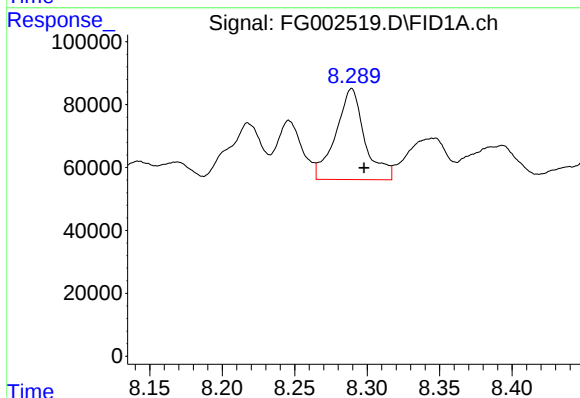


#4 N-TETRADECANE

R.T.: 8.289 min
Delta R.T.: -0.009 min
Response: 404366
Conc: 3.03 ug/ml

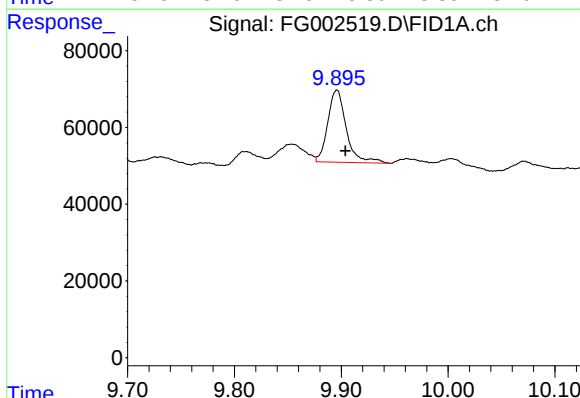


#5 N-HEXADECANE

R.T.: 9.896 min
Delta R.T.: -0.008 min
Response: 226819
Conc: 1.69 ug/ml

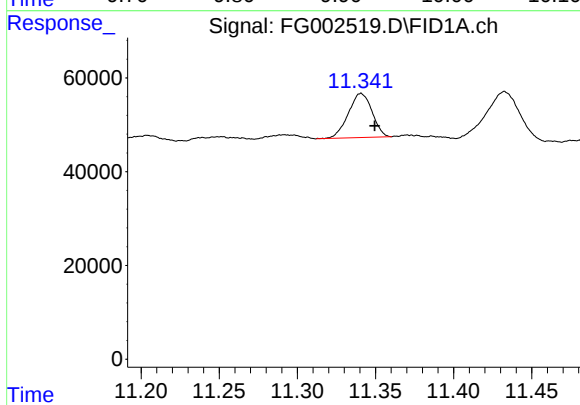


#6 N-OCTADECANE

R.T.: 11.341 min
Delta R.T.: -0.009 min
Response: 99520
Conc: 0.74 ug/ml

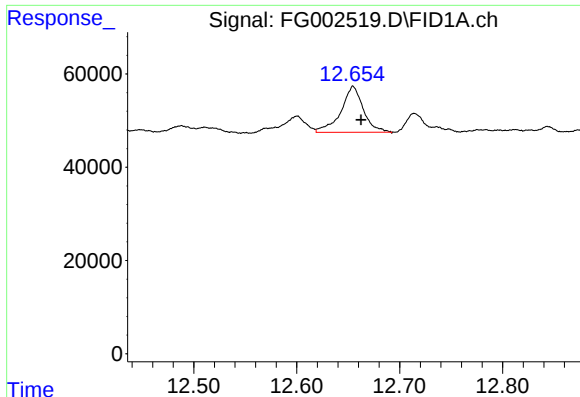


#7 N-EICOSANE

R.T.: 12.655 min
Delta R.T.: -0.008 min
Response: 149116
Conc: 1.12 ug/ml

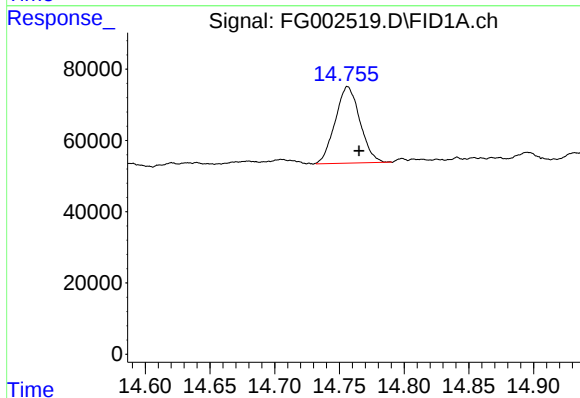


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.756 min
Delta R.T.: -0.009 min
Response: 285293
Conc: 2.49 ug/ml

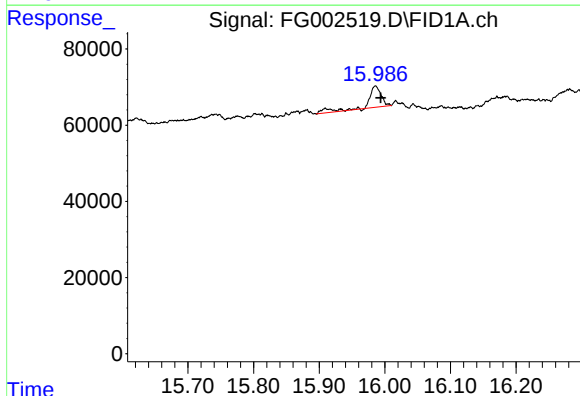


#11 N-HEXACOSANE

R.T.: 15.986 min
Delta R.T.: -0.008 min
Response: 78783
Conc: 0.61 ug/ml

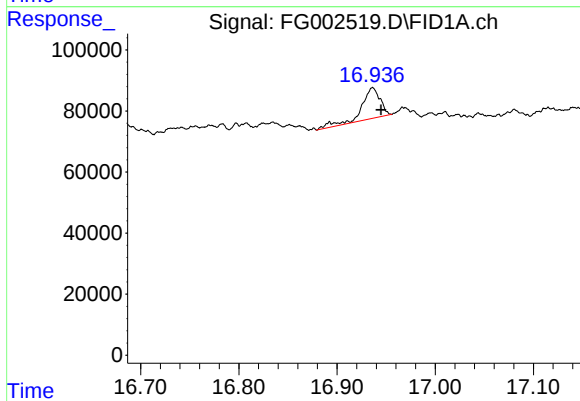


#12 N-OCTACOSANE

R.T.: 16.936 min
Delta R.T.: -0.009 min
Response: 132659
Conc: 1.05 ug/ml

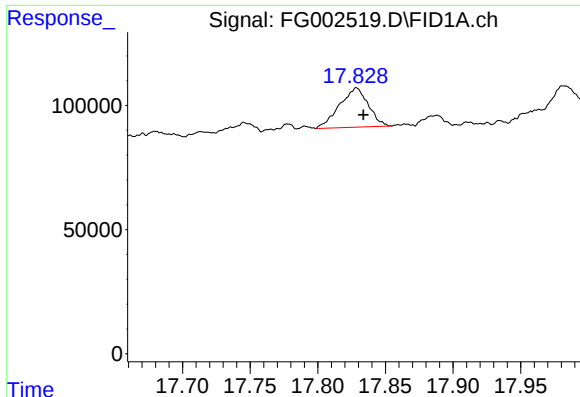


#13 N-TRIACONTANE

R.T.: 17.829 min
Delta R.T.: -0.005 min
Response: 233228
Conc: 1.85 ug/ml

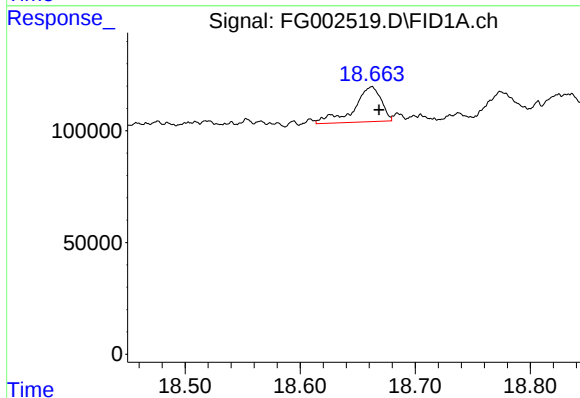


#14 N-DOTRIACONTANE

R.T.: 18.662 min
Delta R.T.: -0.006 min
Response: 258035
Conc: 2.10 ug/ml

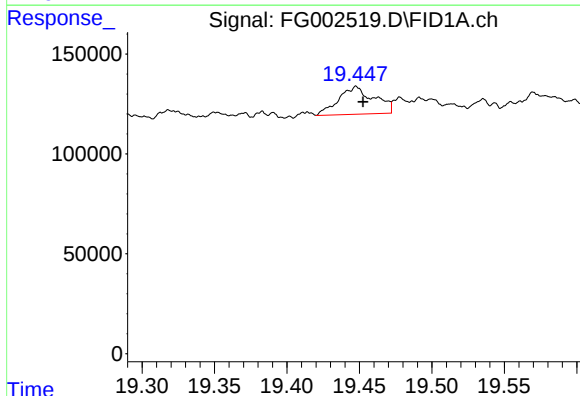


#15 N-TETRATRIACONTANE

R.T.: 19.448 min
Delta R.T.: -0.005 min
Response: 237337
Conc: 1.99 ug/ml

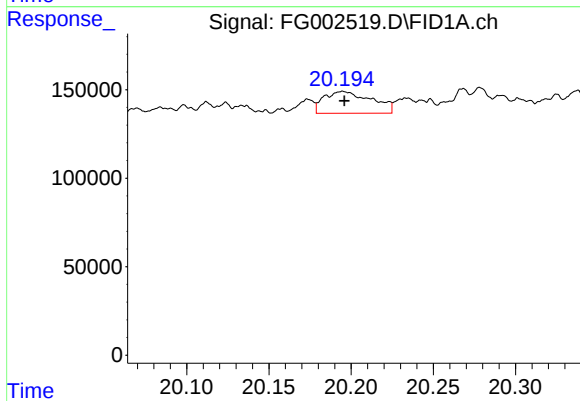


#16 N-HEXATRIACONTANE

R.T.: 20.195 min
Delta R.T.: -0.001 min
Response: 248456
Conc: 2.24 ug/ml

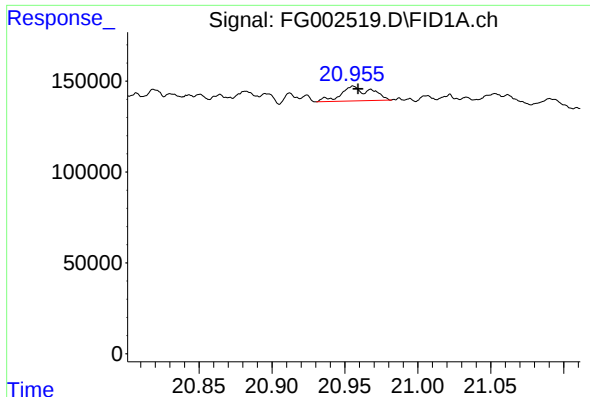

#17 N-OCTATRIACONTANE

R.T.: 20.956 min
Delta R.T.: -0.003 min
Response: 114716
Conc: 1.17 ug/ml

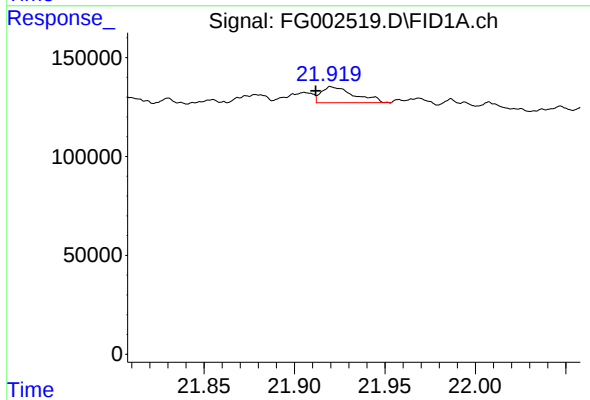

#18 N-TETRACONTANE

R.T.: 21.921 min
Delta R.T.: 0.009 min
Response: 102460
Conc: 1.10 ug/ml