

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG100518\
Data File : FG002520.D
Signal(s) : FID1A.ch
Acq On : 05 Oct 2018 15:59
Operator : AJ\SJ
Sample : J5204-03 10X
Misc :
ALS Vial : 10 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Oct 06 00:43:19 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG100118.M
Quant Title :
QLast Update : Mon Oct 01 12:36:17 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
9) S	TETRACOSANE-d50 (SURR...	14.757	254417	2.217 ug/ml
Target Compounds				
7)	N-EICOSANE	12.717f	1218270	9.133 ug/ml
8)	N-DOCOSANE	13.884	341773	2.590 ug/ml
10)	N-TETRACOSANE	14.940	872814	6.714 ug/ml
11)	N-HEXACOSANE	15.991	129256	1.006 ug/ml
12)	N-OCTACOSANE	16.942	386643	3.050 ug/ml
13)	N-TRIACONTANE	17.837	147612	1.173 ug/ml
14)	N-DOTRIACONTANE	18.656	121623	0.991 ug/ml
15)	N-TETRATRIACONTANE	19.448	139424	1.168 ug/ml
16)	N-HEXATRIACONTANE	20.200	144720	1.304 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG100518\
Data File : FG002520.D
Signal(s) : FID1A.ch
Acq On : 05 Oct 2018 15:59
Operator : AJ\SJ
Sample : J5204-03 10X
Misc :
ALS Vial : 10 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Oct 06 00:43:19 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG100118.M
Quant Title :
QLast Update : Mon Oct 01 12:36:17 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

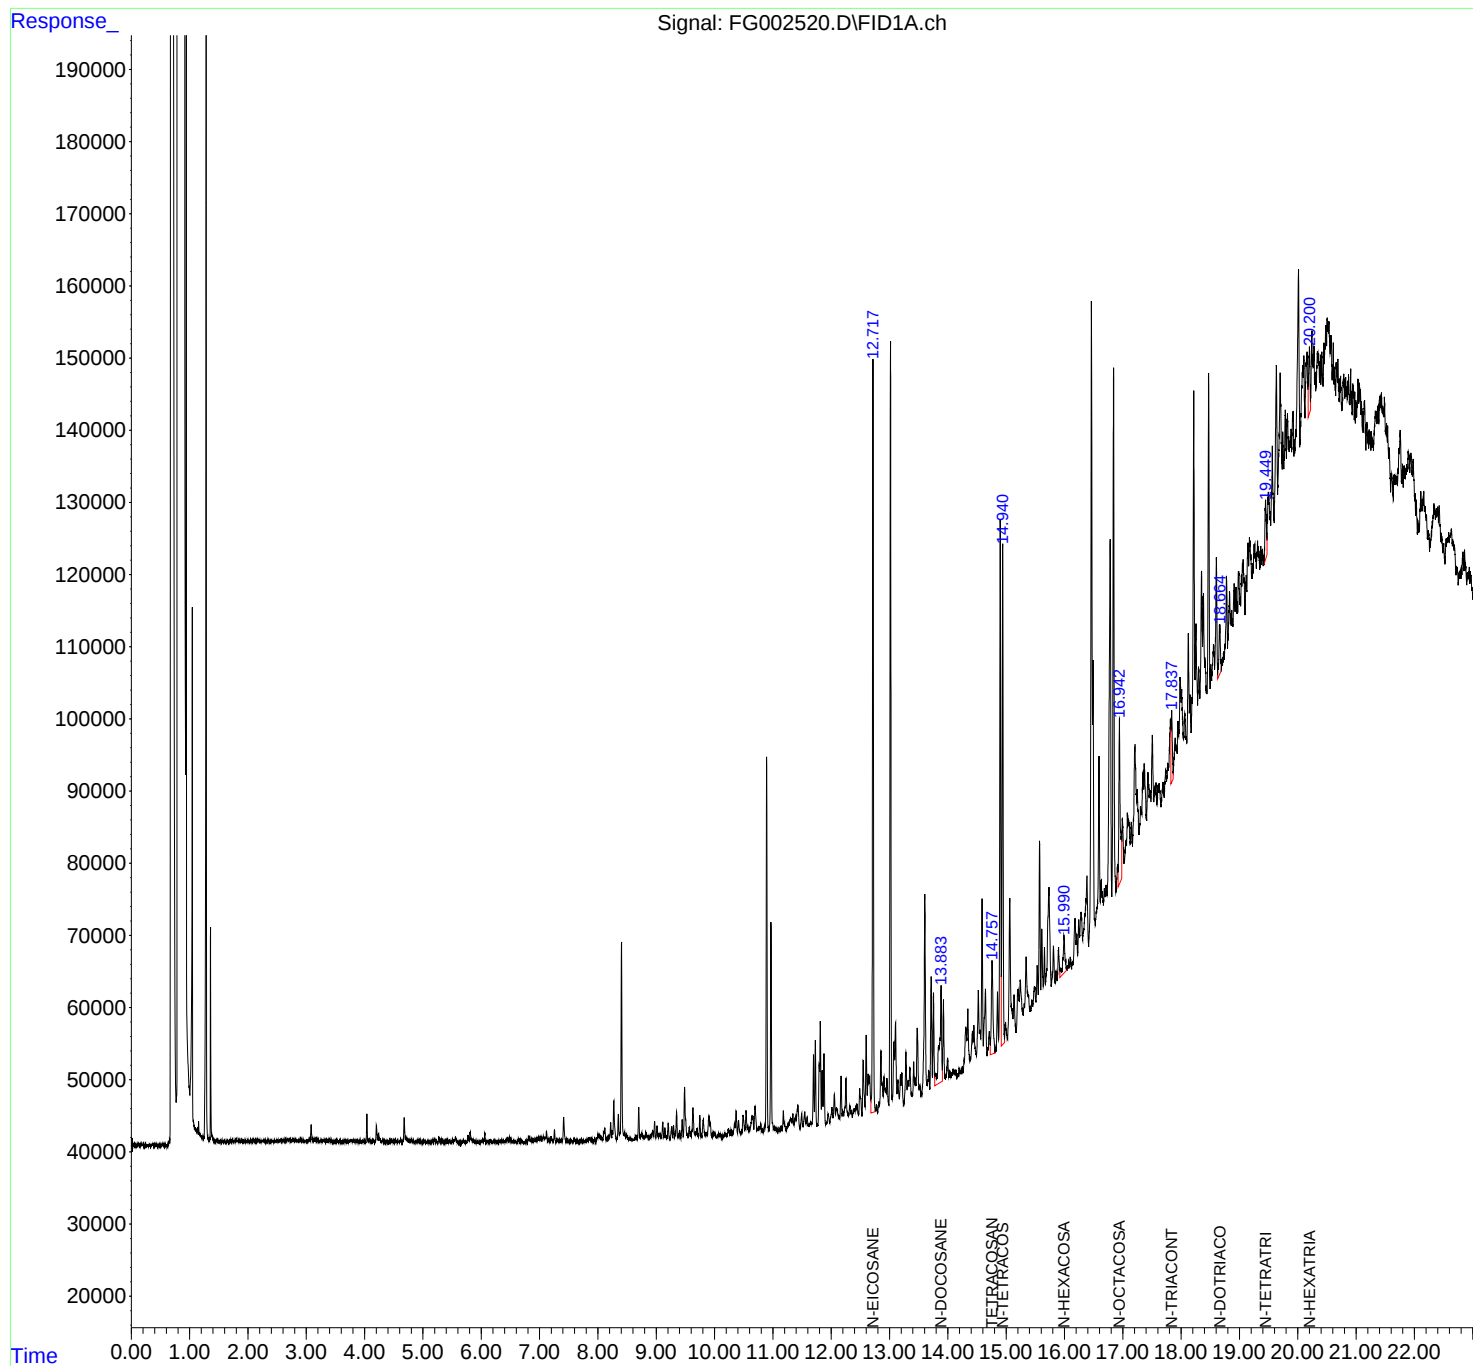

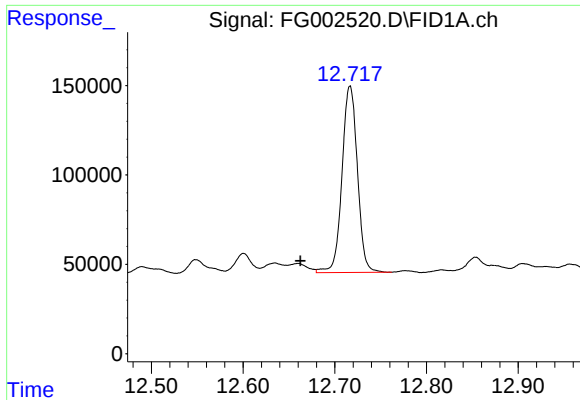


#7 N-EICOSANE

R.T.: 12.717 min
Delta R.T.: 0.054 min
Response: 1218270
Conc: 9.13 ug/ml

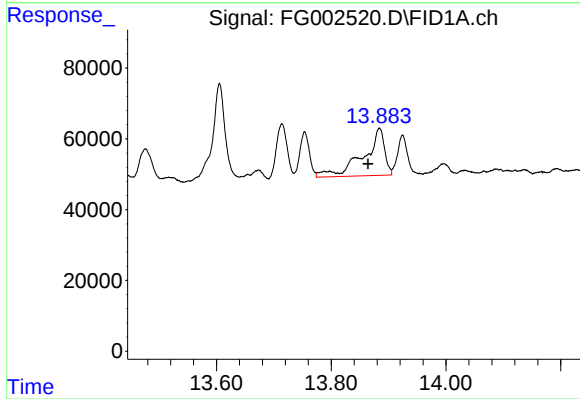


#8 N-DOCOSANE

R.T.: 13.884 min
Delta R.T.: 0.020 min
Response: 341773
Conc: 2.59 ug/ml

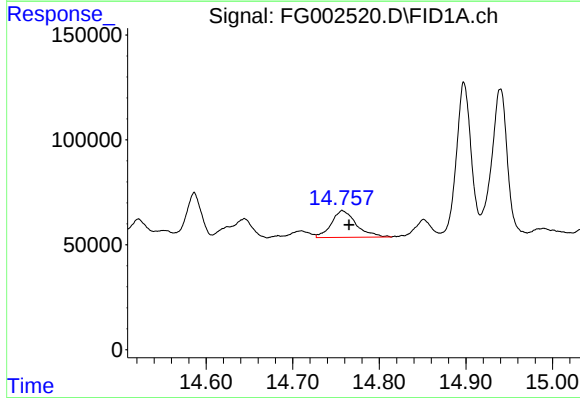


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.757 min
Delta R.T.: -0.008 min
Response: 254417
Conc: 2.22 ug/ml

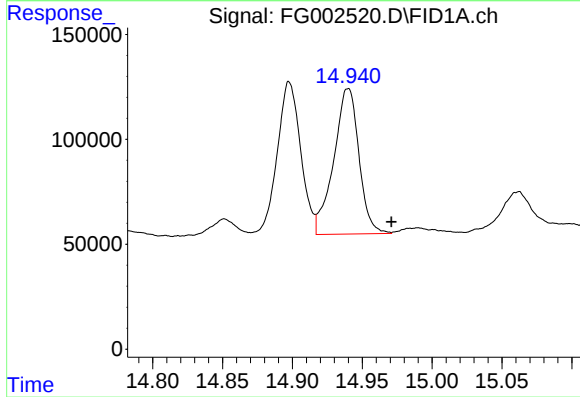


#10 N-TETRACOSANE

R.T.: 14.940 min
Delta R.T.: -0.031 min
Response: 872814
Conc: 6.71 ug/ml

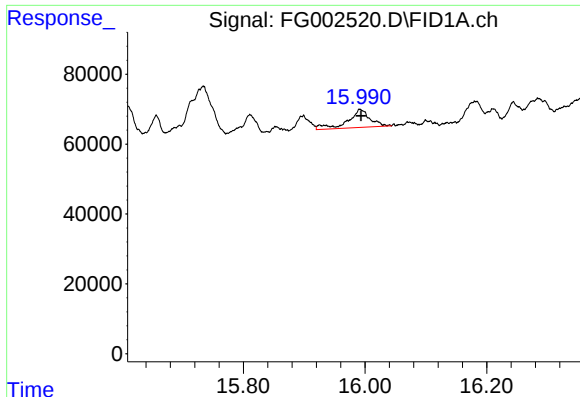


#11 N-HEXACOSANE

R.T.: 15.991 min
Delta R.T.: -0.002 min
Response: 129256
Conc: 1.01 ug/ml

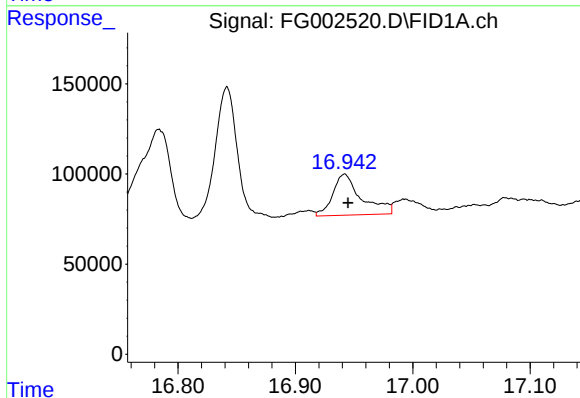


#12 N-OCTACOSANE

R.T.: 16.942 min
Delta R.T.: -0.003 min
Response: 386643
Conc: 3.05 ug/ml

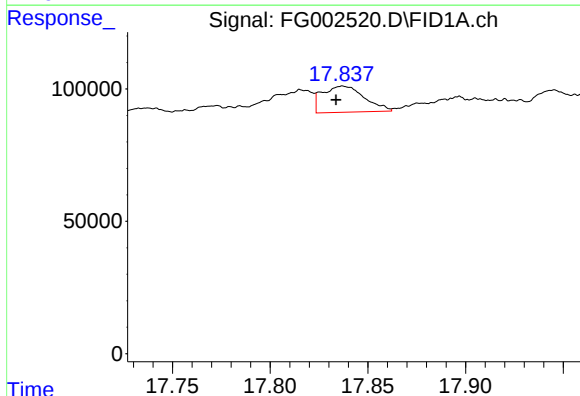


#13 N-TRIACONTANE

R.T.: 17.837 min
Delta R.T.: 0.004 min
Response: 147612
Conc: 1.17 ug/ml

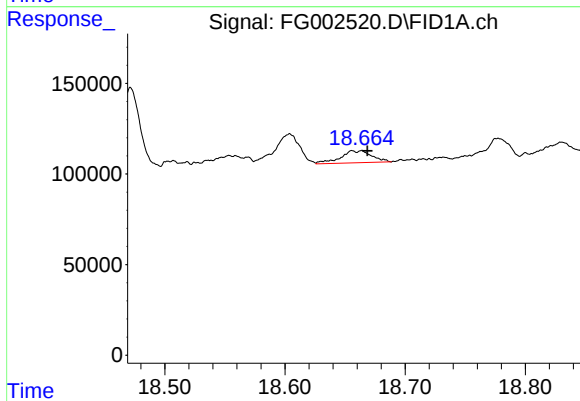

#14 N-DOTRIACONTANE

R.T.: 18.656 min
Delta R.T.: -0.012 min
Response: 121623
Conc: 0.99 ug/ml

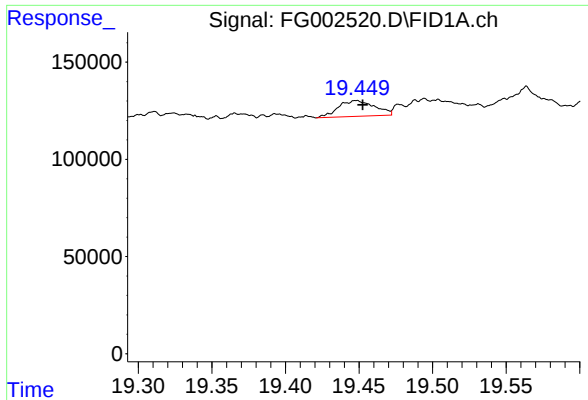


#15 N-TETRATRIACONTANE

R.T.: 19.448 min

Delta R.T.: -0.005 min

Response: 139424

Conc: 1.17 ug/ml

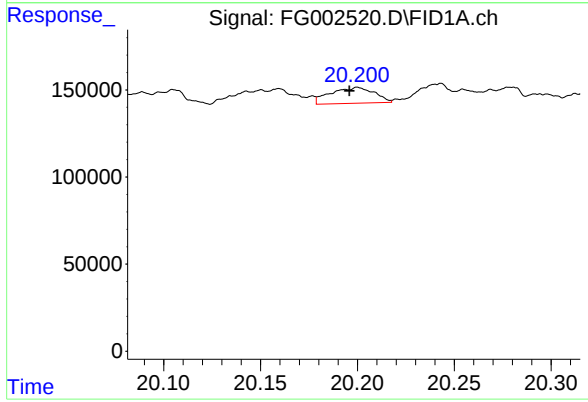

#16 N-HEXATRIACONTANE

R.T.: 20.200 min

Delta R.T.: 0.004 min

Response: 144720

Conc: 1.30 ug/ml