

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG100518\
Data File : FG002531.D
Signal(s) : FID1A.ch
Acq On : 05 Oct 2018 21:32
Operator : AJ\SJ
Sample : RT MARKER
Misc :
ALS Vial : 4 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Oct 06 00:45:29 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG100118.M
Quant Title :
QLast Update : Mon Oct 01 12:36:17 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
3) N-DODECANE	6.490	2398803	18.177 ug/ml
12) N-OCTACOSANE	16.933	2378110	18.757 ug/ml
13) N-TRIACONTANE	17.822	194387	1.545 ug/ml
14) N-DOTRIACONTANE	18.654	228570	1.862 ug/ml
15) N-TETRATRIACONTANE	19.441	154571	1.295 ug/ml
16) N-HEXATRIACONTANE	20.183	90219	0.813 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG100518\
Data File : FG002531.D
Signal(s) : FID1A.ch
Acq On : 05 Oct 2018 21:32
Operator : AJ\SJ
Sample : RT MARKER
Misc :
ALS Vial : 4 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Oct 06 00:45:29 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG100118.M
Quant Title :
QLast Update : Mon Oct 01 12:36:17 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

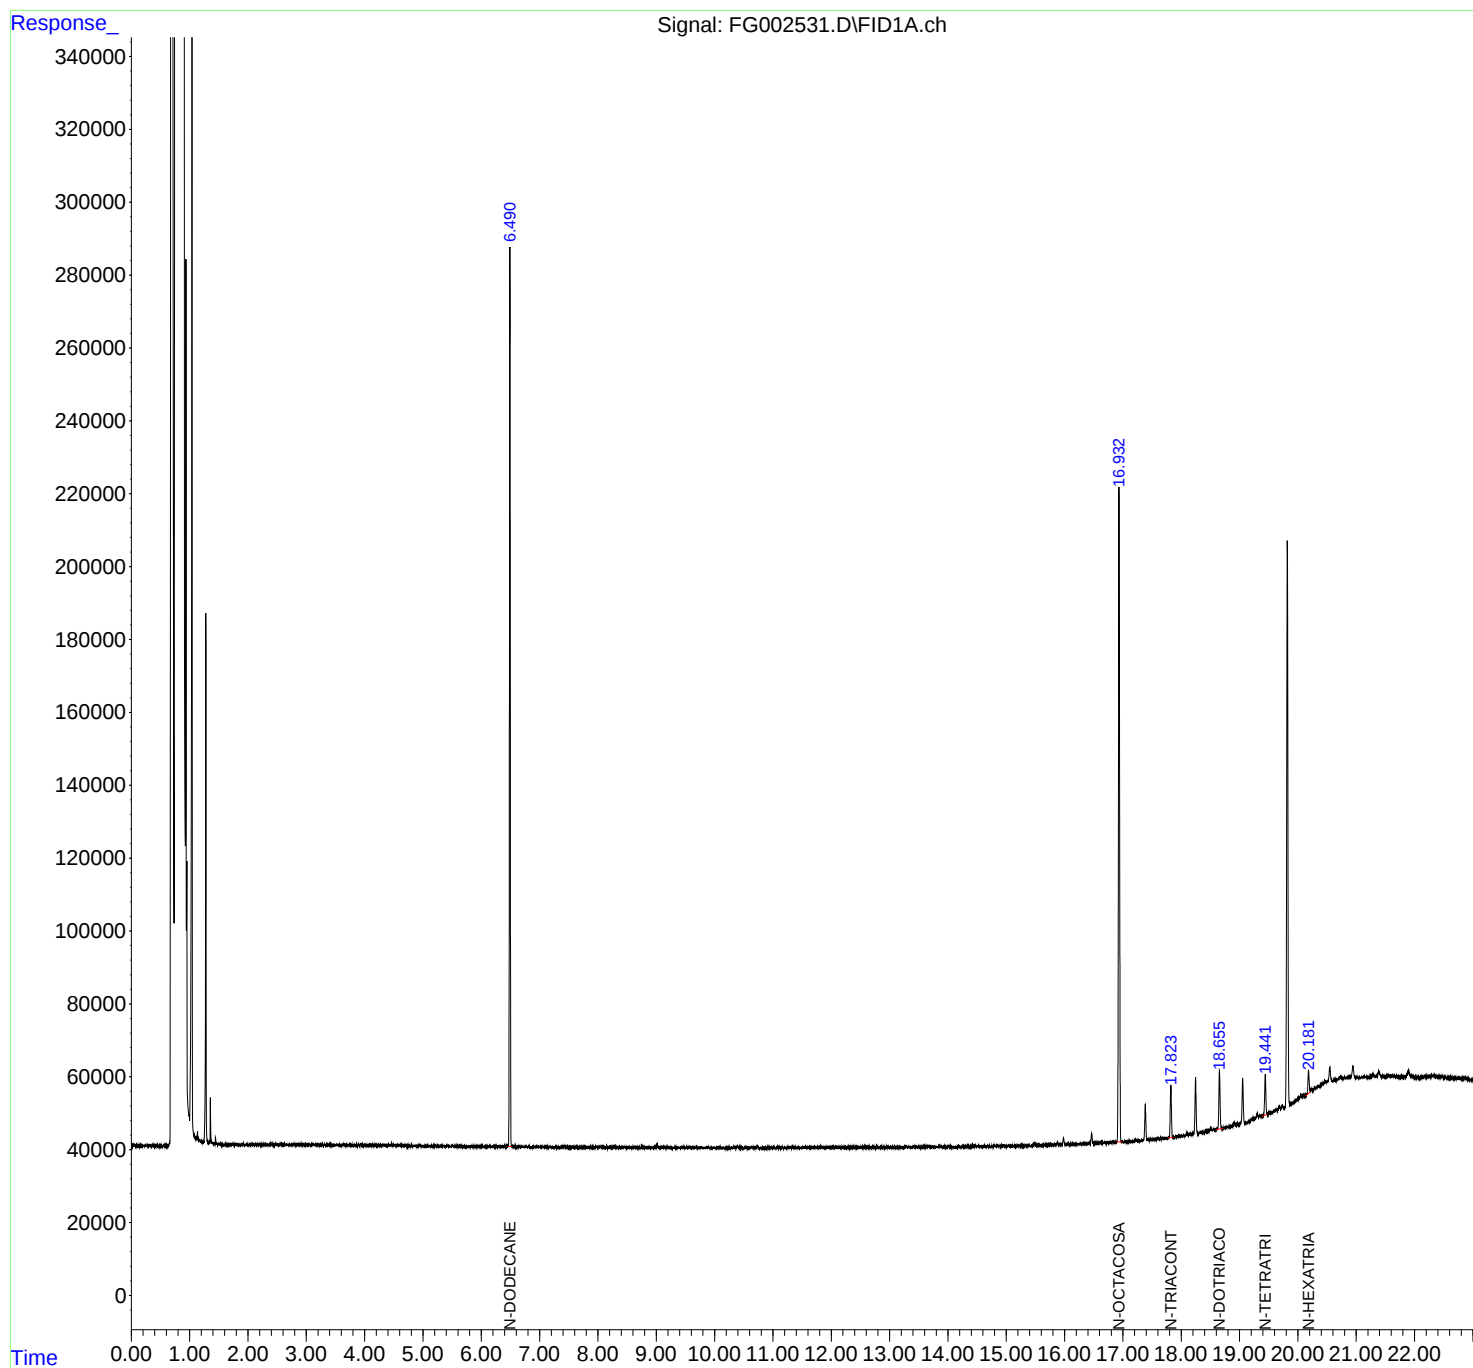

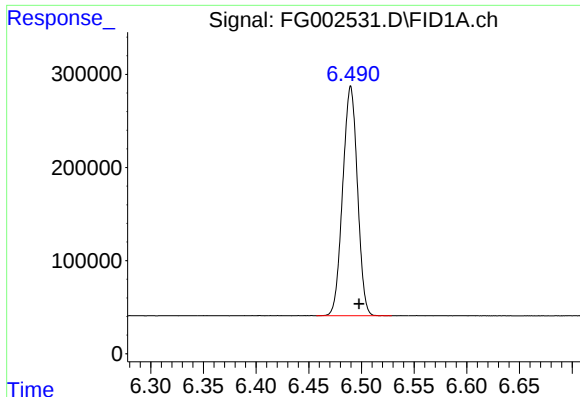


#3 N-DODECANE

R.T.: 6.490 min
Delta R.T.: -0.008 min
Response: 2398803
Conc: 18.18 ug/ml

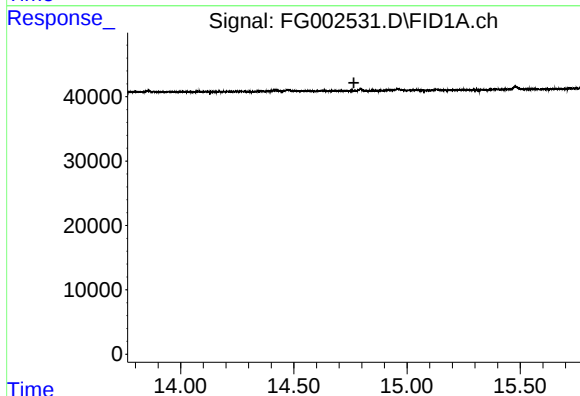


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.765 min
Response: 0
Conc: N.D.

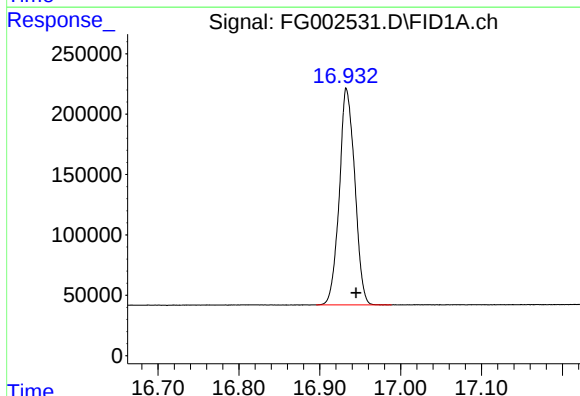


#12 N-OCTACOSANE

R.T.: 16.933 min
Delta R.T.: -0.012 min
Response: 2378110
Conc: 18.76 ug/ml

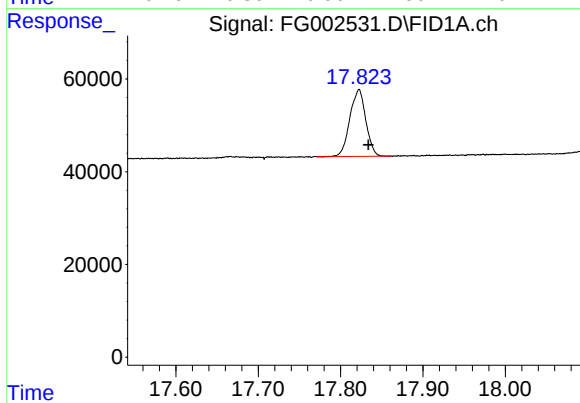


#13 N-TRIACONTANE

R.T.: 17.822 min
Delta R.T.: -0.011 min
Response: 194387
Conc: 1.54 ug/ml

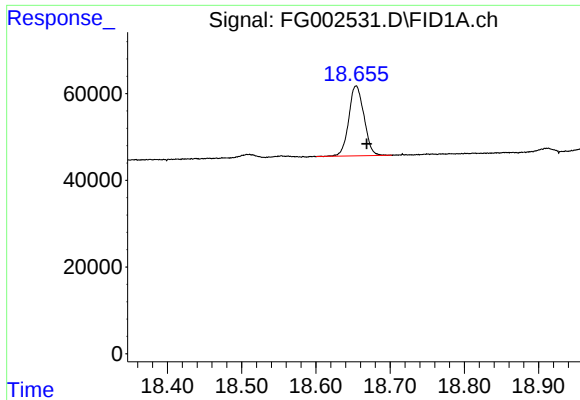


#14 N-DOTRIACONTANE

R.T.: 18.654 min
Delta R.T.: -0.014 min
Response: 228570
Conc: 1.86 ug/ml

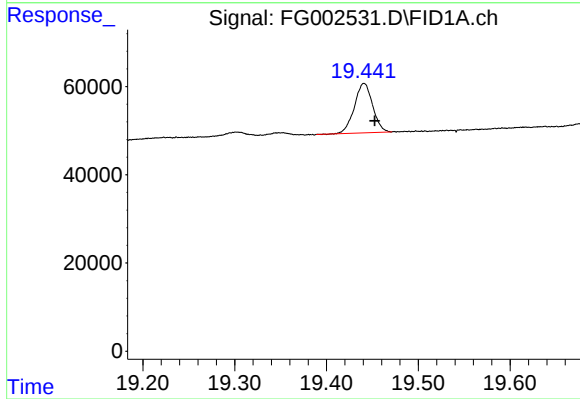

#15 N-TETRATRIACONTANE

R.T.: 19.441 min
Delta R.T.: -0.012 min
Response: 154571
Conc: 1.30 ug/ml

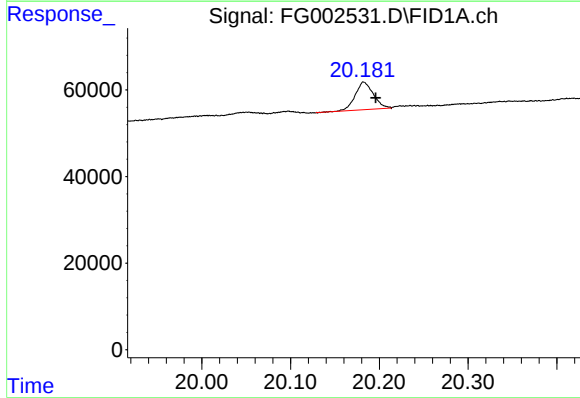

#16 N-HEXATRIACONTANE

R.T.: 20.183 min
Delta R.T.: -0.013 min
Response: 90219
Conc: 0.81 ug/ml