

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG100622\
Data File : FG010794.D
Signal(s) : FID1A.ch
Acq On : 06 Oct 2022 10:53
Operator : YP\AJ
Sample : RT MARKER
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
RT MARKER

Integration File: autoint1.e
Quant Time: Oct 07 05:36:23 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG092822.M
Quant Title :
QLast Update : Thu Sep 29 02:21:49 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
3)	N-DODECANE	6.445	1858127	14.011 ug/ml
12)	N-OCTACOSANE	16.917	1974580	15.058 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG100622\
Data File : FG010794.D
Signal(s) : FID1A.ch
Acq On : 06 Oct 2022 10:53
Operator : YP\AJ
Sample : RT MARKER
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
RT MARKER

Integration File: autoint1.e
Quant Time: Oct 07 05:36:23 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG092822.M
Quant Title :
QLast Update : Thu Sep 29 02:21:49 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

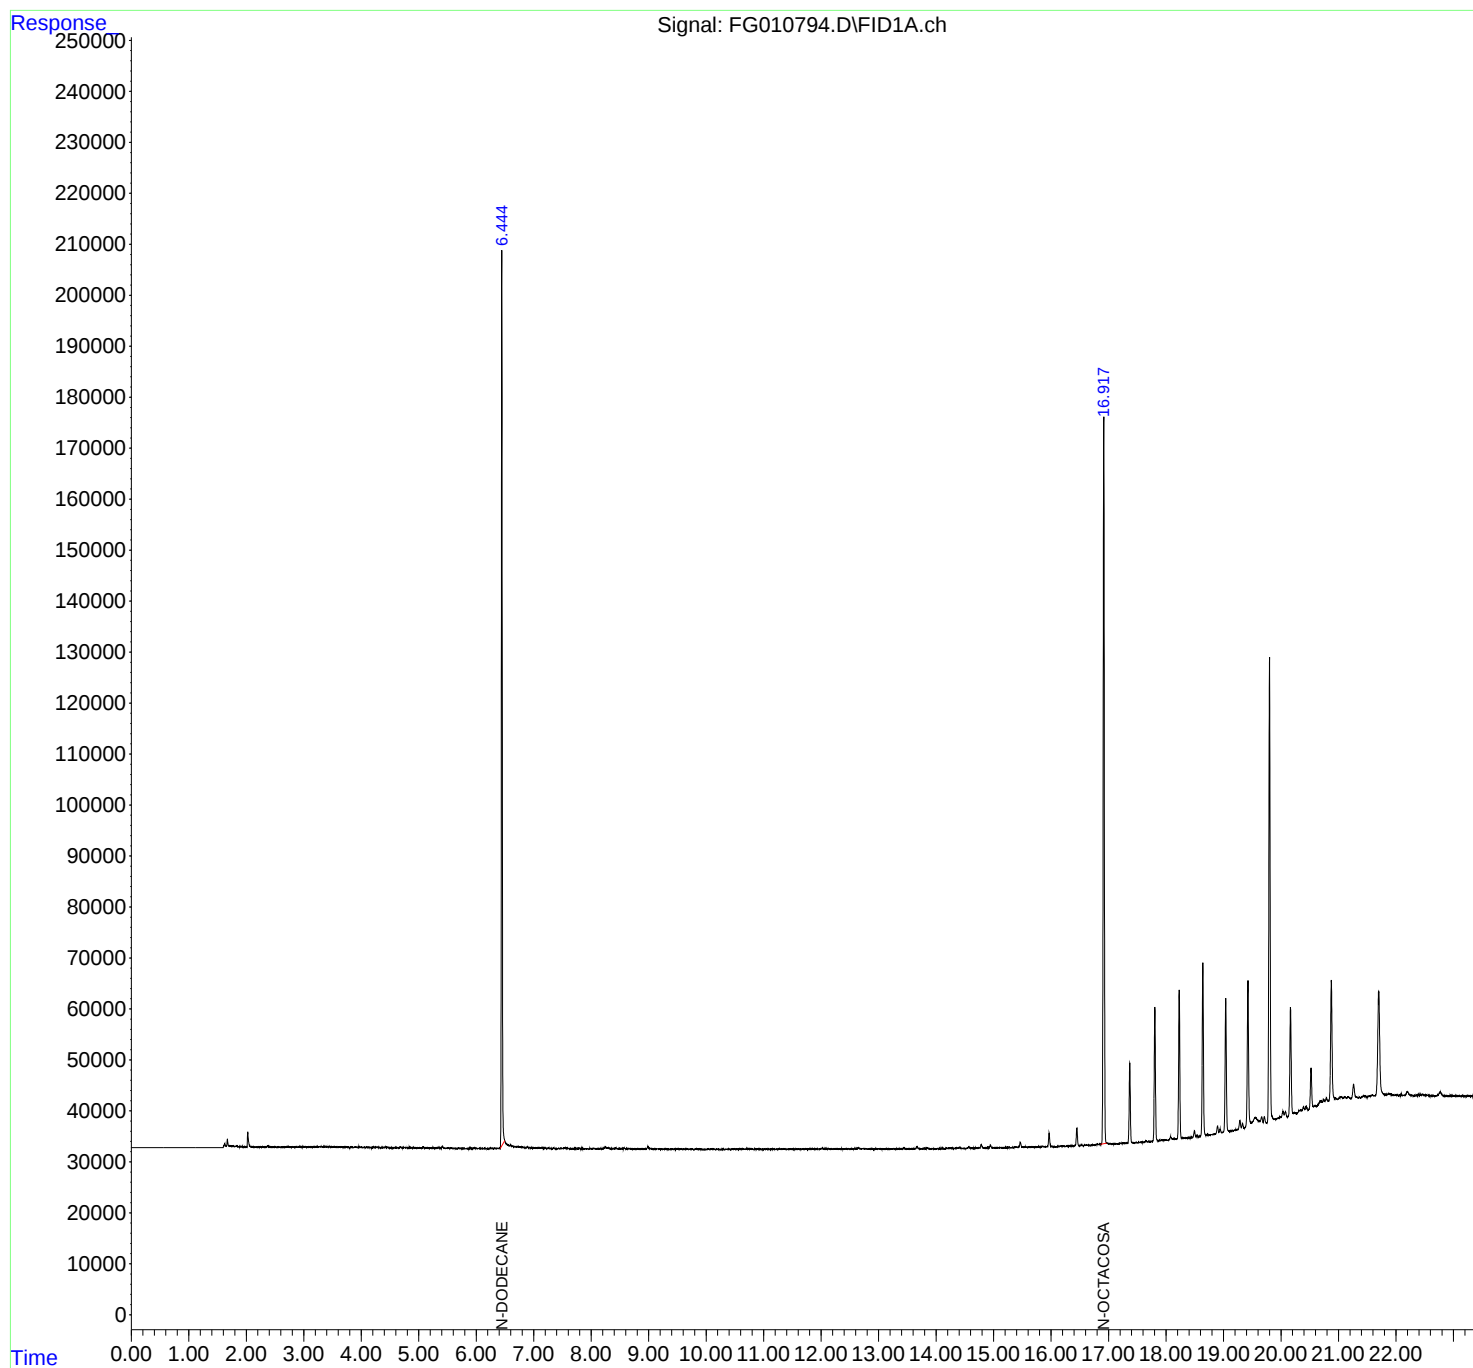


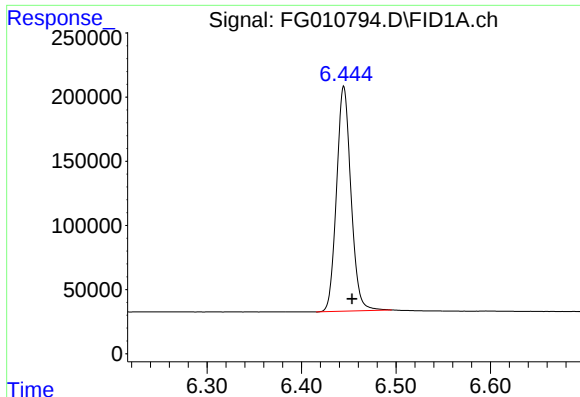

#3 N-DODECANE


R.T.: 6.445 min
Delta R.T.: -0.009 min
Response: 1858127
Conc: 14.01 ug/ml

Instrument :
FID_G
ClientSampleId :
RT MARKER

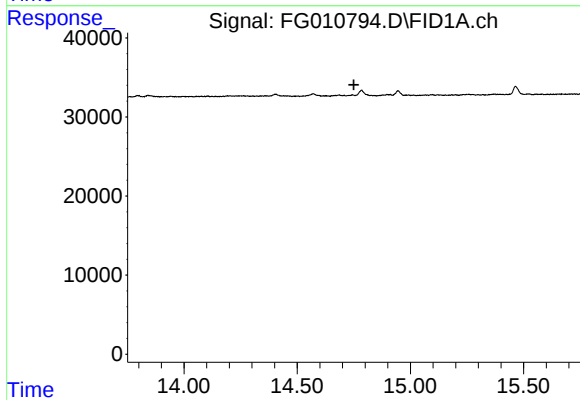

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.751 min
Response: 0
Conc: N.D.

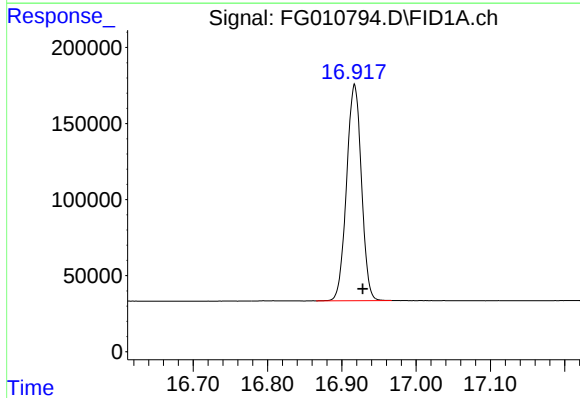

#12 N-OCTACOSANE

R.T.: 16.917 min
Delta R.T.: -0.011 min
Response: 1974580
Conc: 15.06 ug/ml